

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016580.D
 Acq On : 06 Jun 2020 11:19
 Operator : SY/MD
 Sample : L2895-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETW41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	192161	193178	12.55%	1.715%
2	1.560	139	146	159	rVB	128649	158756	10.31%	1.409%
3	2.116	310	319	338	rVB	303092	443319	28.80%	3.935%
4	2.572	454	461	462	rBV6	1155	1487	0.10%	0.013%
5	2.781	521	526	531	rVB8	2494	2580	0.17%	0.023%
6	2.852	545	548	549	rBV3	1588	881	0.06%	0.008%
7	3.126	631	633	636	rVB3	1377	683	0.04%	0.006%
8	3.145	636	639	641	rBV3	956	648	0.04%	0.006%
9	3.212	658	660	662	rBV3	1070	517	0.03%	0.005%
10	3.228	663	665	669	rVV4	1493	1074	0.07%	0.010%
11	3.264	673	676	682	rBV7	1227	988	0.06%	0.009%
12	3.299	686	687	689	rBV2	894	471	0.03%	0.004%
13	3.341	696	700	703	rBV5	1404	1007	0.07%	0.009%
14	3.450	732	734	739	rVB5	1268	968	0.06%	0.009%
15	3.473	739	741	743	rBV3	1024	529	0.03%	0.005%
16	3.498	745	749	751	rBV3	1224	844	0.05%	0.007%
17	3.579	772	774	776	rVV2	1367	591	0.04%	0.005%
18	3.598	778	780	783	rVV3	1050	623	0.04%	0.006%
19	3.614	783	785	788	rVB4	1082	560	0.04%	0.005%
20	3.740	816	824	827	rBV9	1057	1277	0.08%	0.011%
21	3.891	857	871	904	rBV	120751	330064	21.44%	2.930%
22	4.280	990	992	994	rBV3	1080	587	0.04%	0.005%
23	4.370	1003	1020	1044	rBV	249811	640769	41.63%	5.688%
24	4.785	1145	1149	1151	rBV4	1317	1159	0.08%	0.010%
25	4.846	1165	1168	1174	rVB9	1938	1689	0.11%	0.015%
26	4.875	1174	1177	1178	rBV3	1754	934	0.06%	0.008%
27	4.971	1204	1207	1212	rVB6	1548	959	0.06%	0.009%
28	5.068	1220	1237	1263	rVV2	603482	1539217	100.00%	13.662%
29	5.331	1315	1319	1320	rBV4	1580	1244	0.08%	0.011%
30	5.421	1344	1347	1348	rBV3	1270	694	0.05%	0.006%
31	5.559	1388	1390	1393	rBV4	1053	678	0.04%	0.006%
32	5.637	1401	1414	1435	rBV	390893	778136	50.55%	6.907%
33	5.994	1523	1525	1526	rBV3	1423	648	0.04%	0.006%
34	6.090	1543	1555	1577	rBV	349502	693792	45.07%	6.158%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016580.D
 Acq On : 06 Jun 2020 11:19
 Operator : SY/MD
 Sample : L2895-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETW41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.434	1660	1662	1665	rVB3	1456	808	0.05%	0.007%
36	6.524	1688	1690	1693	rVB2	1156	529	0.03%	0.005%
37	6.543	1693	1696	1700	rBV5	1813	1268	0.08%	0.011%
38	6.707	1744	1747	1754	rBV8	1501	2370	0.15%	0.021%
39	6.836	1785	1787	1790	rVV4	1125	736	0.05%	0.007%
40	6.932	1814	1817	1820	rVB3	1282	699	0.05%	0.006%
41	7.006	1828	1840	1863	rBV	199226	368273	23.93%	3.269%
42	7.270	1920	1922	1926	rBB3	1100	606	0.04%	0.005%
43	7.334	1930	1942	1960	rBV	714002	1232305	80.06%	10.938%
44	7.640	2027	2037	2059	rBV	145231	243815	15.84%	2.164%
45	7.887	2112	2114	2116	rBV2	1542	932	0.06%	0.008%
46	7.920	2122	2124	2128	rVB4	1376	745	0.05%	0.007%
47	7.942	2128	2131	2132	rBV3	1883	927	0.06%	0.008%
48	8.106	2172	2182	2216	rBV	441327	766603	49.80%	6.805%
49	8.350	2256	2258	2260	rBV3	1585	1014	0.07%	0.009%
50	8.537	2313	2316	2318	rBV3	1105	563	0.04%	0.005%
51	8.575	2325	2328	2330	rBV3	1124	858	0.06%	0.008%
52	8.608	2336	2338	2341	rBV4	1077	495	0.03%	0.004%
53	8.714	2368	2371	2374	rBV4	997	646	0.04%	0.006%
54	8.759	2383	2385	2386	rBV	1373	531	0.03%	0.005%
55	8.772	2386	2389	2394	rVB5	1335	1342	0.09%	0.012%
56	8.871	2408	2420	2440	rVV	586011	948079	61.59%	8.415%
57	9.228	2529	2531	2532	rBV	1171	516	0.03%	0.005%
58	9.270	2542	2544	2550	rBV6	1097	863	0.06%	0.008%
59	9.373	2572	2576	2580	rBV6	1038	1142	0.07%	0.010%
60	9.540	2623	2628	2629	rBV5	720	614	0.04%	0.005%
61	9.669	2666	2668	2673	rBV5	1122	826	0.05%	0.007%
62	9.707	2678	2680	2682	rBV3	1511	710	0.05%	0.006%
63	9.887	2734	2736	2738	rBV3	947	483	0.03%	0.004%
64	9.945	2750	2754	2756	rBV5	1747	1246	0.08%	0.011%
65	10.035	2780	2782	2785	rBV4	686	479	0.03%	0.004%
66	10.090	2797	2799	2801	rBV3	1233	750	0.05%	0.007%
67	10.238	2829	2845	2863	rBV	464121	738910	48.01%	6.559%
68	10.382	2886	2890	2893	rBV6	2104	1926	0.13%	0.017%
69	10.604	2956	2959	2961	rBV4	1927	1235	0.08%	0.011%
70	10.678	2979	2982	2983	rBV3	1260	634	0.04%	0.006%
71	10.772	3009	3011	3016	rBV4	916	757	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016580.D
 Acq On : 06 Jun 2020 11:19
 Operator : SY/MD
 Sample : L2895-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETW41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.881	3042	3045	3048	rBV5	1501	980	0.06%	0.009%
73	10.929	3055	3060	3062	rBV5	2050	2156	0.14%	0.019%
74	11.186	3137	3140	3141	rBV3	1219	559	0.04%	0.005%
75	11.270	3155	3166	3182	rBV	601555	919893	59.76%	8.165%
76	11.646	3272	3283	3303	rVB	761922	1184087	76.93%	10.510%
77	11.845	3343	3345	3347	rBV3	1459	798	0.05%	0.007%
78	11.993	3390	3391	3394	rBV3	793	459	0.03%	0.004%
79	12.116	3427	3429	3432	rBV3	1335	1004	0.07%	0.009%
80	12.135	3432	3435	3439	rVB3	1489	1173	0.08%	0.010%
81	12.415	3520	3522	3525	rVB4	1406	664	0.04%	0.006%
82	12.488	3543	3545	3550	rBV4	896	593	0.04%	0.005%
83	12.794	3637	3640	3643	rBV3	1147	805	0.05%	0.007%
84	12.868	3661	3663	3666	rBV4	1012	503	0.03%	0.004%
85	12.887	3666	3669	3672	rBV3	795	692	0.04%	0.006%
86	13.032	3712	3714	3716	rBV3	878	511	0.03%	0.005%
87	13.112	3737	3739	3742	rBV4	1429	653	0.04%	0.006%
88	13.222	3772	3773	3775	rBV2	1207	624	0.04%	0.006%
89	13.286	3788	3793	3804	rVB10	4459	6714	0.44%	0.060%
90	13.382	3820	3823	3825	rBV3	1211	708	0.05%	0.006%
91	13.575	3880	3883	3886	rVB4	1679	980	0.06%	0.009%
92	13.598	3886	3890	3891	rBV2	1237	676	0.04%	0.006%
93	13.649	3904	3906	3908	rBV3	989	511	0.03%	0.005%
94	13.768	3937	3943	3952	rVV9	4608	7843	0.51%	0.070%
95	13.820	3956	3959	3961	rBV2	1709	1082	0.07%	0.010%
96	13.919	3988	3990	3992	rVB3	1143	482	0.03%	0.004%
97	14.019	4019	4021	4024	rBV3	1657	996	0.06%	0.009%
98	14.058	4031	4033	4034	rBV	1001	494	0.03%	0.004%
99	14.103	4043	4047	4051	rBV7	1630	1609	0.10%	0.014%
100	14.222	4082	4084	4087	rBV3	1890	981	0.06%	0.009%


Sum of corrected areas: 11266016

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016580.D
Acq On : 06 Jun 2020 11:19
Operator : SY/MD
Sample : L2895-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETW41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

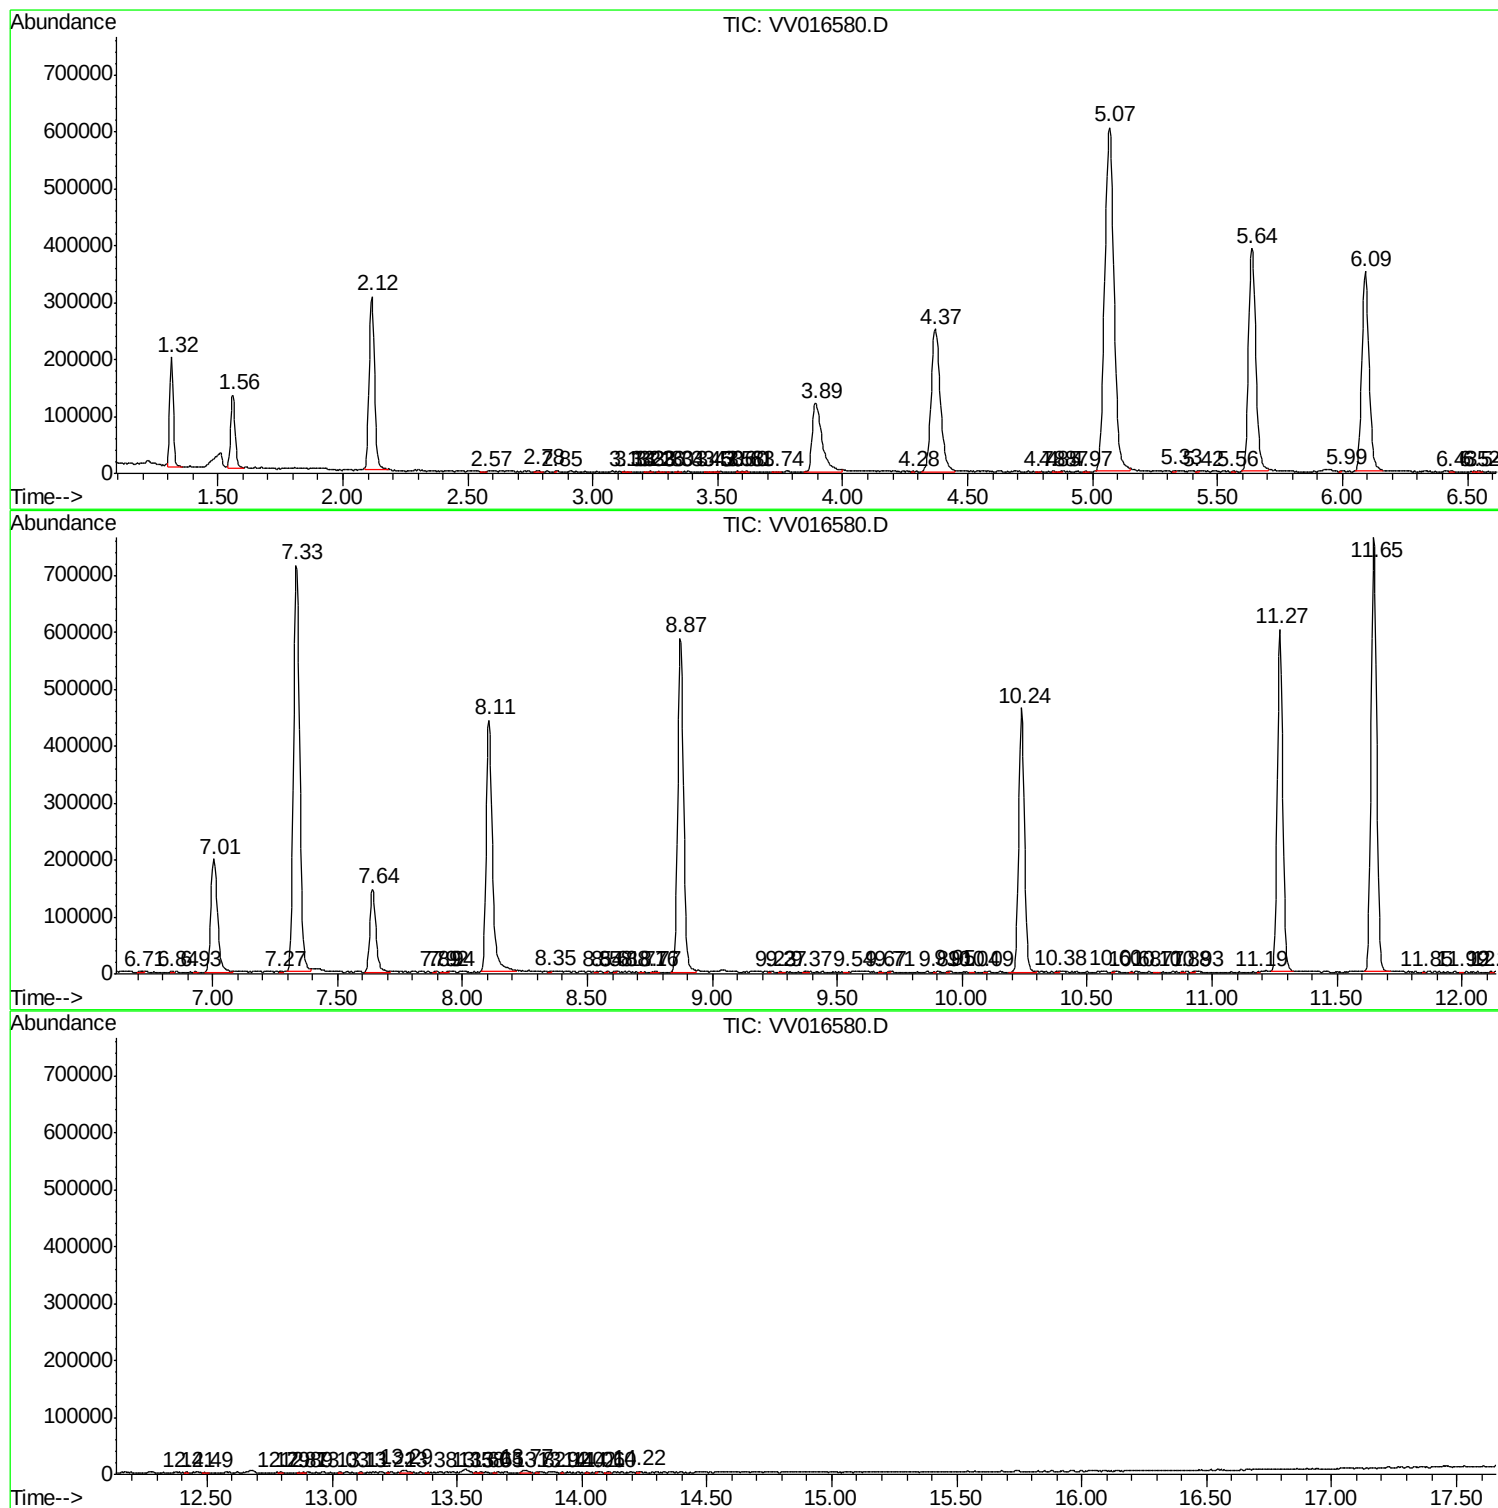

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016580.D
Acq On : 06 Jun 2020 11:19
Operator : SY/MD
Sample : L2895-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETW41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016580.D
Acq On : 06 Jun 2020 11:19
Operator : SY/MD
Sample : L2895-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETW41

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc