

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016582.D
 Acq On : 06 Jun 2020 12:06
 Operator : SY/MD
 Sample : L2872-09 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	222923	225597	1.00%	0.643%
2	1.560	139	146	159	rVB	146167	178808	0.79%	0.509%
3	2.116	310	319	335	rVB	338306	492302	2.19%	1.403%
4	2.383	400	402	405	rBV3	1183	585	0.00%	0.002%
5	2.830	539	541	543	rVB3	1222	560	0.00%	0.002%
6	2.881	552	557	560	rBV6	1836	1956	0.01%	0.006%
7	2.978	584	587	588	rBV2	1034	682	0.00%	0.002%
8	3.090	618	622	623	rBV3	1231	932	0.00%	0.003%
9	3.135	630	636	639	rBV7	2238	2179	0.01%	0.006%
10	3.277	675	680	684	rBV7	1545	1490	0.01%	0.004%
11	3.302	684	688	690	rBV4	1108	603	0.00%	0.002%
12	3.460	733	737	744	rBV8	2352	2115	0.01%	0.006%
13	3.492	744	747	748	rBV2	811	495	0.00%	0.001%
14	3.531	753	759	763	rBV8	1480	1848	0.01%	0.005%
15	3.656	793	798	799	rBV4	1401	1187	0.01%	0.003%
16	3.759	825	830	836	rBV8	1682	2195	0.01%	0.006%
17	3.849	854	858	859	rBV4	705	484	0.00%	0.001%
18	3.894	862	872	899	rVV	129983	339321	1.51%	0.967%
19	4.302	997	999	1002	rBV4	1126	756	0.00%	0.002%
20	4.373	1006	1021	1046	rVB	266300	647445	2.88%	1.845%
21	4.611	1093	1095	1099	rBV2	1070	645	0.00%	0.002%
22	4.685	1115	1118	1119	rBV3	1241	571	0.00%	0.002%
23	4.923	1190	1192	1194	rBV3	823	375	0.00%	0.001%
24	4.984	1209	1211	1213	rBV3	971	408	0.00%	0.001%
25	5.071	1219	1238	1270	rBV2	651979	1684226	7.49%	4.799%
26	5.335	1318	1320	1321	rBV2	1432	628	0.00%	0.002%
27	5.540	1382	1384	1386	rBV2	1455	764	0.00%	0.002%
28	5.640	1402	1415	1439	rBV	482338	955457	4.25%	2.722%
29	5.929	1499	1505	1511	rBV7	5312	9227	0.04%	0.026%
30	6.093	1543	1556	1579	rBV	378348	749766	3.33%	2.136%
31	6.351	1634	1636	1638	rVB3	1407	576	0.00%	0.002%
32	6.389	1644	1648	1649	rBV3	1387	778	0.00%	0.002%
33	6.820	1778	1782	1785	rVB5	1736	1143	0.01%	0.003%
34	6.833	1785	1786	1789	rBV3	1125	526	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016582.D
 Acq On : 06 Jun 2020 12:06
 Operator : SY/MD
 Sample : L2872-09 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.855	1789	1793	1795	rVV4	1429	991	0.00%	0.003%
36	6.878	1798	1800	1803	rVV4	1193	556	0.00%	0.002%
37	6.904	1806	1808	1813	rVB4	855	750	0.00%	0.002%
38	6.933	1813	1817	1820	rBV4	884	764	0.00%	0.002%
39	7.007	1830	1840	1868	rVB	215663	379757	1.69%	1.082%
40	7.293	1926	1929	1931	rBV4	1297	886	0.00%	0.003%
41	7.338	1931	1943	1962	rVV	795085	1344657	5.98%	3.831%
42	7.640	2027	2037	2058	rBV	154237	260397	1.16%	0.742%
43	8.000	2133	2149	2171	rBV	13355821	22498855	100.00%	64.107%
44	8.106	2173	2182	2212	rVB	486601	841477	3.74%	2.398%
45	8.875	2409	2421	2443	rBV	716634	1161860	5.16%	3.311%
46	9.116	2494	2496	2500	rBV5	1475	1209	0.01%	0.003%
47	9.145	2504	2505	2507	rBV2	1194	612	0.00%	0.002%
48	9.232	2530	2532	2537	rVB4	1367	724	0.00%	0.002%
49	9.264	2537	2542	2543	rBV4	1380	1283	0.01%	0.004%
50	9.312	2555	2557	2561	rBV3	805	621	0.00%	0.002%
51	9.360	2568	2572	2573	rBV4	1073	621	0.00%	0.002%
52	9.524	2618	2623	2624	rBV4	1529	919	0.00%	0.003%
53	9.759	2693	2696	2701	rBV5	1656	1630	0.01%	0.005%
54	9.884	2732	2735	2736	rBV3	714	401	0.00%	0.001%
55	9.913	2742	2744	2746	rBV3	847	534	0.00%	0.002%
56	9.942	2751	2753	2755	rBV4	932	492	0.00%	0.001%
57	10.125	2808	2810	2813	rVB3	1109	565	0.00%	0.002%
58	10.145	2814	2816	2819	rVV2	1598	808	0.00%	0.002%
59	10.167	2821	2823	2826	rVB3	2079	855	0.00%	0.002%
60	10.180	2826	2827	2830	rBV2	685	378	0.00%	0.001%
61	10.238	2833	2845	2862	rBV	505842	788132	3.50%	2.246%
62	10.408	2896	2898	2901	rVB3	989	464	0.00%	0.001%
63	10.473	2914	2918	2920	rBV5	1425	1078	0.00%	0.003%
64	10.640	2967	2970	2972	rBV4	1125	712	0.00%	0.002%
65	10.707	2989	2991	2992	rBV2	844	419	0.00%	0.001%
66	10.723	2992	2996	2999	rVV4	2043	1835	0.01%	0.005%
67	10.743	2999	3002	3007	rVB5	1512	1544	0.01%	0.004%
68	10.807	3017	3022	3024	rBV4	2170	1785	0.01%	0.005%
69	10.875	3036	3043	3045	rBV7	1644	1856	0.01%	0.005%
70	10.987	3076	3078	3084	rBV5	842	667	0.00%	0.002%
71	11.045	3092	3096	3097	rBV3	1389	973	0.00%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016582.D
 Acq On : 06 Jun 2020 12:06
 Operator : SY/MD
 Sample : L2872-09 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.148	3126	3128	3130	rBV3	1048	640	0.00%	0.002%
73	11.196	3136	3143	3145	rBV4	2085	2089	0.01%	0.006%
74	11.270	3155	3166	3185	rBV	751535	1152307	5.12%	3.283%
75	11.469	3225	3228	3229	rBV3	1314	616	0.00%	0.002%
76	11.518	3241	3243	3244	rBV2	1031	453	0.00%	0.001%
77	11.530	3244	3247	3249	rVV4	1265	897	0.00%	0.003%
78	11.588	3262	3265	3268	rBV4	1331	849	0.00%	0.002%
79	11.646	3270	3283	3302	rBV	832990	1308047	5.81%	3.727%
80	11.891	3357	3359	3360	rBV2	1021	420	0.00%	0.001%
81	11.926	3365	3370	3371	rBV5	1352	1256	0.01%	0.004%
82	12.045	3405	3407	3410	rVB	798	500	0.00%	0.001%
83	12.067	3410	3414	3419	rBV7	1918	2227	0.01%	0.006%
84	12.180	3445	3449	3453	rBV5	686	614	0.00%	0.002%
85	12.206	3453	3457	3459	rBV4	1507	928	0.00%	0.003%
86	12.392	3513	3515	3518	rBV3	1119	720	0.00%	0.002%
87	12.633	3585	3590	3591	rBV5	990	858	0.00%	0.002%
88	12.698	3608	3610	3613	rBV3	965	505	0.00%	0.001%
89	12.942	3684	3686	3691	rVB6	886	516	0.00%	0.001%
90	13.019	3708	3710	3712	rVB3	1193	449	0.00%	0.001%
91	13.048	3717	3719	3721	rBV3	1283	642	0.00%	0.002%
92	13.218	3769	3772	3774	rVB4	1824	1053	0.00%	0.003%
93	13.247	3778	3781	3785	rBV3	910	557	0.00%	0.002%
94	13.289	3785	3794	3795	rBV8	2930	3823	0.02%	0.011%
95	13.382	3821	3823	3826	rBV2	1506	834	0.00%	0.002%
96	13.865	3968	3973	3974	rBV3	1571	1081	0.00%	0.003%
97	14.138	4055	4058	4060	rBV4	1133	771	0.00%	0.002%
98	14.360	4124	4127	4131	rBV4	1187	935	0.00%	0.003%
99	14.691	4228	4230	4235	rBV4	1541	1337	0.01%	0.004%
100	14.980	4317	4320	4323	rBV4	1371	1058	0.00%	0.003%


Sum of corrected areas: 35095679

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016582.D
Acq On : 06 Jun 2020 12:06
Operator : SY/MD
Sample : L2872-09 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

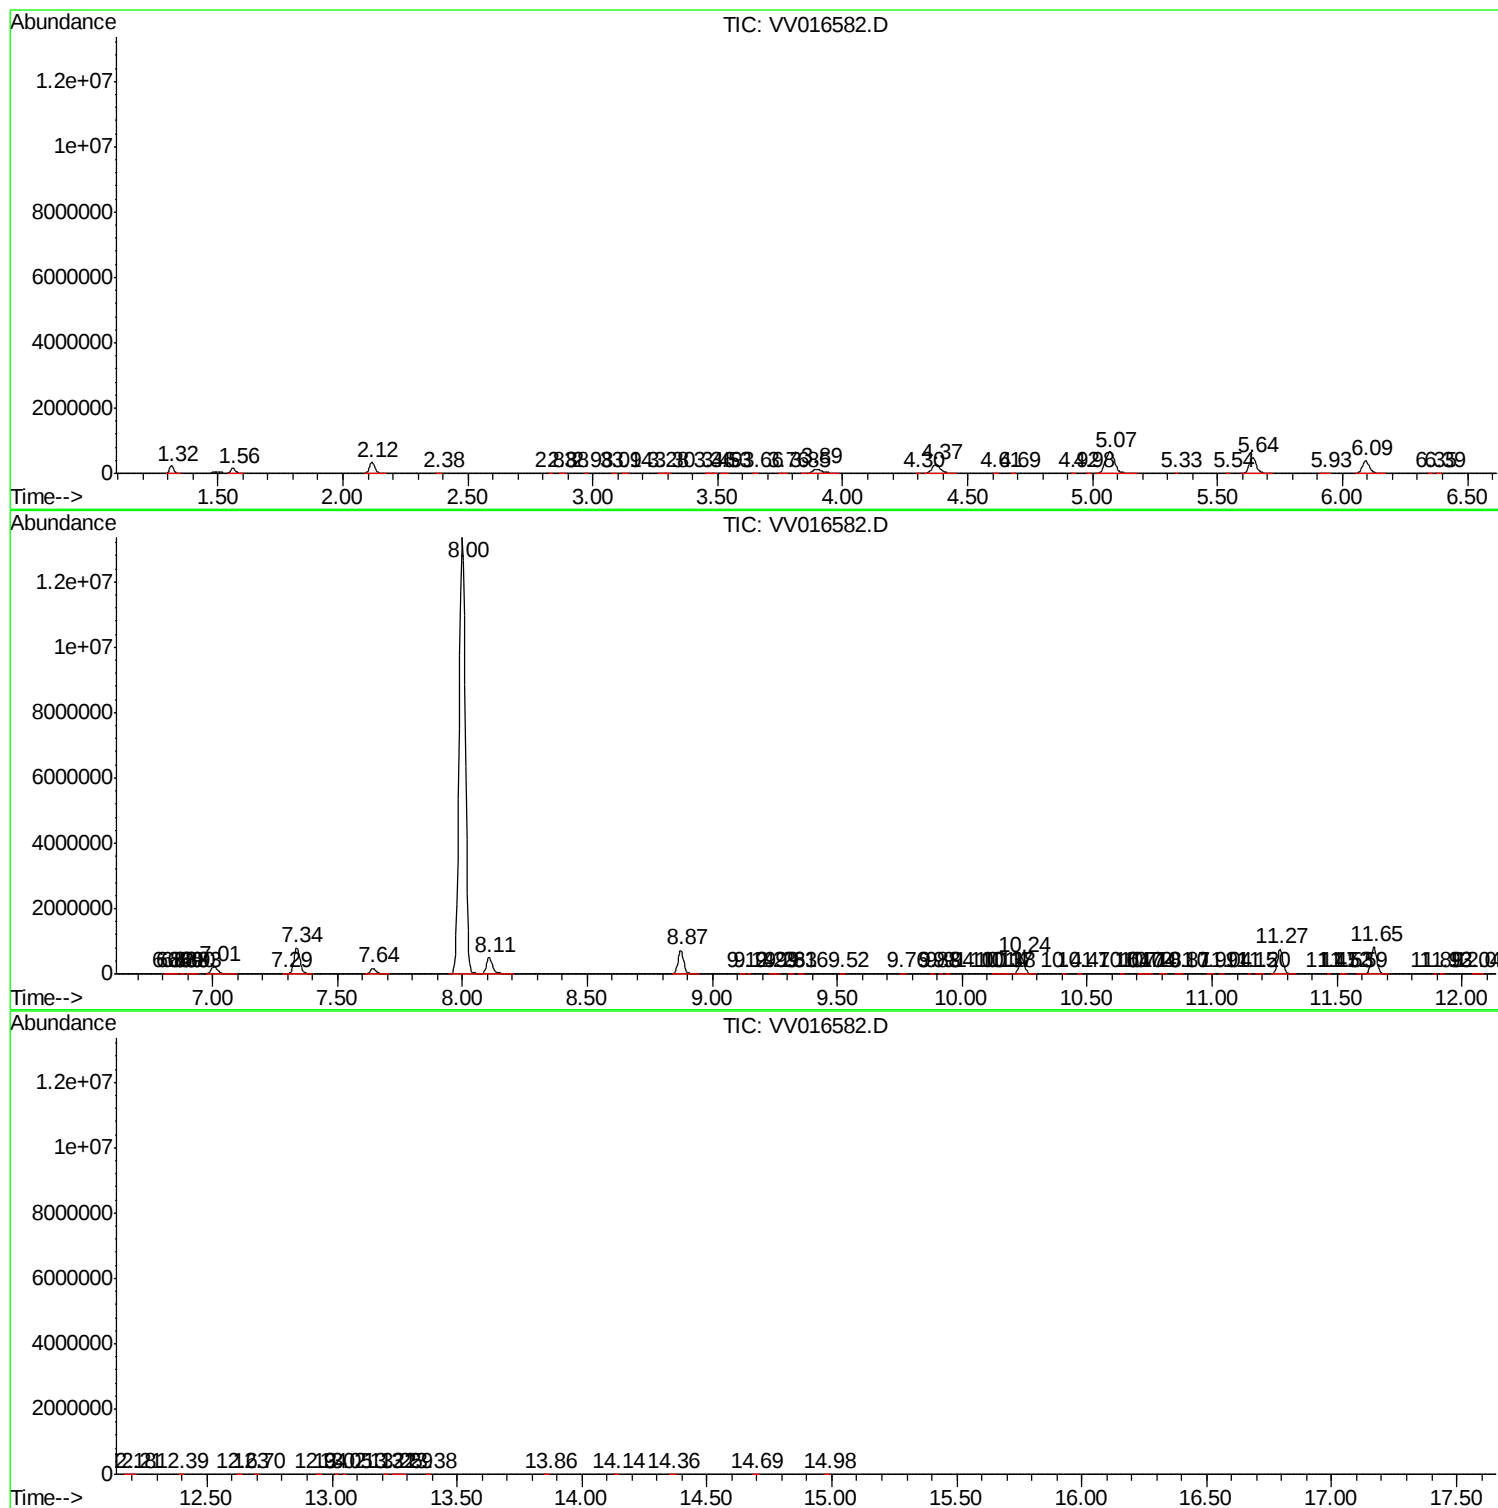

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016582.D
Acq On : 06 Jun 2020 12:06
Operator : SY/MD
Sample : L2872-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016582.D
Acq On : 06 Jun 2020 12:06
Operator : SY/MD
Sample : L2872-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc