

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016583.D
 Acq On : 06 Jun 2020 12:30
 Operator : SY/MD
 Sample : L2895-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0G8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	184256	188900	13.08%	1.818%
2	1.560	139	146	160	rVB	122510	146654	10.15%	1.412%
3	2.116	310	319	336	rVB	274324	405906	28.10%	3.907%
4	2.457	423	425	428	rBV4	1630	1161	0.08%	0.011%
5	2.827	538	540	544	rBV4	1093	557	0.04%	0.005%
6	2.878	552	556	559	rBV4	1334	1267	0.09%	0.012%
7	2.926	569	571	574	rVB3	1337	525	0.04%	0.005%
8	3.415	719	723	725	rVB5	1584	934	0.06%	0.009%
9	3.434	726	729	733	rBV4	809	523	0.04%	0.005%
10	3.454	733	735	738	rBV3	1472	746	0.05%	0.007%
11	3.634	789	791	793	rBV2	1022	521	0.04%	0.005%
12	3.647	793	795	797	rVB3	1364	579	0.04%	0.006%
13	3.669	797	802	804	rBV4	1136	728	0.05%	0.007%
14	3.711	811	815	816	rBV4	1066	628	0.04%	0.006%
15	3.843	854	856	860	rVB4	1245	807	0.06%	0.008%
16	3.897	861	873	876	rBV	125455	216433	14.98%	2.083%
17	4.196	963	966	968	rBV3	1610	1244	0.09%	0.012%
18	4.373	1007	1021	1044	rVB	227250	546759	37.85%	5.263%
19	4.557	1074	1078	1082	rBV7	1494	1043	0.07%	0.010%
20	4.592	1087	1089	1091	rBV2	1395	629	0.04%	0.006%
21	4.695	1119	1121	1124	rBV5	1087	730	0.05%	0.007%
22	4.811	1154	1157	1158	rBV2	1165	769	0.05%	0.007%
23	4.856	1167	1171	1174	rBV5	1269	935	0.06%	0.009%
24	4.894	1180	1183	1187	rVB5	996	908	0.06%	0.009%
25	4.952	1199	1201	1206	rVB4	1097	680	0.05%	0.007%
26	5.003	1215	1217	1219	rBV3	1198	673	0.05%	0.006%
27	5.071	1220	1238	1269	rVV2	557096	1444397	100.00%	13.904%
28	5.392	1335	1338	1340	rBV3	1434	847	0.06%	0.008%
29	5.640	1402	1415	1440	rBV	365873	727126	50.34%	6.999%
30	5.862	1478	1484	1486	rBV7	1947	2058	0.14%	0.020%
31	6.093	1542	1556	1583	rBV	322937	651244	45.09%	6.269%
32	6.219	1593	1595	1596	rBV2	1580	604	0.04%	0.006%
33	6.290	1614	1617	1619	rBV4	1248	1019	0.07%	0.010%
34	6.319	1624	1626	1629	rVV3	1136	559	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016583.D
 Acq On : 06 Jun 2020 12:30
 Operator : SY/MD
 Sample : L2895-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0G8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.531	1690	1692	1695	rBV4	1529	686	0.05%	0.007%
36	6.553	1697	1699	1703	rVV4	1083	599	0.04%	0.006%
37	6.855	1789	1793	1795	rBV4	1675	1268	0.09%	0.012%
38	6.872	1796	1798	1804	rVB6	1434	1374	0.10%	0.013%
39	6.913	1808	1811	1813	rBV2	1560	990	0.07%	0.010%
40	7.007	1828	1840	1857	rBV	183482	325727	22.55%	3.135%
41	7.228	1907	1909	1911	rBV2	1159	662	0.05%	0.006%
42	7.338	1931	1943	1962	rBV	649914	1121586	77.65%	10.796%
43	7.601	2023	2025	2027	rBV2	1039	659	0.05%	0.006%
44	7.640	2027	2037	2058	rVV	130075	223223	15.45%	2.149%
45	7.798	2082	2086	2091	rBV6	1271	1641	0.11%	0.016%
46	7.894	2113	2116	2119	rBV4	824	696	0.05%	0.007%
47	7.955	2131	2135	2137	rBV4	1595	1303	0.09%	0.013%
48	7.997	2137	2148	2163	rVB	58164	100661	6.97%	0.969%
49	8.106	2172	2182	2209	rBV	422776	729998	50.54%	7.027%
50	8.428	2280	2282	2285	rBV3	1736	1175	0.08%	0.011%
51	8.643	2346	2349	2351	rVB2	1109	544	0.04%	0.005%
52	8.707	2364	2369	2372	rBV7	1535	1406	0.10%	0.014%
53	8.781	2390	2392	2395	rBV3	1087	691	0.05%	0.007%
54	8.817	2400	2403	2406	rBV4	1984	1317	0.09%	0.013%
55	8.875	2410	2421	2443	rVV	548109	881582	61.03%	8.486%
56	9.608	2647	2649	2655	rBV7	1644	1447	0.10%	0.014%
57	9.666	2665	2667	2671	rVB3	1330	860	0.06%	0.008%
58	9.698	2671	2677	2680	rBV6	1042	820	0.06%	0.008%
59	9.743	2688	2691	2694	rVV4	880	578	0.04%	0.006%
60	9.826	2714	2717	2721	rBV4	1197	1121	0.08%	0.011%
61	9.913	2741	2744	2746	rBV3	1413	874	0.06%	0.008%
62	9.961	2754	2759	2764	rBV7	1677	1367	0.09%	0.013%
63	9.987	2764	2767	2769	rBV4	1101	728	0.05%	0.007%
64	10.029	2776	2780	2783	rBV5	1023	791	0.05%	0.008%
65	10.148	2814	2817	2820	rBV5	1224	842	0.06%	0.008%
66	10.238	2833	2845	2859	rBV	426389	678322	46.96%	6.530%
67	10.476	2913	2919	2923	rBV7	1549	1866	0.13%	0.018%
68	10.614	2958	2962	2964	rBV5	1556	1130	0.08%	0.011%
69	10.720	2991	2995	2996	rBV3	1510	996	0.07%	0.010%
70	10.839	3026	3032	3037	rBV8	2290	2871	0.20%	0.028%
71	10.862	3037	3039	3041	rBV3	1177	594	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016583.D
 Acq On : 06 Jun 2020 12:30
 Operator : SY/MD
 Sample : L2895-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0G8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.875	3041	3043	3046	rVV3	1188	626	0.04%	0.006%
73	11.122	3117	3120	3122	rBV3	1543	859	0.06%	0.008%
74	11.151	3124	3129	3132	rBV5	1560	1447	0.10%	0.014%
75	11.212	3145	3148	3150	rBV3	1615	1043	0.07%	0.010%
76	11.270	3155	3166	3186	rVV	536836	836352	57.90%	8.051%
77	11.463	3223	3226	3231	rBV6	1547	1421	0.10%	0.014%
78	11.556	3249	3255	3262	rBV6	7054	10140	0.70%	0.098%
79	11.646	3272	3283	3305	rVB	671060	1070650	74.12%	10.306%
80	11.952	3376	3378	3382	rBV3	1550	1326	0.09%	0.013%
81	12.090	3415	3421	3423	rBV7	1742	1920	0.13%	0.018%
82	12.125	3429	3432	3434	rBV4	1030	700	0.05%	0.007%
83	12.248	3466	3470	3475	rBV7	1853	1848	0.13%	0.018%
84	12.309	3484	3489	3490	rBV4	1032	971	0.07%	0.009%
85	12.344	3496	3500	3501	rBV4	1747	1207	0.08%	0.012%
86	12.749	3623	3626	3630	rBV6	994	834	0.06%	0.008%
87	12.900	3670	3673	3674	rBV2	1326	787	0.05%	0.008%
88	12.945	3684	3687	3689	rBV3	1116	560	0.04%	0.005%
89	13.058	3718	3722	3723	rBV4	939	680	0.05%	0.007%
90	13.122	3738	3742	3745	rBV5	1140	973	0.07%	0.009%
91	13.238	3773	3778	3780	rBV5	1353	1136	0.08%	0.011%
92	13.530	3865	3869	3872	rBV5	2325	2179	0.15%	0.021%
93	13.659	3906	3909	3911	rBV3	2065	1100	0.08%	0.011%
94	13.813	3955	3957	3959	rBV2	1148	562	0.04%	0.005%
95	13.984	4006	4010	4013	rBV5	1328	1408	0.10%	0.014%
96	14.064	4031	4035	4038	rBV4	1805	1393	0.10%	0.013%
97	14.154	4059	4063	4064	rBV3	1370	886	0.06%	0.009%
98	14.219	4079	4083	4085	rBV4	1681	1392	0.10%	0.013%
99	14.318	4110	4114	4116	rBV4	1437	1077	0.07%	0.010%
100	14.363	4124	4128	4129	rBV4	1244	901	0.06%	0.009%


Sum of corrected areas: 10388466

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016583.D
Acq On : 06 Jun 2020 12:30
Operator : SY/MD
Sample : L2895-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
EW0G8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

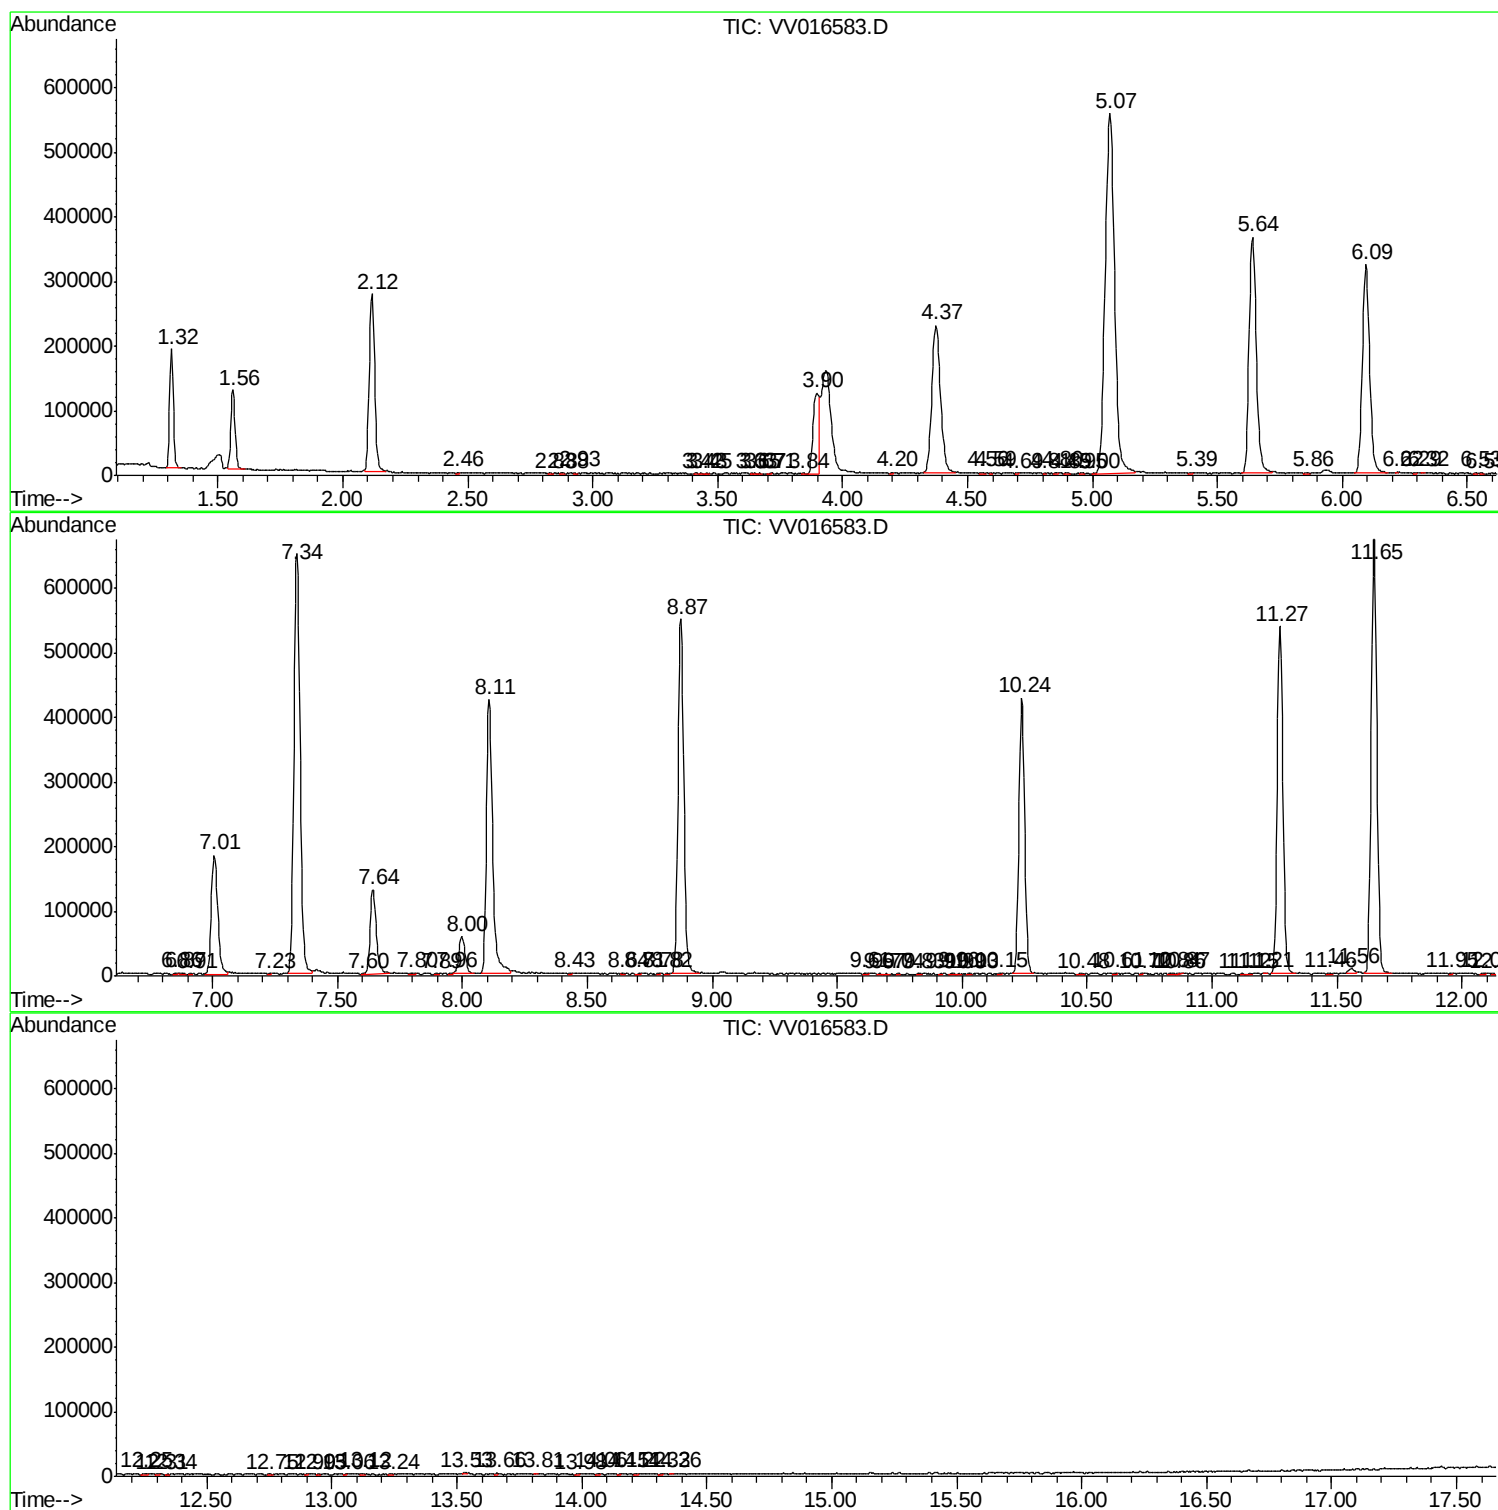

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016583.D
Acq On : 06 Jun 2020 12:30
Operator : SY/MD
Sample : L2895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0G8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016583.D
Acq On : 06 Jun 2020 12:30
Operator : SY/MD
Sample : L2895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0G8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc