

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016586.D
 Acq On : 06 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2895-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0J5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	86	rVB2	519769	551152	24.98%	4.363%
2	1.553	139	144	158	rVB	105375	131577	5.96%	1.042%
3	2.116	309	319	331	rBV	254518	376459	17.06%	2.980%
4	2.846	544	546	548	rBV3	1254	637	0.03%	0.005%
5	3.087	619	621	625	rVB5	1406	760	0.03%	0.006%
6	3.116	625	630	631	rBV4	1289	1170	0.05%	0.009%
7	3.145	635	639	641	rBV4	1386	1009	0.05%	0.008%
8	3.274	676	679	683	rVB5	1609	1077	0.05%	0.009%
9	3.293	683	685	687	rBV3	921	615	0.03%	0.005%
10	3.357	703	705	710	rVB4	1277	795	0.04%	0.006%
11	3.409	714	721	724	rBV7	1850	1993	0.09%	0.016%
12	3.470	737	740	742	rBV4	1570	925	0.04%	0.007%
13	3.547	759	764	767	rBV7	1310	1228	0.06%	0.010%
14	3.566	767	770	775	rVV7	1260	1211	0.05%	0.010%
15	3.608	780	783	787	rBV4	865	674	0.03%	0.005%
16	3.650	793	796	797	rBV3	1223	553	0.03%	0.004%
17	3.782	834	837	838	rBV2	1103	625	0.03%	0.005%
18	3.852	855	859	862	rBV5	1276	1118	0.05%	0.009%
19	3.933	862	884	916	rVV2	807732	2206232	100.00%	17.466%
20	4.373	1001	1021	1048	rBV	216273	542537	24.59%	4.295%
21	4.601	1089	1092	1094	rBV4	1473	915	0.04%	0.007%
22	4.643	1102	1105	1111	rVB7	1802	1957	0.09%	0.015%
23	4.682	1111	1117	1118	rBV4	2342	1770	0.08%	0.014%
24	4.907	1185	1187	1189	rBV3	1184	617	0.03%	0.005%
25	4.971	1205	1207	1209	rBV3	1382	849	0.04%	0.007%
26	5.068	1219	1237	1271	rBV2	532543	1366752	61.95%	10.820%
27	5.556	1385	1389	1391	rBV4	1306	909	0.04%	0.007%
28	5.640	1402	1415	1435	rBV	415282	826969	37.48%	6.547%
29	5.878	1488	1489	1492	rVB3	1611	719	0.03%	0.006%
30	5.897	1492	1495	1497	rBV2	1527	1073	0.05%	0.008%
31	6.093	1538	1556	1577	rBV	301309	621294	28.16%	4.918%
32	6.383	1644	1646	1648	rBV4	986	558	0.03%	0.004%
33	6.421	1654	1658	1659	rBV3	1129	903	0.04%	0.007%
34	6.547	1694	1697	1699	rBV4	1715	998	0.05%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016586.D
 Acq On : 06 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2895-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0J5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.772	1763	1767	1769	rBV4	1077	721	0.03%	0.006%
36	6.862	1788	1795	1798	rBV7	1755	1789	0.08%	0.014%
37	6.884	1798	1802	1804	rBV3	1226	848	0.04%	0.007%
38	6.923	1812	1814	1817	rBV3	1422	962	0.04%	0.008%
39	7.007	1830	1840	1857	rBV	172369	307096	13.92%	2.431%
40	7.109	1869	1872	1874	rBV4	1468	1059	0.05%	0.008%
41	7.338	1931	1943	1961	rBV	624519	1067708	48.40%	8.452%
42	7.563	2011	2013	2014	rBV2	1355	578	0.03%	0.005%
43	7.640	2028	2037	2053	rBV	125323	211732	9.60%	1.676%
44	7.923	2122	2125	2127	rBV3	1541	905	0.04%	0.007%
45	8.106	2172	2182	2212	rBV	390353	694256	31.47%	5.496%
46	8.531	2311	2314	2316	rBV4	996	642	0.03%	0.005%
47	8.582	2328	2330	2332	rBV3	1062	535	0.02%	0.004%
48	8.775	2386	2390	2393	rBV5	1449	1411	0.06%	0.011%
49	8.875	2409	2421	2439	rBV	615824	989960	44.87%	7.837%
50	9.019	2464	2466	2467	rBV3	1528	698	0.03%	0.006%
51	9.225	2526	2530	2532	rBV4	915	708	0.03%	0.006%
52	9.299	2550	2553	2554	rBV2	1048	549	0.02%	0.004%
53	9.354	2564	2570	2574	rBV7	1557	1763	0.08%	0.014%
54	9.428	2589	2593	2595	rBV3	967	639	0.03%	0.005%
55	9.469	2604	2606	2609	rBV4	1257	648	0.03%	0.005%
56	9.685	2666	2673	2676	rBV5	1745	2241	0.10%	0.018%
57	9.717	2681	2683	2688	rBV4	922	970	0.04%	0.008%
58	9.765	2695	2698	2701	rBV4	706	549	0.02%	0.004%
59	9.884	2733	2735	2742	rVB7	1403	1069	0.05%	0.008%
60	10.077	2792	2795	2801	rBV7	1403	1561	0.07%	0.012%
61	10.238	2834	2845	2864	rBV	410127	643792	29.18%	5.097%
62	10.392	2891	2893	2895	rBV2	2035	1035	0.05%	0.008%
63	10.457	2908	2913	2915	rBV5	1057	833	0.04%	0.007%
64	10.527	2934	2935	2939	rVB3	1335	600	0.03%	0.005%
65	10.550	2939	2942	2944	rBV3	804	657	0.03%	0.005%
66	10.916	3054	3056	3059	rBV4	1000	699	0.03%	0.006%
67	11.010	3082	3085	3088	rBV3	954	974	0.04%	0.008%
68	11.112	3114	3117	3119	rBV3	1403	943	0.04%	0.007%
69	11.154	3127	3130	3131	rBV3	976	513	0.02%	0.004%
70	11.270	3154	3166	3185	rBV	635269	967168	43.84%	7.657%
71	11.415	3209	3211	3213	rBV2	1493	669	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016586.D
 Acq On : 06 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2895-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0J5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.450	3218	3222	3223	rBV3	1498	1004	0.05%	0.008%
73	11.646	3269	3283	3298	rBV	669075	1047748	47.49%	8.294%
74	11.881	3351	3356	3357	rBV5	1332	917	0.04%	0.007%
75	11.907	3362	3364	3368	rVB4	1513	720	0.03%	0.006%
76	12.032	3401	3403	3405	rBV3	1426	492	0.02%	0.004%
77	12.119	3429	3430	3433	rBV3	936	606	0.03%	0.005%
78	12.174	3445	3447	3448	rVV2	2050	615	0.03%	0.005%
79	12.193	3451	3453	3458	rVB4	1685	1075	0.05%	0.009%
80	12.212	3458	3459	3462	rVB3	1039	509	0.02%	0.004%
81	12.244	3466	3469	3470	rBV3	1042	493	0.02%	0.004%
82	12.460	3534	3536	3538	rBV3	1237	614	0.03%	0.005%
83	12.620	3582	3586	3588	rVB3	1022	606	0.03%	0.005%
84	12.649	3588	3595	3598	rBV8	1383	1300	0.06%	0.010%
85	12.903	3670	3674	3677	rBV5	1966	1670	0.08%	0.013%
86	12.981	3695	3698	3703	rBV6	1427	1488	0.07%	0.012%
87	13.177	3754	3759	3762	rBV7	1908	1823	0.08%	0.014%
88	13.196	3763	3765	3767	rBV3	1025	552	0.03%	0.004%
89	13.238	3775	3778	3780	rBV3	1367	913	0.04%	0.007%
90	13.267	3785	3787	3788	rBV2	1255	521	0.02%	0.004%
91	13.344	3807	3811	3812	rVB3	1176	730	0.03%	0.006%
92	13.360	3812	3816	3818	rBV4	815	516	0.02%	0.004%
93	13.411	3828	3832	3833	rBV2	1520	987	0.04%	0.008%
94	13.501	3857	3860	3863	rBV3	1500	1157	0.05%	0.009%
95	13.749	3935	3937	3940	rBV3	1248	691	0.03%	0.005%
96	13.768	3940	3943	3945	rBV5	1457	985	0.04%	0.008%
97	13.813	3953	3957	3961	rBV5	1422	1308	0.06%	0.010%
98	14.196	4071	4076	4077	rBV4	1632	1360	0.06%	0.011%
99	14.296	4102	4107	4110	rBV6	1386	1397	0.06%	0.011%
100	14.347	4122	4123	4128	rVB3	1557	997	0.05%	0.008%


Sum of corrected areas: 12631904

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016586.D
Acq On : 06 Jun 2020 13:41
Operator : SY/MD
Sample : L2895-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0J5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

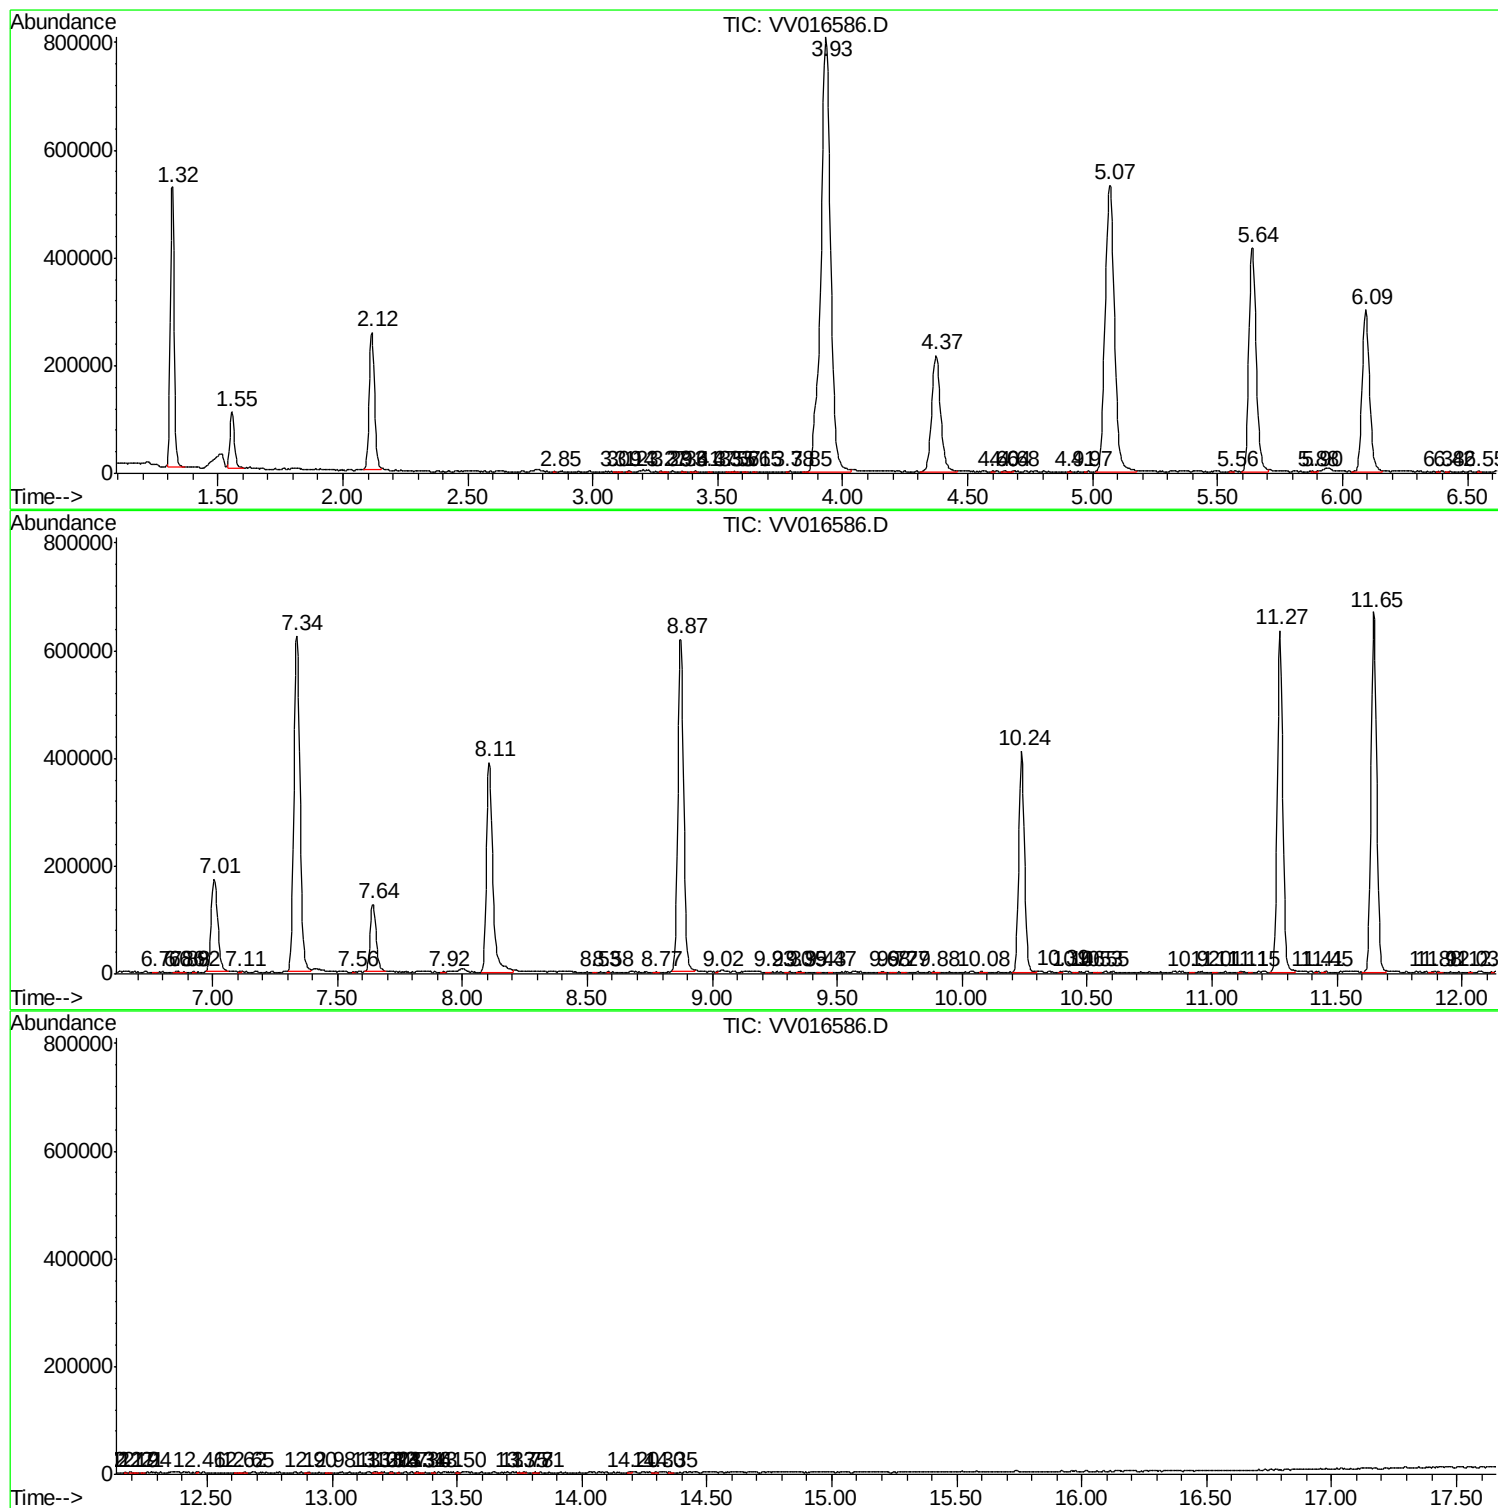

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016586.D
Acq On : 06 Jun 2020 13:41
Operator : SY/MD
Sample : L2895-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0J5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016586.D
Acq On : 06 Jun 2020 13:41
Operator : SY/MD
Sample : L2895-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
EW0J5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc