

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016587.D
 Acq On : 06 Jun 2020 14:05
 Operator : SY/MD
 Sample : L2895-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0J6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	82	rVB2	547060	574247	25.63%	4.361%
2	1.560	140	146	161	rVB	120167	146587	6.54%	1.113%
3	2.116	309	319	334	rBV	268247	398873	17.80%	3.029%
4	2.608	470	472	475	rBV3	1612	1083	0.05%	0.008%
5	2.711	501	504	505	rBV3	998	571	0.03%	0.004%
6	2.942	571	576	577	rBV5	720	538	0.02%	0.004%
7	3.052	607	610	612	rBV4	752	468	0.02%	0.004%
8	3.097	620	624	625	rVB4	966	565	0.03%	0.004%
9	3.145	637	639	641	rVB2	1338	610	0.03%	0.005%
10	3.164	641	645	647	rBV5	1284	660	0.03%	0.005%
11	3.367	702	708	710	rBV7	1481	1259	0.06%	0.010%
12	3.441	729	731	733	rBV2	1364	575	0.03%	0.004%
13	3.486	743	745	747	rBV2	884	549	0.02%	0.004%
14	3.672	801	803	805	rBV2	1185	538	0.02%	0.004%
15	3.730	818	821	824	rVB4	1393	918	0.04%	0.007%
16	3.753	826	828	832	rBV4	1045	671	0.03%	0.005%
17	3.782	832	837	838	rBV3	1012	826	0.04%	0.006%
18	3.830	848	852	853	rBV2	1115	548	0.02%	0.004%
19	3.843	853	856	861	rVV6	1105	1124	0.05%	0.009%
20	3.933	861	884	915	rBV2	825953	2240444	100.00%	17.014%
21	4.196	964	966	968	rBV4	1012	470	0.02%	0.004%
22	4.270	987	989	991	rBV3	904	477	0.02%	0.004%
23	4.373	1007	1021	1042	rBV	220890	530782	23.69%	4.031%
24	4.608	1089	1094	1095	rBV4	1725	1342	0.06%	0.010%
25	4.653	1106	1108	1112	rBV4	780	480	0.02%	0.004%
26	4.785	1146	1149	1150	rBV	997	609	0.03%	0.005%
27	4.856	1167	1171	1172	rBV3	1364	839	0.04%	0.006%
28	5.000	1213	1216	1220	rBV4	1135	859	0.04%	0.007%
29	5.071	1220	1238	1267	rBV2	543213	1409948	62.93%	10.707%
30	5.277	1300	1302	1307	rBV4	1556	1217	0.05%	0.009%
31	5.476	1361	1364	1366	rBV3	1484	1001	0.04%	0.008%
32	5.515	1374	1376	1379	rBV4	1477	1102	0.05%	0.008%
33	5.640	1402	1415	1435	rBV	464120	916183	40.89%	6.958%
34	5.875	1484	1488	1490	rBV3	1713	1187	0.05%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016587.D
 Acq On : 06 Jun 2020 14:05
 Operator : SY/MD
 Sample : L2895-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0J6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1543	1556	1577	rBV	312104	627423	28.00%	4.765%
36	6.277	1610	1613	1615	rBV3	1547	778	0.03%	0.006%
37	6.351	1633	1636	1639	rBV4	1222	776	0.03%	0.006%
38	6.557	1698	1700	1703	rBV2	1168	465	0.02%	0.004%
39	6.621	1717	1720	1721	rBV4	993	568	0.03%	0.004%
40	6.737	1752	1756	1759	rBV4	1883	1370	0.06%	0.010%
41	6.794	1772	1774	1779	rVB5	1616	973	0.04%	0.007%
42	6.817	1779	1781	1785	rVB2	1926	1318	0.06%	0.010%
43	7.007	1830	1840	1854	rVV	181051	314438	14.03%	2.388%
44	7.338	1931	1943	1960	rBV	648352	1109365	49.52%	8.425%
45	7.643	2028	2038	2052	rBV	125169	209648	9.36%	1.592%
46	7.810	2088	2090	2094	rVB4	1711	946	0.04%	0.007%
47	7.926	2123	2126	2128	rBV4	1127	648	0.03%	0.005%
48	7.997	2142	2148	2149	rBV5	3561	3363	0.15%	0.026%
49	8.106	2170	2182	2210	rBV	405585	710808	31.73%	5.398%
50	8.476	2294	2297	2298	rBV3	1052	505	0.02%	0.004%
51	8.495	2299	2303	2306	rVV5	1228	1111	0.05%	0.008%
52	8.534	2312	2315	2321	rBV6	1427	1504	0.07%	0.011%
53	8.589	2330	2332	2333	rBV2	1185	534	0.02%	0.004%
54	8.730	2374	2376	2379	rVB3	1467	796	0.04%	0.006%
55	8.801	2396	2398	2403	rVB4	1271	964	0.04%	0.007%
56	8.875	2409	2421	2442	rBV	689167	1107119	49.42%	8.408%
57	9.135	2498	2502	2504	rBV4	1169	942	0.04%	0.007%
58	9.219	2527	2528	2530	rBV2	1113	482	0.02%	0.004%
59	9.254	2536	2539	2540	rBV3	1136	589	0.03%	0.004%
60	9.367	2571	2574	2578	rVB6	1210	719	0.03%	0.005%
61	9.428	2590	2593	2598	rBV6	2213	2065	0.09%	0.016%
62	9.454	2598	2601	2603	rBV3	974	584	0.03%	0.004%
63	9.563	2630	2635	2636	rBV2	2197	1146	0.05%	0.009%
64	9.656	2661	2664	2669	rBV6	1308	1372	0.06%	0.010%
65	9.679	2669	2671	2673	rBV3	1418	586	0.03%	0.004%
66	9.711	2678	2681	2684	rVB4	1201	729	0.03%	0.006%
67	9.727	2684	2686	2688	rBV3	1195	598	0.03%	0.005%
68	9.791	2705	2706	2713	rVB8	1427	1137	0.05%	0.009%
69	10.013	2771	2775	2776	rBV4	1479	936	0.04%	0.007%
70	10.238	2830	2845	2861	rBV	424511	671018	29.95%	5.096%
71	10.367	2883	2885	2886	rBV2	1299	599	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016587.D
 Acq On : 06 Jun 2020 14:05
 Operator : SY/MD
 Sample : L2895-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0J6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.672	2978	2980	2982	rBV3	835	541	0.02%	0.004%
73	10.820	3023	3026	3031	rBV5	1303	1053	0.05%	0.008%
74	11.074	3102	3105	3109	rBV5	1244	1194	0.05%	0.009%
75	11.097	3109	3112	3115	rBV4	1141	1028	0.05%	0.008%
76	11.270	3155	3166	3185	rVV	699763	1067159	47.63%	8.104%
77	11.518	3241	3243	3244	rBV	1201	489	0.02%	0.004%
78	11.646	3272	3283	3300	rVB	677139	1058507	47.25%	8.038%
79	11.942	3369	3375	3378	rBV7	1079	1293	0.06%	0.010%
80	12.003	3392	3394	3396	rBV2	1001	517	0.02%	0.004%
81	12.148	3437	3439	3443	rBV4	1103	811	0.04%	0.006%
82	12.521	3552	3555	3556	rBV2	1361	664	0.03%	0.005%
83	12.682	3603	3605	3607	rBV3	1119	558	0.02%	0.004%
84	12.720	3612	3617	3621	rBV6	1544	1951	0.09%	0.015%
85	12.904	3672	3674	3677	rVB4	1633	865	0.04%	0.007%
86	12.923	3677	3680	3681	rBV2	1761	878	0.04%	0.007%
87	13.003	3701	3705	3706	rBV3	918	666	0.03%	0.005%
88	13.096	3731	3734	3735	rBV3	1670	798	0.04%	0.006%
89	13.186	3759	3762	3763	rBV3	1303	618	0.03%	0.005%
90	13.264	3784	3786	3789	rVB4	1377	848	0.04%	0.006%
91	13.283	3789	3792	3796	rVB4	2082	1693	0.08%	0.013%
92	13.302	3796	3798	3800	rBV2	1587	684	0.03%	0.005%
93	13.347	3810	3812	3816	rVV5	1281	1014	0.05%	0.008%
94	13.376	3819	3821	3825	rVB4	1239	809	0.04%	0.006%
95	13.431	3836	3838	3840	rBV3	1131	523	0.02%	0.004%
96	13.444	3840	3842	3845	rBV4	1097	669	0.03%	0.005%
97	13.691	3915	3919	3923	rVV5	1655	1883	0.08%	0.014%
98	13.932	3991	3994	3996	rBV4	1231	948	0.04%	0.007%
99	14.804	4263	4265	4267	rBV2	1799	996	0.04%	0.008%
100	14.916	4297	4300	4302	rBV3	1746	1250	0.06%	0.009%


Sum of corrected areas: 13167979

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016587.D
Acq On : 06 Jun 2020 14:05
Operator : SY/MD
Sample : L2895-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0J6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

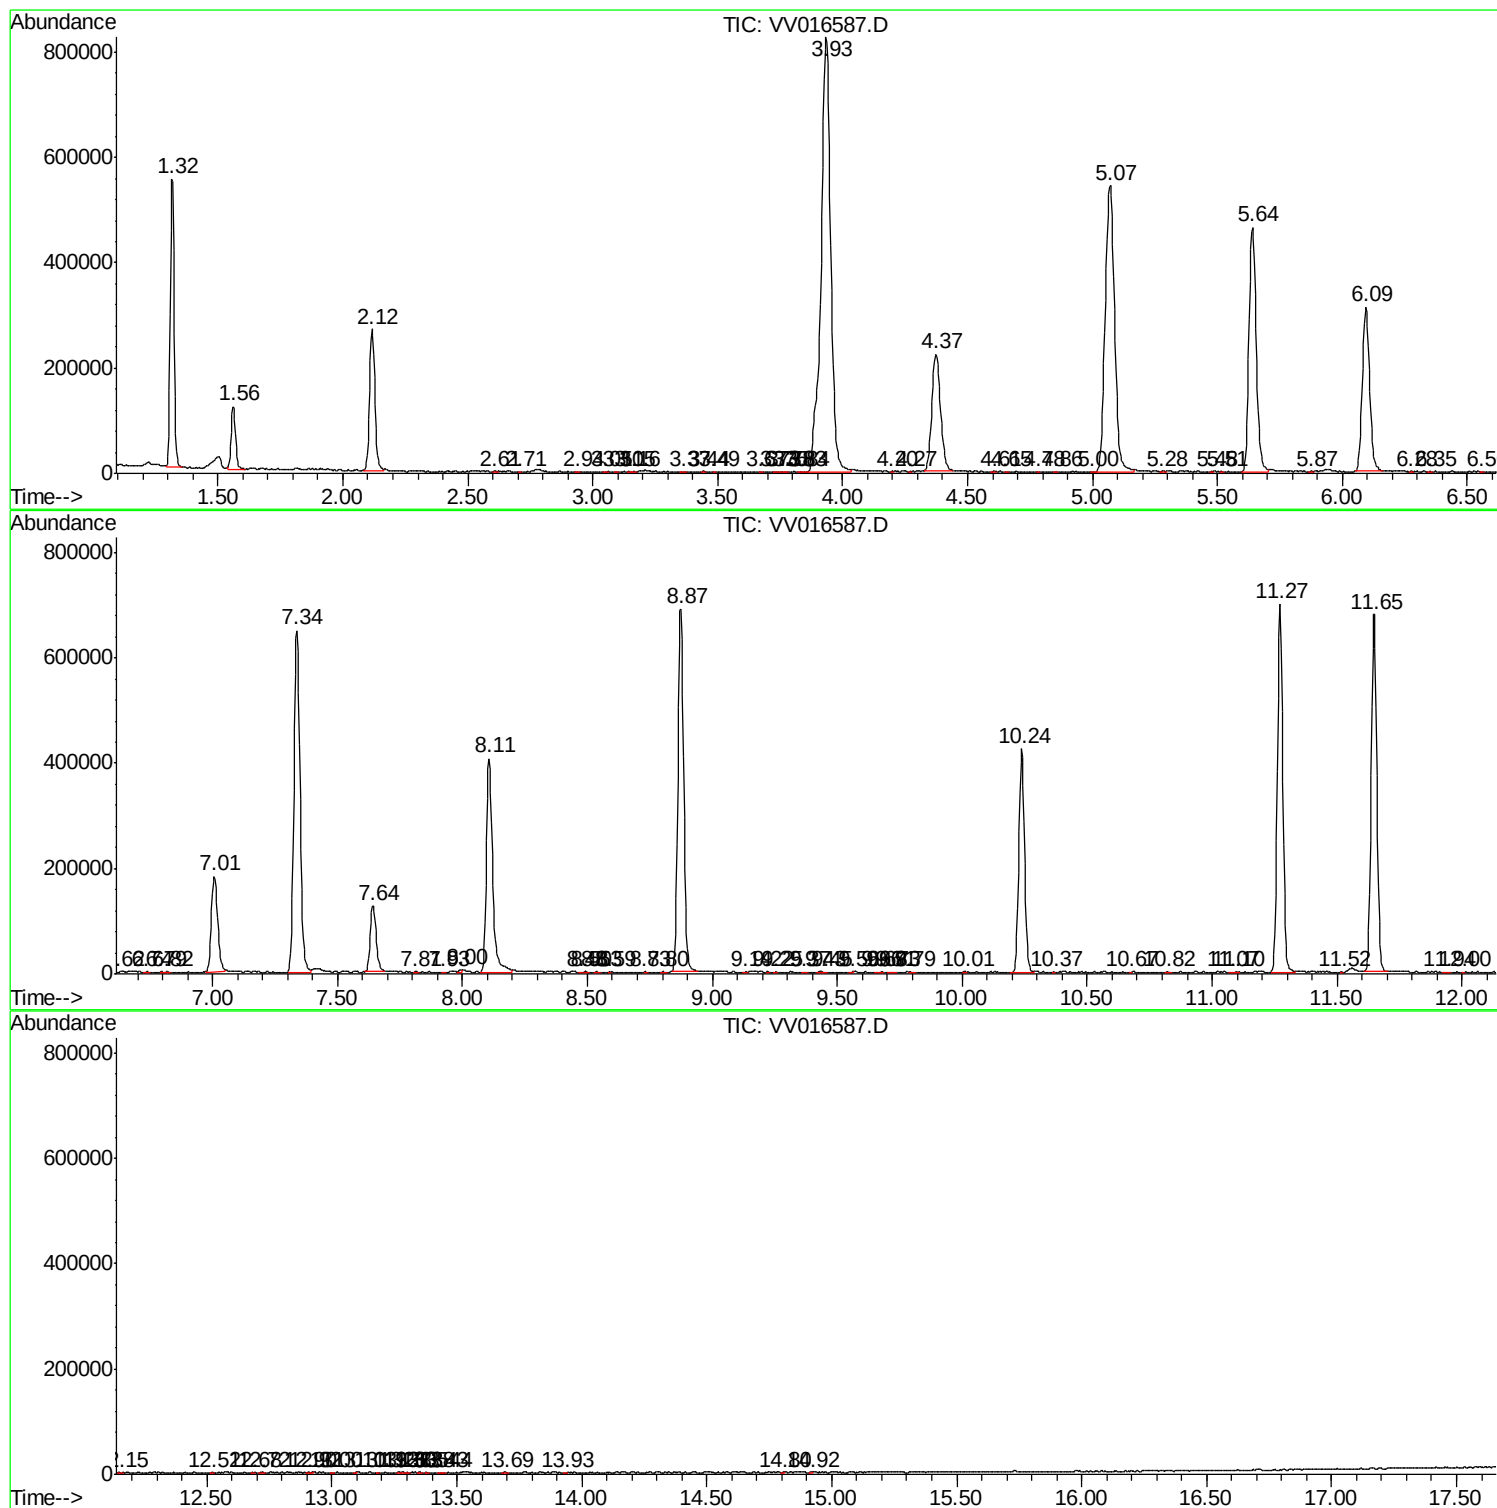

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016587.D
Acq On : 06 Jun 2020 14:05
Operator : SY/MD
Sample : L2895-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0J6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016587.D
Acq On : 06 Jun 2020 14:05
Operator : SY/MD
Sample : L2895-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
EW0J6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc