

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016588.D
 Acq On : 06 Jun 2020 14:29
 Operator : SY/MD
 Sample : L2895-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	83	rVB	171538	174114	12.50%	1.647%
2	1.560	140	146	155	rVB	113706	132414	9.51%	1.252%
3	2.116	310	319	337	rVB	258714	382765	27.49%	3.620%
4	2.766	518	521	523	rBV3	1456	942	0.07%	0.009%
5	2.827	538	540	543	rVB4	1253	686	0.05%	0.006%
6	2.872	549	554	556	rBV4	945	914	0.07%	0.009%
7	2.885	556	558	561	rVV4	1165	726	0.05%	0.007%
8	2.971	582	585	589	rVV5	1290	971	0.07%	0.009%
9	3.090	620	622	625	rVB3	1354	613	0.04%	0.006%
10	3.155	640	642	644	rBV2	889	562	0.04%	0.005%
11	3.296	683	686	687	rBV3	984	618	0.04%	0.006%
12	3.460	735	737	740	rVB4	1180	662	0.05%	0.006%
13	3.541	760	762	767	rBV6	946	752	0.05%	0.007%
14	3.566	767	770	773	rVV6	1050	786	0.06%	0.007%
15	3.595	777	779	782	rVB3	1414	680	0.05%	0.006%
16	3.788	836	839	841	rBV3	977	669	0.05%	0.006%
17	3.897	862	873	875	rBV	120040	182966	13.14%	1.730%
18	4.312	999	1002	1004	rBV3	994	677	0.05%	0.006%
19	4.373	1007	1021	1046	rVB	221277	540897	38.84%	5.115%
20	4.650	1105	1107	1112	rBV3	1523	1150	0.08%	0.011%
21	4.836	1160	1165	1166	rBV3	1073	916	0.07%	0.009%
22	4.878	1176	1178	1182	rVB3	1104	743	0.05%	0.007%
23	4.897	1182	1184	1185	rBV2	1528	557	0.04%	0.005%
24	4.978	1205	1209	1212	rVB4	1695	1137	0.08%	0.011%
25	5.007	1214	1218	1219	rBV4	1474	835	0.06%	0.008%
26	5.071	1219	1238	1268	rVV2	544180	1392466	100.00%	13.169%
27	5.319	1314	1315	1317	rBV2	1379	672	0.05%	0.006%
28	5.492	1363	1369	1370	rBV5	782	756	0.05%	0.007%
29	5.579	1393	1396	1398	rBV4	1343	644	0.05%	0.006%
30	5.640	1398	1415	1437	rBV	459202	916917	65.85%	8.671%
31	5.791	1460	1462	1465	rBV3	1172	787	0.06%	0.007%
32	6.093	1543	1556	1581	rBV	312748	628617	45.14%	5.945%
33	6.402	1651	1652	1656	rVB4	1762	826	0.06%	0.008%
34	6.518	1685	1688	1692	rVB6	1677	1022	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016588.D
 Acq On : 06 Jun 2020 14:29
 Operator : SY/MD
 Sample : L2895-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.537	1692	1694	1698	rBV6	859	704	0.05%	0.007%
36	6.640	1720	1726	1731	rBV8	2109	2240	0.16%	0.021%
37	6.785	1769	1771	1774	rVB4	1275	626	0.04%	0.006%
38	6.907	1807	1809	1812	rBV4	1261	770	0.06%	0.007%
39	7.007	1826	1840	1857	rBV	177084	314700	22.60%	2.976%
40	7.293	1926	1929	1930	rBV2	1206	701	0.05%	0.007%
41	7.338	1930	1943	1959	rVV	633453	1091990	78.42%	10.327%
42	7.579	2015	2018	2021	rBV4	1787	1356	0.10%	0.013%
43	7.640	2028	2037	2057	rBV	125551	209453	15.04%	1.981%
44	7.814	2089	2091	2094	rVB5	1266	641	0.05%	0.006%
45	7.897	2114	2117	2120	rBV4	1673	994	0.07%	0.009%
46	8.106	2172	2182	2213	rBV	395229	691317	49.65%	6.538%
47	8.434	2282	2284	2286	rBV3	1039	573	0.04%	0.005%
48	8.460	2290	2292	2298	rVB5	1767	1657	0.12%	0.016%
49	8.756	2380	2384	2388	rBV5	1387	1501	0.11%	0.014%
50	8.801	2395	2398	2401	rBV3	1052	691	0.05%	0.007%
51	8.875	2408	2421	2436	rBV	684136	1091253	78.37%	10.320%
52	9.373	2573	2576	2578	rBV3	988	702	0.05%	0.007%
53	9.408	2583	2587	2588	rBV3	992	720	0.05%	0.007%
54	9.566	2633	2636	2637	rBV2	1379	711	0.05%	0.007%
55	9.643	2657	2660	2662	rBV3	2094	1407	0.10%	0.013%
56	9.704	2677	2679	2684	rBV6	1219	872	0.06%	0.008%
57	9.804	2707	2710	2712	rBV4	1351	987	0.07%	0.009%
58	9.846	2719	2723	2724	rBV2	1114	653	0.05%	0.006%
59	10.183	2826	2828	2832	rBV5	979	575	0.04%	0.005%
60	10.238	2832	2845	2861	rVV	423892	663957	47.68%	6.279%
61	10.389	2890	2892	2894	rBV3	1430	693	0.05%	0.007%
62	10.470	2914	2917	2919	rBV4	1194	688	0.05%	0.007%
63	10.736	2995	3000	3002	rBV6	1387	1048	0.08%	0.010%
64	10.836	3029	3031	3034	rBV3	1276	808	0.06%	0.008%
65	10.871	3037	3042	3050	rVV9	1565	2304	0.17%	0.022%
66	10.990	3075	3079	3081	rBV4	1281	978	0.07%	0.009%
67	11.097	3110	3112	3117	rBV4	1888	1849	0.13%	0.017%
68	11.270	3154	3166	3183	rBV	678236	1042163	74.84%	9.856%
69	11.550	3249	3253	3255	rBV5	2615	2283	0.16%	0.022%
70	11.646	3271	3283	3299	rBV	665662	1041392	74.79%	9.848%
71	11.910	3363	3365	3368	rBV4	956	577	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016588.D
 Acq On : 06 Jun 2020 14:29
 Operator : SY/MD
 Sample : L2895-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.122	3429	3431	3434	rBV4	963	602	0.04%	0.006%
73	12.138	3434	3436	3440	rVB5	1843	1301	0.09%	0.012%
74	12.187	3449	3451	3453	rBV3	1462	680	0.05%	0.006%
75	12.325	3492	3494	3499	rVB4	1869	1111	0.08%	0.011%
76	12.360	3499	3505	3507	rBV6	1413	1587	0.11%	0.015%
77	12.453	3530	3534	3537	rVB5	1725	1325	0.10%	0.013%
78	12.479	3540	3542	3545	rVB3	1542	661	0.05%	0.006%
79	12.508	3545	3551	3555	rBV8	1891	1846	0.13%	0.017%
80	12.531	3556	3558	3562	rVB3	1149	608	0.04%	0.006%
81	12.553	3562	3565	3566	rBV3	1278	556	0.04%	0.005%
82	12.756	3624	3628	3629	rBV3	1361	668	0.05%	0.006%
83	12.778	3633	3635	3638	rVB3	1055	548	0.04%	0.005%
84	12.797	3638	3641	3643	rBV3	1481	888	0.06%	0.008%
85	12.897	3669	3672	3673	rBV3	1240	760	0.05%	0.007%
86	12.945	3684	3687	3689	rVB3	1255	703	0.05%	0.007%
87	13.145	3746	3749	3750	rBV4	1239	786	0.06%	0.007%
88	13.424	3832	3836	3837	rBV4	1376	845	0.06%	0.008%
89	13.447	3840	3843	3845	rBV3	1287	815	0.06%	0.008%
90	13.598	3885	3890	3891	rBV3	1161	775	0.06%	0.007%
91	13.685	3913	3917	3919	rBV4	987	611	0.04%	0.006%
92	13.862	3970	3972	3976	rVB3	1110	566	0.04%	0.005%
93	13.952	3996	4000	4004	rBV5	1278	1564	0.11%	0.015%
94	14.000	4013	4015	4019	rVB3	1292	713	0.05%	0.007%
95	14.026	4019	4023	4027	rBV7	1069	933	0.07%	0.009%
96	14.739	4243	4245	4250	rBV4	1186	856	0.06%	0.008%
97	14.842	4275	4277	4281	rBV3	1471	1410	0.10%	0.013%
98	14.862	4281	4283	4286	rVV4	1194	677	0.05%	0.006%
99	14.948	4307	4310	4312	rBV4	1165	798	0.06%	0.008%
100	15.662	4529	4532	4533	rBV3	1719	983	0.07%	0.009%


Sum of corrected areas: 10574169

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016588.D
Acq On : 06 Jun 2020 14:29
Operator : SY/MD
Sample : L2895-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

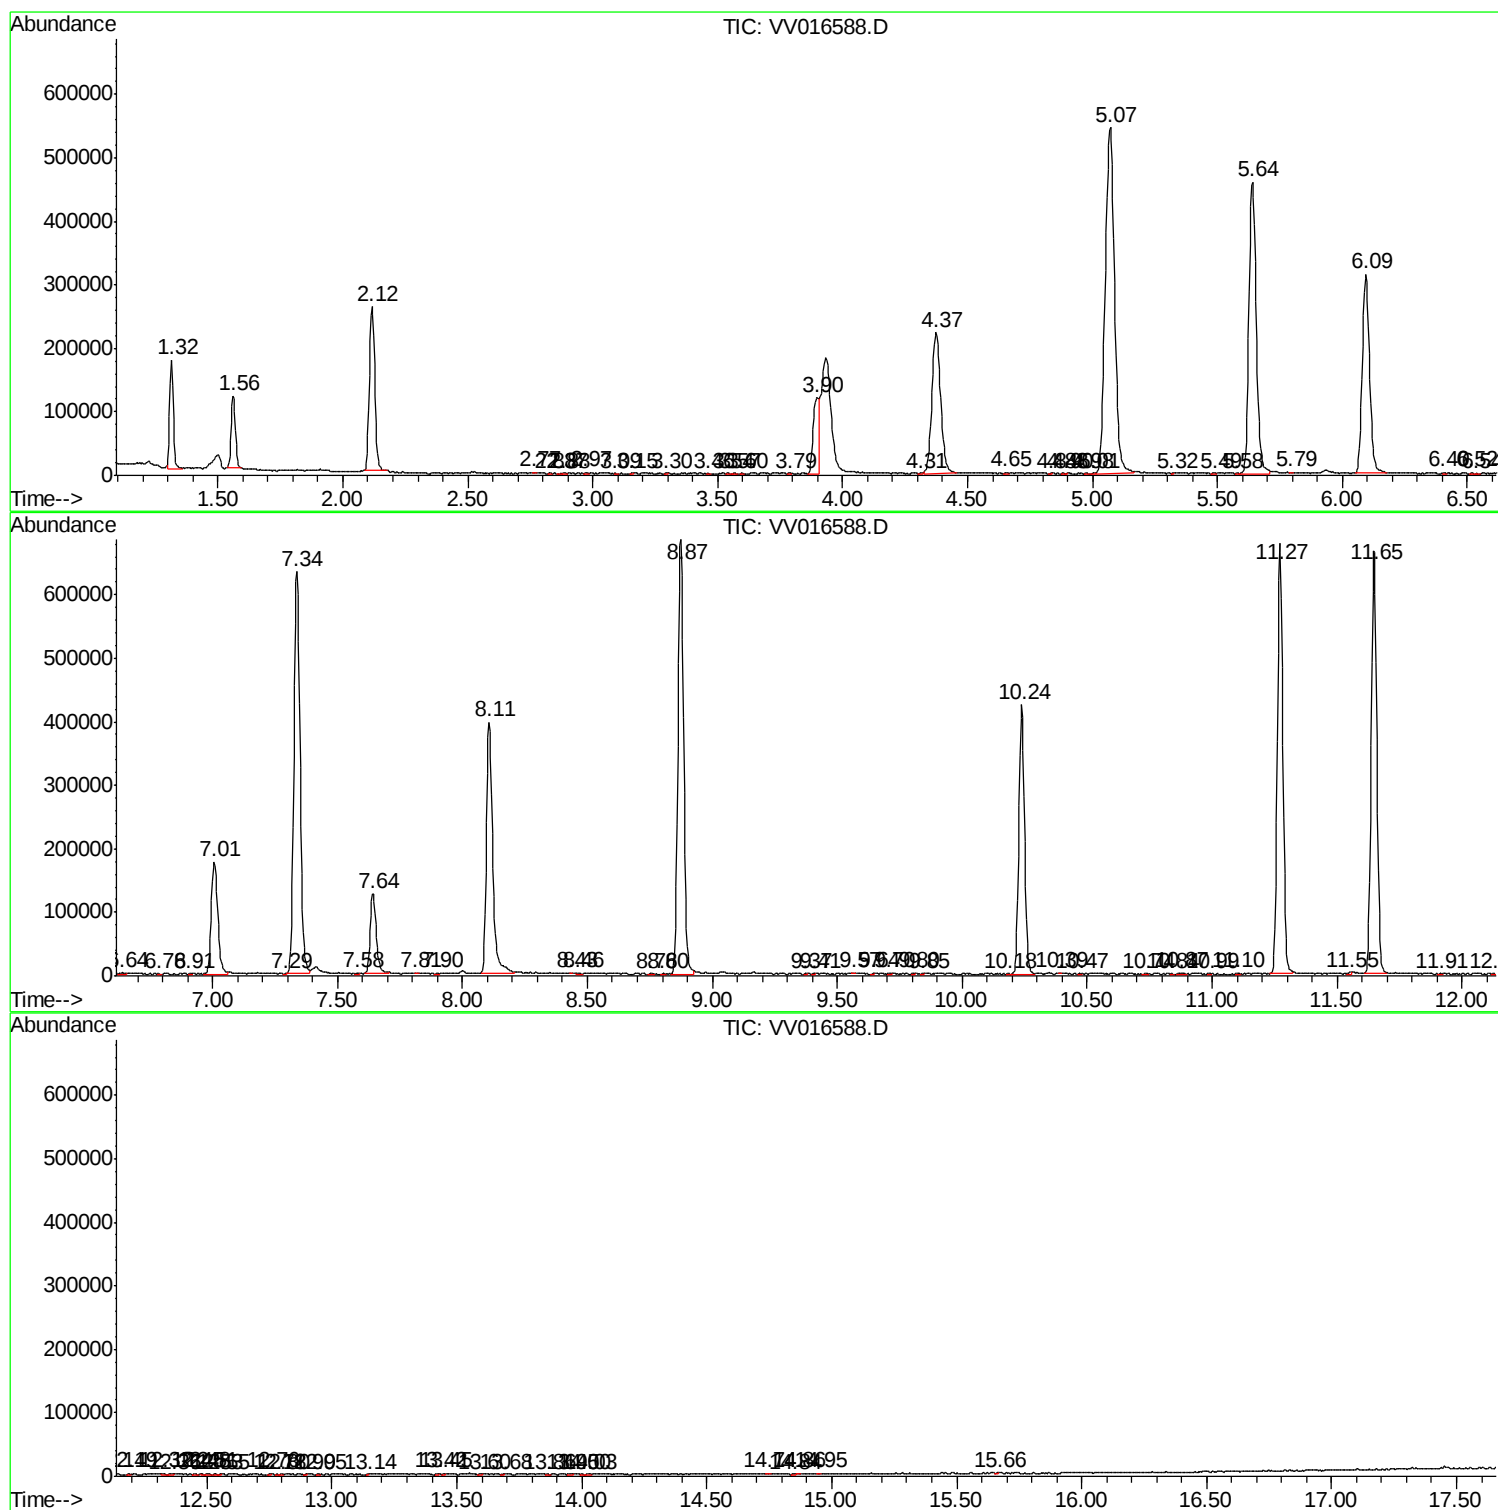

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016588.D
Acq On : 06 Jun 2020 14:29
Operator : SY/MD
Sample : L2895-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016588.D
Acq On : 06 Jun 2020 14:29
Operator : SY/MD
Sample : L2895-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc