

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016589.D
 Acq On : 06 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2895-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	83	rVB	163377	166220	12.07%	1.454%
2	1.560	140	146	160	rVB	113971	136039	9.88%	1.190%
3	2.116	310	319	335	rVB	255935	379896	27.59%	3.322%
4	2.283	366	371	375	rBV5	2332	3042	0.22%	0.027%
5	2.421	411	414	416	rBV3	1191	728	0.05%	0.006%
6	2.579	459	463	464	rBV3	1463	1052	0.08%	0.009%
7	2.820	535	538	540	rBV4	1078	696	0.05%	0.006%
8	2.904	561	564	568	rBV4	1263	1066	0.08%	0.009%
9	3.026	600	602	604	rBV3	1033	620	0.05%	0.005%
10	3.055	609	611	614	rVV4	1143	609	0.04%	0.005%
11	3.071	614	616	620	rVB4	1710	853	0.06%	0.007%
12	3.100	623	625	628	rVB3	1214	719	0.05%	0.006%
13	3.116	628	630	634	rBV4	991	793	0.06%	0.007%
14	3.261	673	675	680	rBV4	1439	1219	0.09%	0.011%
15	3.296	683	686	689	rBV4	1196	966	0.07%	0.008%
16	3.328	694	696	698	rBV3	1231	602	0.04%	0.005%
17	3.418	721	724	726	rVB3	1248	674	0.05%	0.006%
18	3.502	746	750	752	rBV4	1059	717	0.05%	0.006%
19	3.614	781	785	786	rBV2	976	593	0.04%	0.005%
20	3.630	789	790	795	rVB4	1538	679	0.05%	0.006%
21	3.672	797	803	805	rBV7	1337	1198	0.09%	0.010%
22	3.778	833	836	838	rBV4	1916	1186	0.09%	0.010%
23	3.933	861	884	908	rBV2	278855	926560	67.30%	8.103%
24	4.373	1004	1021	1047	rBV2	222889	545330	39.61%	4.769%
25	4.585	1085	1087	1093	rBV8	1462	1161	0.08%	0.010%
26	4.804	1153	1155	1159	rBV3	1574	1106	0.08%	0.010%
27	4.855	1168	1171	1177	rVB8	1967	1466	0.11%	0.013%
28	4.910	1185	1188	1190	rBV4	1274	779	0.06%	0.007%
29	4.958	1202	1203	1207	rBV4	1016	786	0.06%	0.007%
30	5.071	1221	1238	1264	rBV2	530653	1376863	100.00%	12.042%
31	5.425	1345	1348	1351	rBV5	1541	1132	0.08%	0.010%
32	5.640	1402	1415	1439	rBV	454402	906632	65.85%	7.929%
33	5.939	1496	1508	1523	rBV3	44976	96438	7.00%	0.843%
34	6.093	1543	1556	1581	rBV	306299	620175	45.04%	5.424%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016589.D
 Acq On : 06 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2895-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.347	1632	1635	1636	rBV3	1319	717	0.05%	0.006%
36	6.476	1673	1675	1680	rBV6	897	905	0.07%	0.008%
37	6.547	1694	1697	1698	rBV3	1416	742	0.05%	0.006%
38	6.566	1701	1703	1707	rVB4	1506	804	0.06%	0.007%
39	6.704	1743	1746	1748	rBV2	1414	860	0.06%	0.008%
40	6.817	1777	1781	1783	rBV4	821	619	0.04%	0.005%
41	7.006	1830	1840	1856	rBV	180016	312228	22.68%	2.731%
42	7.280	1922	1925	1928	rVB4	1844	1164	0.08%	0.010%
43	7.338	1928	1943	1961	rBV	637759	1097760	79.73%	9.601%
44	7.531	2000	2003	2005	rBV3	1323	660	0.05%	0.006%
45	7.640	2027	2037	2052	rBV	125605	211819	15.38%	1.852%
46	8.106	2172	2182	2212	rBV	400313	697733	50.68%	6.102%
47	8.457	2288	2291	2295	rBV4	1643	1785	0.13%	0.016%
48	8.595	2330	2334	2338	rVB6	1609	1318	0.10%	0.012%
49	8.749	2380	2382	2385	rVB2	1490	851	0.06%	0.007%
50	8.768	2385	2388	2390	rBV3	1126	778	0.06%	0.007%
51	8.813	2399	2402	2406	rBV6	1498	1406	0.10%	0.012%
52	8.875	2409	2421	2440	rVV	679648	1097014	79.67%	9.594%
53	9.296	2549	2552	2557	rVB7	1594	1396	0.10%	0.012%
54	9.321	2557	2560	2563	rBV5	1511	1209	0.09%	0.011%
55	9.338	2563	2565	2567	rVB3	1631	588	0.04%	0.005%
56	9.386	2573	2580	2582	rBV5	1578	1487	0.11%	0.013%
57	9.505	2613	2617	2620	rBV5	1159	966	0.07%	0.008%
58	9.592	2642	2644	2649	rBV6	954	593	0.04%	0.005%
59	9.733	2685	2688	2689	rBV2	1165	658	0.05%	0.006%
60	10.067	2790	2792	2796	rVB4	1505	1015	0.07%	0.009%
61	10.093	2796	2800	2801	rBV3	1008	603	0.04%	0.005%
62	10.112	2801	2806	2809	rBV7	1536	1256	0.09%	0.011%
63	10.186	2827	2829	2833	rBV5	840	656	0.05%	0.006%
64	10.238	2833	2845	2858	rBV	426083	663984	48.22%	5.807%
65	10.370	2882	2886	2887	rBV3	1186	820	0.06%	0.007%
66	10.402	2892	2896	2900	rBV6	2111	2366	0.17%	0.021%
67	10.489	2919	2923	2926	rBV6	1214	1005	0.07%	0.009%
68	10.598	2953	2957	2958	rBV3	1067	627	0.05%	0.005%
69	10.768	3008	3010	3013	rVB3	1375	758	0.06%	0.007%
70	10.884	3043	3046	3052	rVB6	1881	1498	0.11%	0.013%
71	10.945	3059	3065	3069	rVB7	1813	1992	0.14%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016589.D
 Acq On : 06 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2895-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.971	3069	3073	3074	rBV3	827	585	0.04%	0.005%
73	11.128	3119	3122	3126	rVV4	1378	950	0.07%	0.008%
74	11.270	3155	3166	3183	rBV	683003	1059700	76.96%	9.268%
75	11.428	3213	3215	3220	rVB6	1704	1260	0.09%	0.011%
76	11.450	3220	3222	3224	rBV3	1524	709	0.05%	0.006%
77	11.649	3271	3284	3300	rBV	673768	1058118	76.85%	9.254%
78	11.849	3343	3346	3350	rBV5	1570	990	0.07%	0.009%
79	11.868	3350	3352	3354	rBV3	1183	764	0.06%	0.007%
80	11.942	3373	3375	3377	rBV2	1328	656	0.05%	0.006%
81	11.981	3383	3387	3390	rBV5	895	603	0.04%	0.005%
82	12.061	3407	3412	3413	rBV4	1158	919	0.07%	0.008%
83	12.260	3471	3474	3476	rVV4	1697	1255	0.09%	0.011%
84	12.382	3508	3512	3515	rBV5	1137	1187	0.09%	0.010%
85	12.675	3601	3603	3607	rBV4	903	618	0.04%	0.005%
86	12.852	3655	3658	3662	rVB4	2112	1402	0.10%	0.012%
87	12.961	3690	3692	3694	rBV3	1482	756	0.05%	0.007%
88	13.019	3708	3710	3713	rBV4	889	657	0.05%	0.006%
89	13.074	3724	3727	3731	rVB3	1221	840	0.06%	0.007%
90	13.238	3776	3778	3781	rVV3	926	589	0.04%	0.005%
91	13.501	3857	3860	3863	rBV4	1658	959	0.07%	0.008%
92	13.755	3937	3939	3942	rBV3	1592	891	0.06%	0.008%
93	13.823	3956	3960	3964	rBV6	1307	1404	0.10%	0.012%
94	14.087	4040	4042	4047	rVB5	1024	844	0.06%	0.007%
95	14.119	4047	4052	4054	rBV4	1290	1140	0.08%	0.010%
96	14.151	4060	4062	4065	rBV3	1191	691	0.05%	0.006%
97	14.370	4128	4130	4131	rBV2	1516	637	0.05%	0.006%
98	14.559	4187	4189	4192	rVB2	1358	699	0.05%	0.006%
99	15.038	4333	4338	4344	rBV8	1519	2078	0.15%	0.018%
100	15.122	4361	4364	4366	rBV3	1625	1104	0.08%	0.010%


Sum of corrected areas: 11434240

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016589.D
Acq On : 06 Jun 2020 14:52
Operator : SY/MD
Sample : L2895-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

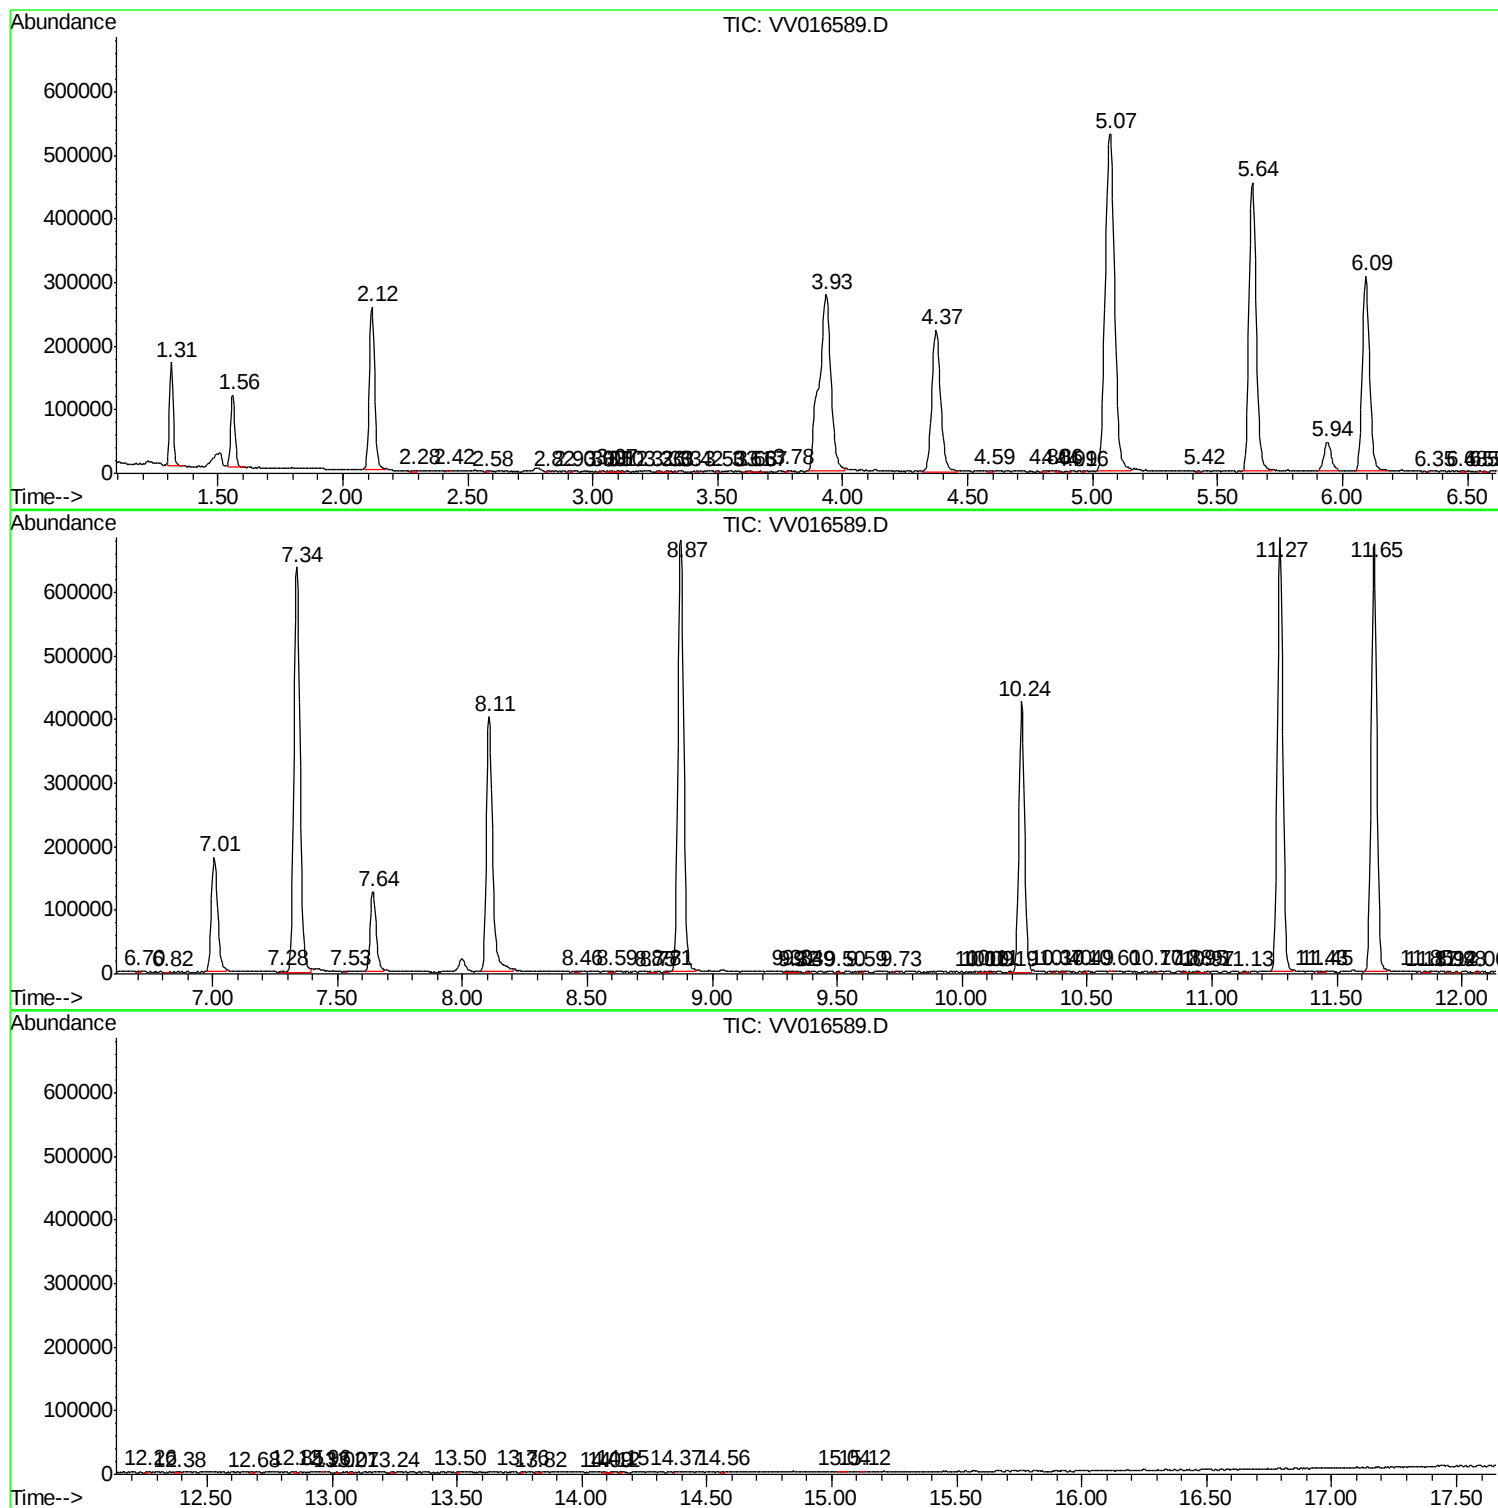

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016589.D
Acq On : 06 Jun 2020 14:52
Operator : SY/MD
Sample : L2895-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016589.D
Acq On : 06 Jun 2020 14:52
Operator : SY/MD
Sample : L2895-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc