

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016590.D
 Acq On : 06 Jun 2020 15:16
 Operator : SY/MD
 Sample : L2895-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	175103	183319	7.08%	1.366%
2	1.566	142	148	160	rVB	117534	139769	5.40%	1.041%
3	2.119	310	320	335	rBV	266614	395175	15.26%	2.944%
4	2.579	461	463	465	rBV3	1168	638	0.02%	0.005%
5	2.849	545	547	551	rBV5	1276	1041	0.04%	0.008%
6	3.039	603	606	607	rBV3	1353	722	0.03%	0.005%
7	3.071	612	616	618	rBV4	1223	1038	0.04%	0.008%
8	3.109	625	628	633	rVB6	1839	1670	0.06%	0.012%
9	3.132	633	635	638	rBV4	1525	1024	0.04%	0.008%
10	3.267	675	677	680	rBV4	756	588	0.02%	0.004%
11	3.379	710	712	715	rBV3	1428	788	0.03%	0.006%
12	3.408	718	721	723	rBV3	1532	818	0.03%	0.006%
13	3.473	739	741	743	rBV3	1176	696	0.03%	0.005%
14	3.515	750	754	758	rBV6	1507	1400	0.05%	0.010%
15	3.547	760	764	766	rVV5	1519	1208	0.05%	0.009%
16	3.572	766	772	776	rVV8	1277	1516	0.06%	0.011%
17	3.592	776	778	782	rVV5	784	606	0.02%	0.005%
18	3.637	790	792	797	rBV4	1051	734	0.03%	0.005%
19	3.752	824	828	831	rBV6	1018	822	0.03%	0.006%
20	3.772	831	834	835	rBV3	872	596	0.02%	0.004%
21	3.794	839	841	844	rBV3	1061	735	0.03%	0.005%
22	3.859	858	861	862	rBV3	1351	727	0.03%	0.005%
23	3.936	862	885	913	rVV2	974158	2590344	100.00%	19.301%
24	4.312	1000	1002	1004	rBV2	1560	804	0.03%	0.006%
25	4.373	1007	1021	1042	rVV	222582	541467	20.90%	4.034%
26	4.585	1083	1087	1088	rBV4	1357	1072	0.04%	0.008%
27	4.678	1114	1116	1124	rBV9	1203	1281	0.05%	0.010%
28	4.756	1138	1140	1142	rBV3	1411	798	0.03%	0.006%
29	5.000	1213	1216	1218	rBV4	1056	736	0.03%	0.005%
30	5.071	1219	1238	1261	rBV2	538564	1397953	53.97%	10.416%
31	5.640	1401	1415	1438	rBV	450175	895291	34.56%	6.671%
32	5.939	1496	1508	1523	rBV2	104606	208913	8.07%	1.557%
33	6.093	1543	1556	1575	rBV	313283	631238	24.37%	4.703%
34	6.270	1609	1611	1615	rVB5	1058	729	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016590.D
 Acq On : 06 Jun 2020 15:16
 Operator : SY/MD
 Sample : L2895-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.357	1635	1638	1640	rBV4	1317	762	0.03%	0.006%
36	6.428	1657	1660	1666	rBV8	1951	1691	0.07%	0.013%
37	6.530	1690	1692	1696	rVB3	1390	1017	0.04%	0.008%
38	6.556	1696	1700	1703	rBV6	1273	1263	0.05%	0.009%
39	6.891	1801	1804	1806	rBV3	1544	944	0.04%	0.007%
40	7.006	1829	1840	1863	rBV	178194	319446	12.33%	2.380%
41	7.215	1902	1905	1910	rVB6	1546	931	0.04%	0.007%
42	7.338	1931	1943	1960	rBV	648099	1103254	42.59%	8.220%
43	7.643	2027	2038	2053	rVV	126268	215519	8.32%	1.606%
44	7.855	2101	2104	2106	rBV4	1393	1128	0.04%	0.008%
45	7.894	2114	2116	2120	rVB4	1668	950	0.04%	0.007%
46	7.997	2136	2148	2166	rVB	129308	219853	8.49%	1.638%
47	8.106	2172	2182	2199	rBV	406586	671082	25.91%	5.000%
48	8.685	2360	2362	2365	rBV4	1404	853	0.03%	0.006%
49	8.874	2407	2421	2442	rBV	669582	1080644	41.72%	8.052%
50	9.022	2465	2467	2468	rBV2	1272	699	0.03%	0.005%
51	9.148	2503	2506	2508	rBV3	1402	1136	0.04%	0.008%
52	9.193	2518	2520	2526	rVB7	1234	961	0.04%	0.007%
53	9.241	2531	2535	2536	rBV3	1301	806	0.03%	0.006%
54	9.392	2580	2582	2586	rVB5	1497	783	0.03%	0.006%
55	9.710	2679	2681	2683	rBV3	1452	792	0.03%	0.006%
56	9.804	2707	2710	2713	rBV4	1332	810	0.03%	0.006%
57	9.874	2727	2732	2739	rVV7	1890	2259	0.09%	0.017%
58	9.974	2761	2763	2767	rVB3	1149	632	0.02%	0.005%
59	10.000	2767	2771	2775	rVB7	1142	988	0.04%	0.007%
60	10.022	2775	2778	2783	rVB7	1306	1003	0.04%	0.007%
61	10.106	2802	2804	2808	rVB4	950	667	0.03%	0.005%
62	10.196	2829	2832	2834	rBV4	1757	975	0.04%	0.007%
63	10.238	2834	2845	2863	rVV	424343	659809	25.47%	4.916%
64	10.350	2877	2880	2882	rBV5	1062	698	0.03%	0.005%
65	10.398	2891	2895	2897	rBV4	1737	1456	0.06%	0.011%
66	10.649	2969	2973	2976	rBV4	1044	698	0.03%	0.005%
67	10.794	3015	3018	3020	rBV4	1184	648	0.03%	0.005%
68	10.849	3034	3035	3040	rBV5	903	625	0.02%	0.005%
69	10.939	3060	3063	3066	rBV4	1208	1145	0.04%	0.009%
70	11.132	3121	3123	3126	rBV2	951	607	0.02%	0.005%
71	11.148	3126	3128	3133	rVB4	1299	800	0.03%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016590.D
 Acq On : 06 Jun 2020 15:16
 Operator : SY/MD
 Sample : L2895-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3186	rBV	664629	1020268	39.39%	7.602%
73	11.476	3225	3230	3232	rBV5	1515	1083	0.04%	0.008%
74	11.556	3245	3255	3264	rBV9	6840	13964	0.54%	0.104%
75	11.646	3273	3283	3304	rVB	660741	1048658	40.48%	7.813%
76	11.829	3336	3340	3341	rBV4	1063	733	0.03%	0.005%
77	11.887	3355	3358	3362	rBV6	2132	1466	0.06%	0.011%
78	11.919	3365	3368	3371	rVV4	1280	645	0.02%	0.005%
79	11.971	3381	3384	3389	rBV5	1468	1260	0.05%	0.009%
80	12.093	3418	3422	3423	rBV4	1663	872	0.03%	0.006%
81	12.202	3452	3456	3458	rBV4	1237	879	0.03%	0.007%
82	12.251	3467	3471	3473	rBV3	1592	1287	0.05%	0.010%
83	12.283	3479	3481	3485	rVB2	1205	674	0.03%	0.005%
84	12.508	3547	3551	3554	rBV4	1041	838	0.03%	0.006%
85	12.662	3595	3599	3601	rBV4	1025	796	0.03%	0.006%
86	12.755	3623	3628	3630	rBV5	1336	1132	0.04%	0.008%
87	12.797	3638	3641	3643	rBV4	1485	706	0.03%	0.005%
88	12.948	3687	3688	3693	rVB4	1367	733	0.03%	0.005%
89	13.022	3706	3711	3713	rVB4	1187	833	0.03%	0.006%
90	13.054	3716	3721	3722	rBV4	1031	836	0.03%	0.006%
91	13.099	3732	3735	3736	rBV3	1478	947	0.04%	0.007%
92	13.125	3739	3743	3744	rBV4	1366	888	0.03%	0.007%
93	13.228	3772	3775	3780	rBV6	1211	1138	0.04%	0.008%
94	13.267	3784	3787	3789	rVV3	1067	696	0.03%	0.005%
95	13.331	3803	3807	3809	rBV4	1745	1191	0.05%	0.009%
96	13.366	3815	3818	3820	rBV3	1283	926	0.04%	0.007%
97	14.148	4058	4061	4062	rBV2	1156	701	0.03%	0.005%
98	14.183	4069	4072	4078	rVB	15884	9696	0.37%	0.072%
99	14.562	4185	4190	4192	rBV5	2181	1613	0.06%	0.012%
100	14.842	4274	4277	4281	rBV4	1166	1061	0.04%	0.008%


Sum of corrected areas: 13421110

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016590.D
Acq On : 06 Jun 2020 15:16
Operator : SY/MD
Sample : L2895-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

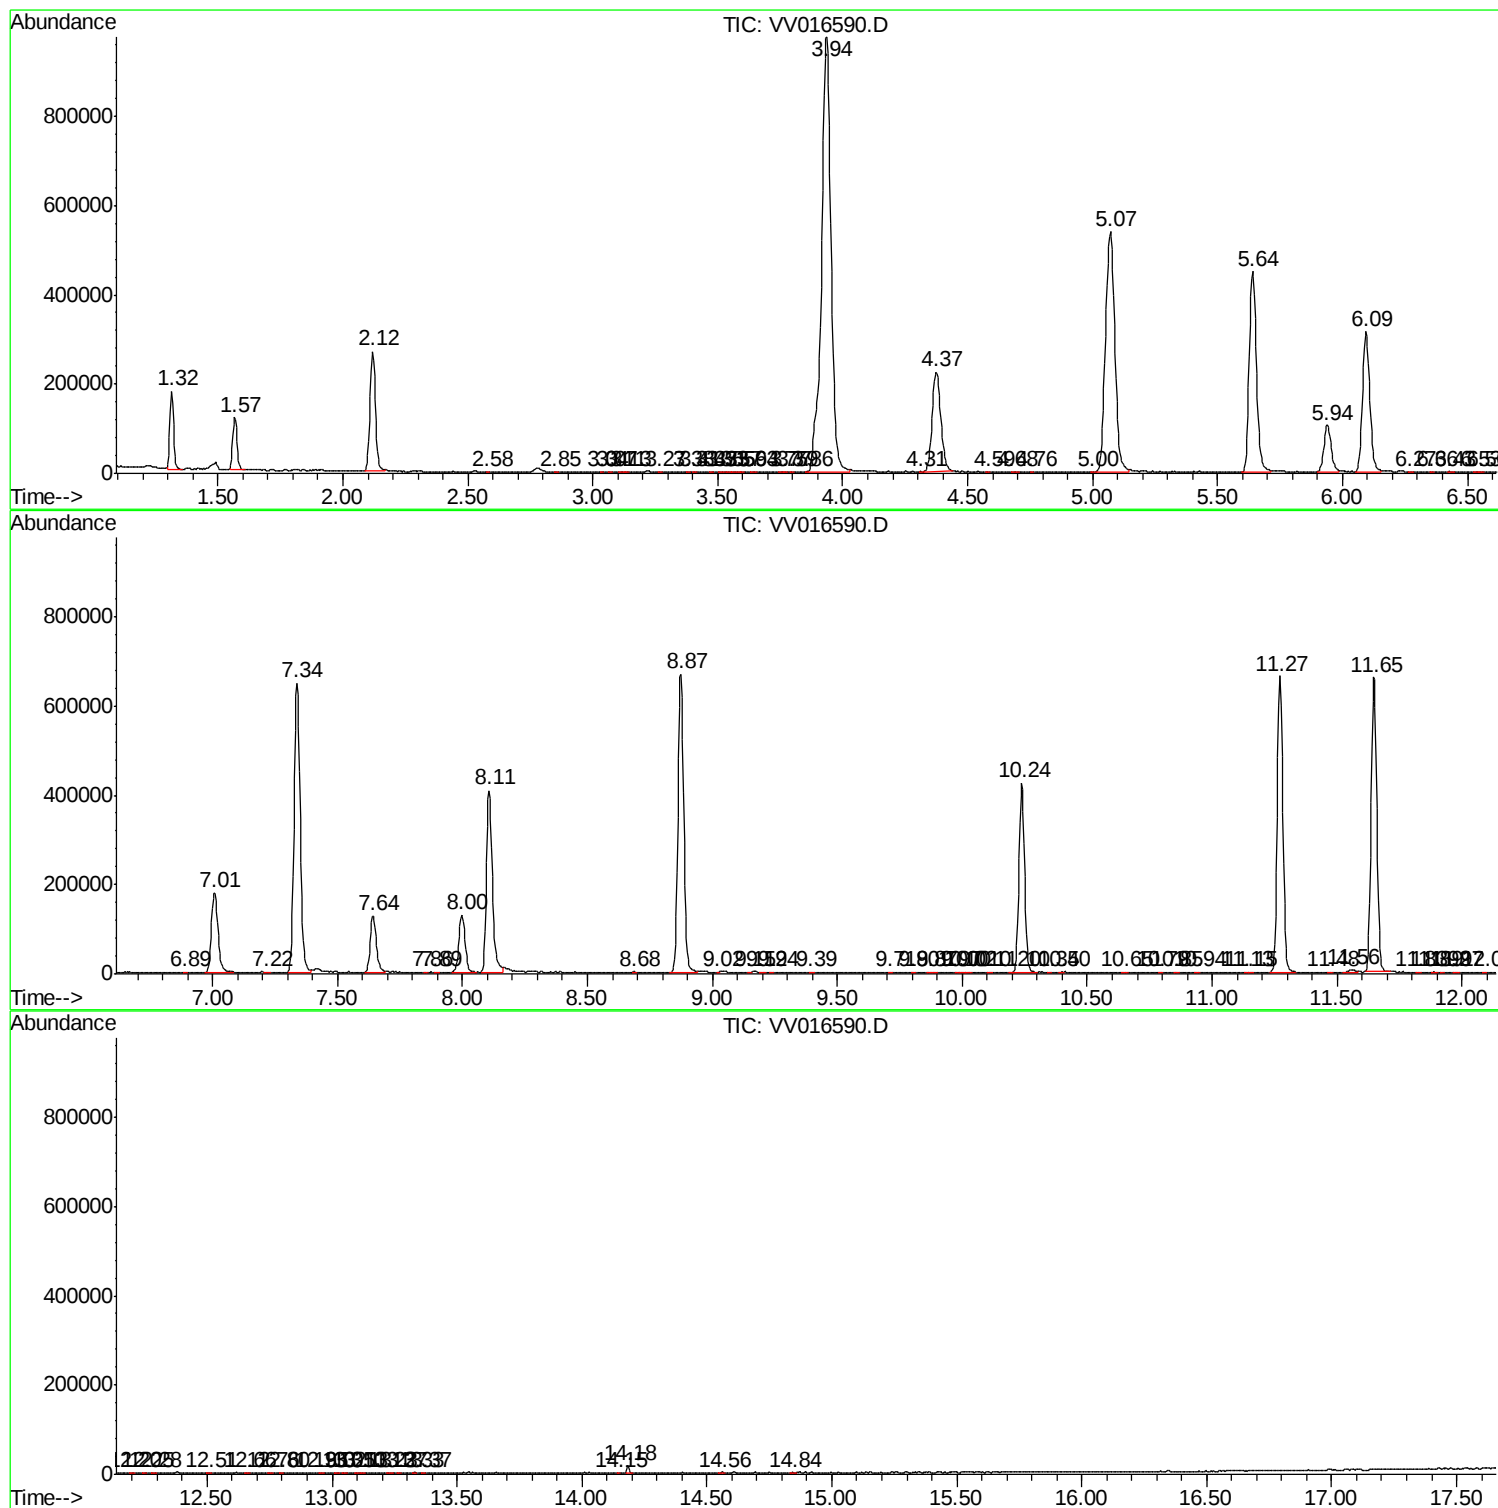

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016590.D
Acq On : 06 Jun 2020 15:16
Operator : SY/MD
Sample : L2895-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016590.D
Acq On : 06 Jun 2020 15:16
Operator : SY/MD
Sample : L2895-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc