

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016593.D
 Acq On : 06 Jun 2020 16:27
 Operator : SY/MD
 Sample : L2895-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB2	275068	291534	8.00%	1.944%
2	1.560	140	146	159	rVB	113197	135029	3.70%	0.900%
3	2.116	309	319	333	rBV	254496	385933	10.59%	2.574%
4	2.296	370	375	377	rBV5	2399	1911	0.05%	0.013%
5	2.373	397	399	403	rBV3	1064	879	0.02%	0.006%
6	2.672	489	492	493	rBV2	1163	699	0.02%	0.005%
7	2.711	502	504	506	rBV3	1738	939	0.03%	0.006%
8	2.778	516	525	539	rVB3	14091	24294	0.67%	0.162%
9	2.894	556	561	564	rBV4	1566	1525	0.04%	0.010%
10	2.949	576	578	580	rBV3	1290	703	0.02%	0.005%
11	3.109	623	628	631	rBV7	1707	1782	0.05%	0.012%
12	3.151	638	641	646	rVB6	1421	1194	0.03%	0.008%
13	3.376	706	711	715	rBV5	1647	1751	0.05%	0.012%
14	3.450	731	734	738	rVB4	1818	1054	0.03%	0.007%
15	3.470	738	740	742	rBV3	1094	592	0.02%	0.004%
16	3.521	753	756	757	rVV2	972	598	0.02%	0.004%
17	3.553	764	766	770	rVB4	1408	804	0.02%	0.005%
18	3.662	798	800	804	rBV4	1115	609	0.02%	0.004%
19	3.711	813	815	819	rVB3	1009	695	0.02%	0.005%
20	3.933	861	884	919	rBV2	1410682	3645678	100.00%	24.311%
21	4.373	1004	1021	1045	rBV	219198	537529	14.74%	3.585%
22	4.746	1134	1137	1143	rVB6	2345	1870	0.05%	0.012%
23	4.772	1143	1145	1147	rBV2	1733	863	0.02%	0.006%
24	4.839	1164	1166	1169	rVB2	1121	613	0.02%	0.004%
25	4.878	1175	1178	1181	rBV4	1140	653	0.02%	0.004%
26	5.071	1220	1238	1269	rVV2	519993	1358587	37.27%	9.060%
27	5.640	1402	1415	1437	rBV	455762	903981	24.80%	6.028%
28	5.836	1474	1476	1479	rVB3	1270	687	0.02%	0.005%
29	5.936	1494	1507	1528	rBV	424138	837200	22.96%	5.583%
30	6.093	1543	1556	1577	rBV	306834	612837	16.81%	4.087%
31	6.286	1614	1616	1618	rBV3	1201	582	0.02%	0.004%
32	6.469	1671	1673	1676	rBV4	923	675	0.02%	0.005%
33	6.534	1689	1693	1696	rBV3	962	845	0.02%	0.006%
34	6.556	1696	1700	1702	rBV4	1209	1048	0.03%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016593.D
 Acq On : 06 Jun 2020 16:27
 Operator : SY/MD
 Sample : L2895-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.617	1717	1719	1721	rBV3	1238	776	0.02%	0.005%
36	6.736	1754	1756	1760	rVB3	1100	591	0.02%	0.004%
37	6.756	1760	1762	1765	rBV3	871	587	0.02%	0.004%
38	7.006	1828	1840	1859	rBV	170820	307663	8.44%	2.052%
39	7.264	1915	1920	1923	rBV7	1232	1218	0.03%	0.008%
40	7.338	1931	1943	1959	rBV	632394	1071993	29.40%	7.149%
41	7.643	2023	2038	2055	rBV	122004	212617	5.83%	1.418%
42	7.852	2099	2103	2106	rBV5	1828	1666	0.05%	0.011%
43	7.894	2113	2116	2117	rBV3	1643	864	0.02%	0.006%
44	8.106	2172	2182	2218	rBV	407725	708603	19.44%	4.725%
45	8.601	2334	2336	2338	rBV2	1309	689	0.02%	0.005%
46	8.810	2398	2401	2406	rBV6	2184	2121	0.06%	0.014%
47	8.874	2409	2421	2440	rVV	690900	1108567	30.41%	7.392%
48	9.116	2491	2496	2497	rBV4	981	725	0.02%	0.005%
49	9.157	2503	2509	2510	rBV5	2430	1953	0.05%	0.013%
50	9.354	2568	2570	2572	rBV2	1623	842	0.02%	0.006%
51	9.485	2606	2611	2613	rBV6	1310	969	0.03%	0.006%
52	9.890	2734	2737	2744	rVB9	1415	1409	0.04%	0.009%
53	9.926	2744	2748	2751	rBV4	1493	1439	0.04%	0.010%
54	10.058	2782	2789	2790	rBV4	1395	1263	0.03%	0.008%
55	10.087	2794	2798	2801	rBV7	1652	1346	0.04%	0.009%
56	10.238	2832	2845	2864	rBV	416172	661171	18.14%	4.409%
57	10.444	2906	2909	2913	rBV5	1355	1131	0.03%	0.008%
58	10.524	2932	2934	2936	rBV3	1504	715	0.02%	0.005%
59	10.553	2938	2943	2945	rVV5	1656	1347	0.04%	0.009%
60	10.746	3000	3003	3005	rBV3	1021	759	0.02%	0.005%
61	10.878	3040	3044	3045	rBV3	931	660	0.02%	0.004%
62	10.910	3051	3054	3057	rBV5	1242	923	0.03%	0.006%
63	11.022	3087	3089	3092	rVB3	1061	594	0.02%	0.004%
64	11.042	3092	3095	3097	rVB4	1229	600	0.02%	0.004%
65	11.177	3134	3137	3138	rBV3	1196	596	0.02%	0.004%
66	11.270	3154	3166	3186	rBV	692851	1057851	29.02%	7.054%
67	11.405	3207	3208	3214	rVB5	1452	974	0.03%	0.006%
68	11.556	3249	3255	3266	rVB5	3238	6512	0.18%	0.043%
69	11.649	3271	3284	3302	rVV	667705	1047772	28.74%	6.987%
70	11.804	3329	3332	3334	rBV4	1698	1169	0.03%	0.008%
71	12.038	3403	3405	3407	rBV3	987	621	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016593.D
 Acq On : 06 Jun 2020 16:27
 Operator : SY/MD
 Sample : L2895-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.180	3446	3449	3451	rVB3	1553	990	0.03%	0.007%
73	12.199	3453	3455	3459	rBV5	803	622	0.02%	0.004%
74	12.222	3459	3462	3465	rBV4	1345	711	0.02%	0.005%
75	12.431	3523	3527	3529	rVB5	1694	1069	0.03%	0.007%
76	12.508	3547	3551	3552	rBV4	1157	694	0.02%	0.005%
77	12.517	3552	3554	3558	rVB5	1065	682	0.02%	0.005%
78	12.630	3586	3589	3591	rVV4	2003	1066	0.03%	0.007%
79	12.652	3591	3596	3597	rBV4	1009	808	0.02%	0.005%
80	12.736	3616	3622	3623	rBV4	1272	1061	0.03%	0.007%
81	12.752	3623	3627	3629	rBV3	918	666	0.02%	0.004%
82	12.852	3656	3658	3662	rBV5	899	856	0.02%	0.006%
83	12.932	3682	3683	3687	rVB2	1413	692	0.02%	0.005%
84	13.067	3721	3725	3727	rBV4	1235	941	0.03%	0.006%
85	13.157	3749	3753	3755	rBV5	1624	1066	0.03%	0.007%
86	13.263	3783	3786	3788	rBV5	1485	977	0.03%	0.007%
87	13.289	3791	3794	3798	rVV4	1181	880	0.02%	0.006%
88	13.623	3896	3898	3902	rVB3	1559	846	0.02%	0.006%
89	13.707	3921	3924	3925	rBV3	1572	773	0.02%	0.005%
90	13.820	3955	3959	3962	rBV5	1739	1535	0.04%	0.010%
91	13.836	3962	3964	3966	rBV3	1186	693	0.02%	0.005%
92	14.051	4029	4031	4036	rBV5	1134	833	0.02%	0.006%
93	14.074	4036	4038	4043	rVV6	1367	1243	0.03%	0.008%
94	14.151	4059	4062	4065	rBV4	1897	1508	0.04%	0.010%
95	14.218	4078	4083	4084	rBV5	1149	902	0.02%	0.006%
96	14.421	4144	4146	4150	rBV4	1500	782	0.02%	0.005%
97	14.546	4182	4185	4187	rBV3	1417	728	0.02%	0.005%
98	14.594	4196	4200	4206	rBV7	2151	2684	0.07%	0.018%
99	14.810	4264	4267	4269	rBV3	1595	955	0.03%	0.006%
100	14.894	4291	4293	4297	rBV5	1643	1123	0.03%	0.007%


Sum of corrected areas: 14995855

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016593.D
Acq On : 06 Jun 2020 16:27
Operator : SY/MD
Sample : L2895-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

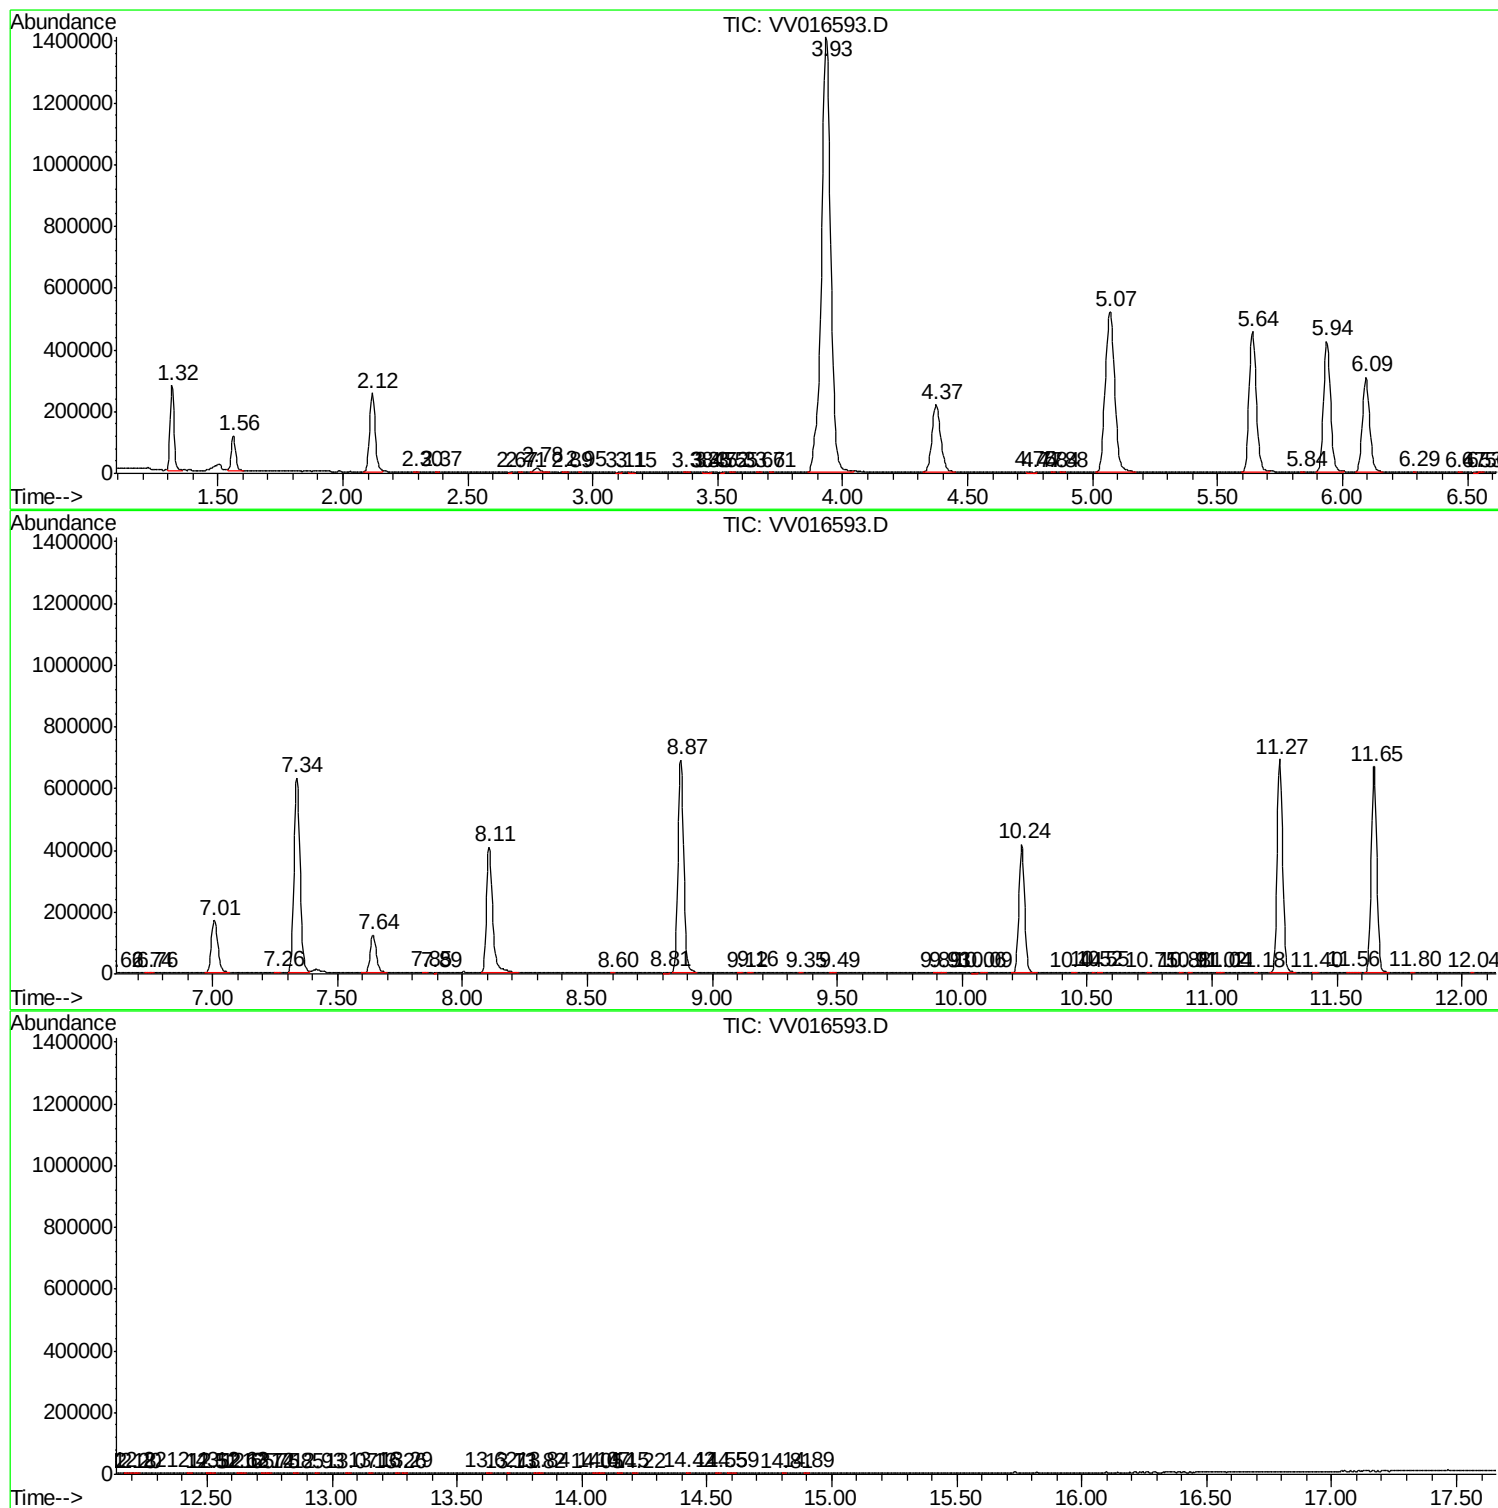

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016593.D
Acq On : 06 Jun 2020 16:27
Operator : SY/MD
Sample : L2895-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016593.D
Acq On : 06 Jun 2020 16:27
Operator : SY/MD
Sample : L2895-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc