

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016595.D
 Acq On : 06 Jun 2020 17:15
 Operator : SY/MD
 Sample : L2895-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	76	rBV	149352	141715	10.60%	1.358%
2	1.563	142	147	157	rVB	113517	130695	9.77%	1.253%
3	2.116	311	319	333	rVB	250809	366305	27.39%	3.511%
4	2.894	558	561	563	rBV3	1440	914	0.07%	0.009%
5	2.958	574	581	583	rBV6	1874	2253	0.17%	0.022%
6	3.048	607	609	615	rVB5	1561	1126	0.08%	0.011%
7	3.180	647	650	651	rBV3	865	549	0.04%	0.005%
8	3.286	680	683	687	rBV6	1451	1066	0.08%	0.010%
9	3.399	714	718	719	rBV3	938	595	0.04%	0.006%
10	3.608	780	783	785	rVB4	1225	631	0.05%	0.006%
11	3.627	785	789	791	rBV4	1659	1093	0.08%	0.010%
12	3.772	832	834	837	rVB3	905	495	0.04%	0.005%
13	3.836	850	854	857	rBV5	1303	870	0.07%	0.008%
14	3.894	861	872	902	rBV	110011	300851	22.49%	2.884%
15	4.257	983	985	988	rBV4	1109	782	0.06%	0.007%
16	4.373	1007	1021	1041	rBV	213700	514662	38.48%	4.933%
17	4.550	1074	1076	1081	rBV4	1463	1420	0.11%	0.014%
18	4.701	1121	1123	1126	rBV3	1191	885	0.07%	0.008%
19	4.762	1140	1142	1145	rVB3	1076	462	0.03%	0.004%
20	4.797	1150	1153	1154	rBV3	2037	1299	0.10%	0.012%
21	4.871	1174	1176	1177	rBV2	1864	875	0.07%	0.008%
22	5.071	1221	1238	1262	rBV2	523420	1337504	100.00%	12.819%
23	5.325	1312	1317	1318	rBV4	1833	1511	0.11%	0.014%
24	5.640	1403	1415	1439	rBV	445054	873139	65.28%	8.369%
25	5.814	1465	1469	1471	rBV5	1333	1244	0.09%	0.012%
26	5.939	1496	1508	1520	rBV5	6418	16733	1.25%	0.160%
27	6.093	1543	1556	1579	rBV	304771	613347	45.86%	5.879%
28	6.354	1632	1637	1640	rBV6	2383	2526	0.19%	0.024%
29	6.402	1650	1652	1658	rBV7	1418	1000	0.07%	0.010%
30	6.514	1683	1687	1688	rBV2	1995	1105	0.08%	0.011%
31	6.556	1698	1700	1703	rBV4	1066	487	0.04%	0.005%
32	6.836	1785	1787	1793	rBV7	1528	1080	0.08%	0.010%
33	7.006	1825	1840	1857	rBV	173649	308091	23.03%	2.953%
34	7.338	1931	1943	1960	rBV	626289	1062974	79.47%	10.188%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016595.D
 Acq On : 06 Jun 2020 17:15
 Operator : SY/MD
 Sample : L2895-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.640	2028	2037	2057	rBV	118022	203475	15.21%	1.950%
36	7.820	2089	2093	2097	rBV6	2109	1936	0.14%	0.019%
37	7.855	2100	2104	2107	rVB4	1290	923	0.07%	0.009%
38	7.939	2127	2130	2133	rBV5	1481	1408	0.11%	0.013%
39	7.990	2142	2146	2147	rBV3	2205	1404	0.10%	0.013%
40	8.035	2158	2160	2162	rVB3	1507	500	0.04%	0.005%
41	8.106	2171	2182	2214	rBV	402014	705687	52.76%	6.764%
42	8.646	2349	2350	2354	rVB4	1401	486	0.04%	0.005%
43	8.710	2369	2370	2372	rBV2	931	497	0.04%	0.005%
44	8.874	2409	2421	2436	rBV	662401	1071149	80.09%	10.267%
45	9.077	2482	2484	2486	rBV3	1385	469	0.04%	0.004%
46	9.386	2577	2580	2584	rBV4	1423	854	0.06%	0.008%
47	9.505	2615	2617	2619	rBV3	1063	657	0.05%	0.006%
48	9.630	2653	2656	2658	rBV4	1624	1193	0.09%	0.011%
49	9.688	2672	2674	2677	rBV3	819	583	0.04%	0.006%
50	9.817	2710	2714	2717	rBV4	1247	1169	0.09%	0.011%
51	9.961	2754	2759	2763	rBV8	1661	1731	0.13%	0.017%
52	10.019	2775	2777	2780	rBV3	1070	496	0.04%	0.005%
53	10.112	2804	2806	2809	rVB3	1405	668	0.05%	0.006%
54	10.238	2832	2845	2862	rBV	412047	651327	48.70%	6.243%
55	10.341	2875	2877	2879	rBV3	922	455	0.03%	0.004%
56	10.476	2916	2919	2921	rBV3	973	611	0.05%	0.006%
57	10.524	2931	2934	2935	rBV3	1056	597	0.04%	0.006%
58	10.685	2981	2984	2985	rBV3	1540	908	0.07%	0.009%
59	10.800	3016	3020	3021	rBV3	873	600	0.04%	0.006%
60	10.855	3036	3037	3040	rBV3	1286	633	0.05%	0.006%
61	11.022	3087	3089	3093	rBV5	1193	948	0.07%	0.009%
62	11.074	3101	3105	3106	rBV4	1003	722	0.05%	0.007%
63	11.096	3110	3112	3115	rBV4	1004	481	0.04%	0.005%
64	11.138	3122	3125	3126	rBV3	808	495	0.04%	0.005%
65	11.180	3134	3138	3140	rBV4	1667	1316	0.10%	0.013%
66	11.270	3154	3166	3186	rBV	662986	1029286	76.96%	9.865%
67	11.553	3246	3254	3255	rBV7	5752	5655	0.42%	0.054%
68	11.646	3272	3283	3301	rBV	664539	1027877	76.85%	9.852%
69	11.788	3324	3327	3328	rBV3	1146	677	0.05%	0.006%
70	12.048	3404	3408	3411	rBV4	2074	1732	0.13%	0.017%
71	12.161	3441	3443	3447	rVV5	1291	706	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016595.D
 Acq On : 06 Jun 2020 17:15
 Operator : SY/MD
 Sample : L2895-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.238	3465	3467	3472	rVB3	1743	1075	0.08%	0.010%
73	12.482	3540	3543	3545	rBV4	1592	1046	0.08%	0.010%
74	12.514	3550	3553	3555	rBV4	1186	598	0.04%	0.006%
75	12.546	3560	3563	3566	rVB5	1554	1108	0.08%	0.011%
76	12.669	3596	3601	3603	rBV5	1320	1318	0.10%	0.013%
77	12.720	3614	3617	3618	rBV3	1007	541	0.04%	0.005%
78	12.858	3657	3660	3661	rBV2	1563	1053	0.08%	0.010%
79	12.884	3664	3668	3670	rVV5	1137	770	0.06%	0.007%
80	12.894	3670	3671	3676	rVB5	827	544	0.04%	0.005%
81	12.923	3678	3680	3682	rVB3	1454	651	0.05%	0.006%
82	13.218	3771	3772	3775	rBV	1082	612	0.05%	0.006%
83	13.254	3781	3783	3786	rVB4	1173	473	0.04%	0.005%
84	13.270	3786	3788	3790	rBV3	861	480	0.04%	0.005%
85	13.324	3803	3805	3807	rBV3	1162	552	0.04%	0.005%
86	13.514	3861	3864	3866	rVB2	1146	591	0.04%	0.006%
87	13.527	3866	3868	3870	rBV3	1725	1072	0.08%	0.010%
88	13.585	3883	3886	3888	rBV3	1797	1124	0.08%	0.011%
89	13.685	3914	3917	3920	rBV4	1524	892	0.07%	0.009%
90	13.816	3956	3958	3961	rBV4	885	477	0.04%	0.005%
91	13.926	3989	3992	3993	rBV3	1623	829	0.06%	0.008%
92	13.984	4008	4010	4014	rBV4	865	460	0.03%	0.004%
93	14.093	4041	4044	4045	rBV2	948	542	0.04%	0.005%
94	14.151	4059	4062	4063	rBV3	1125	703	0.05%	0.007%
95	14.389	4134	4136	4140	rVB4	1955	1094	0.08%	0.010%
96	14.533	4179	4181	4183	rVB3	1273	458	0.03%	0.004%
97	14.733	4240	4243	4245	rBV3	1253	865	0.06%	0.008%
98	15.032	4334	4336	4337	rBV2	1232	528	0.04%	0.005%
99	15.061	4343	4345	4347	rBV3	1303	827	0.06%	0.008%
100	15.463	4468	4470	4475	rBV5	1775	1541	0.12%	0.015%


Sum of corrected areas: 10433419

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016595.D
Acq On : 06 Jun 2020 17:15
Operator : SY/MD
Sample : L2895-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

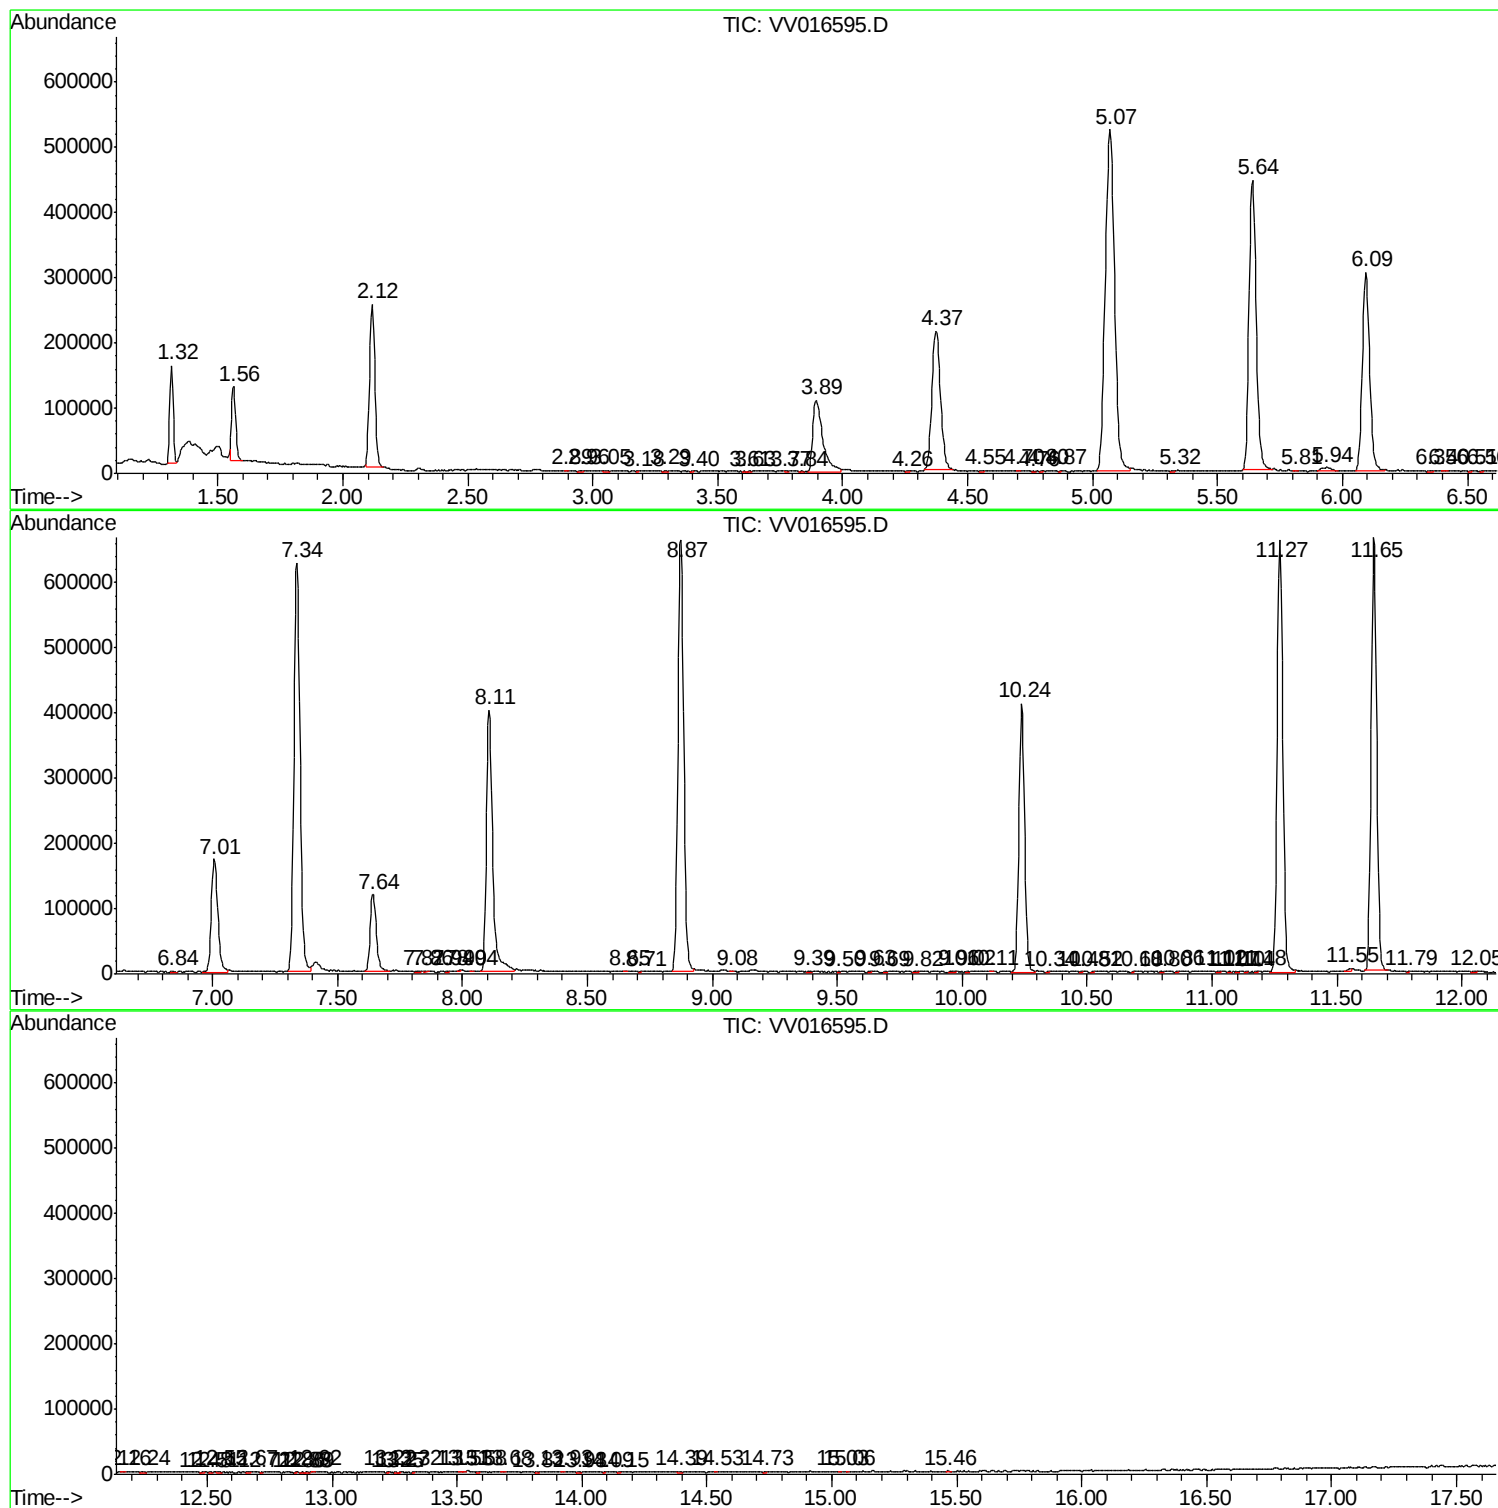

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016595.D
Acq On : 06 Jun 2020 17:15
Operator : SY/MD
Sample : L2895-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016595.D
Acq On : 06 Jun 2020 17:15
Operator : SY/MD
Sample : L2895-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc