

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016596.D
 Acq On : 06 Jun 2020 17:39
 Operator : SY/MD
 Sample : L2895-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB2	281066	294792	6.38%	1.959%
2	1.563	141	147	160	rVB	111911	132161	2.86%	0.878%
3	2.116	310	319	333	rBV	249064	375293	8.12%	2.494%
4	2.450	421	423	425	rBV3	1126	709	0.02%	0.005%
5	2.576	460	462	467	rVB4	1189	647	0.01%	0.004%
6	2.775	512	524	530	rBV4	9333	16641	0.36%	0.111%
7	2.846	543	546	550	rVB3	1863	1556	0.03%	0.010%
8	3.155	639	642	645	rBV4	1709	1189	0.03%	0.008%
9	3.267	674	677	680	rVB5	1221	722	0.02%	0.005%
10	3.290	680	684	687	rVB5	1223	1020	0.02%	0.007%
11	3.322	692	694	697	rVB4	1541	713	0.02%	0.005%
12	3.338	697	699	702	rBV3	1304	915	0.02%	0.006%
13	3.544	761	763	765	rVB3	1167	547	0.01%	0.004%
14	3.579	771	774	776	rBV3	1278	731	0.02%	0.005%
15	3.653	794	797	798	rBV3	1831	922	0.02%	0.006%
16	3.711	812	815	816	rBV3	1578	689	0.01%	0.005%
17	3.756	826	829	833	rBV6	1074	1097	0.02%	0.007%
18	3.788	834	839	841	rBV5	1125	1148	0.02%	0.008%
19	3.843	854	856	860	rBV4	873	628	0.01%	0.004%
20	3.933	862	884	916	rBV2	1819619	4621919	100.00%	30.717%
21	4.373	1003	1021	1043	rBV2	217549	531751	11.50%	3.534%
22	4.534	1069	1071	1073	rBV3	1206	710	0.02%	0.005%
23	4.576	1078	1084	1086	rBV7	1648	1775	0.04%	0.012%
24	4.733	1130	1133	1137	rBV5	1950	1172	0.03%	0.008%
25	4.830	1159	1163	1168	rBV7	901	794	0.02%	0.005%
26	5.068	1220	1237	1268	rBV2	522568	1357151	29.36%	9.020%
27	5.492	1364	1369	1372	rBV7	1431	1435	0.03%	0.010%
28	5.508	1372	1374	1376	rBV3	1066	681	0.01%	0.005%
29	5.640	1403	1415	1444	rVB	446180	882819	19.10%	5.867%
30	5.939	1497	1508	1516	rBV	7889	18462	0.40%	0.123%
31	6.093	1539	1556	1578	rBV	310678	622883	13.48%	4.140%
32	6.421	1656	1658	1664	rVB6	1779	1366	0.03%	0.009%
33	6.470	1671	1673	1674	rBV2	1005	531	0.01%	0.004%
34	7.007	1826	1840	1858	rBV	169663	308936	6.68%	2.053%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016596.D
 Acq On : 06 Jun 2020 17:39
 Operator : SY/MD
 Sample : L2895-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.338	1929	1943	1960	rBV	622290	1061653	22.97%	7.056%
36	7.643	2028	2038	2051	rBV	118459	200803	4.34%	1.335%
37	7.756	2071	2073	2077	rBV4	2227	1466	0.03%	0.010%
38	7.926	2124	2126	2130	rBV5	1330	944	0.02%	0.006%
39	8.055	2164	2166	2168	rBV2	1147	596	0.01%	0.004%
40	8.106	2172	2182	2215	rBV	402781	710620	15.37%	4.723%
41	8.502	2303	2305	2308	rVB4	1633	883	0.02%	0.006%
42	8.527	2312	2313	2318	rVB4	929	632	0.01%	0.004%
43	8.621	2339	2342	2345	rBV3	1544	1324	0.03%	0.009%
44	8.752	2381	2383	2387	rBV4	1626	1095	0.02%	0.007%
45	8.778	2387	2391	2397	rVB8	1206	1068	0.02%	0.007%
46	8.810	2397	2401	2402	rBV3	879	645	0.01%	0.004%
47	8.871	2407	2420	2441	rBV	664149	1079669	23.36%	7.175%
48	9.103	2488	2492	2498	rVB7	2065	2308	0.05%	0.015%
49	9.264	2540	2542	2545	rBV4	1357	719	0.02%	0.005%
50	9.370	2572	2575	2579	rBV5	1124	771	0.02%	0.005%
51	9.441	2595	2597	2599	rBV3	1404	698	0.02%	0.005%
52	9.498	2612	2615	2619	rBV6	1233	1069	0.02%	0.007%
53	9.518	2619	2621	2624	rBV4	973	658	0.01%	0.004%
54	9.563	2633	2635	2636	rBV2	1610	709	0.02%	0.005%
55	9.624	2648	2654	2657	rBV7	1346	1421	0.03%	0.009%
56	9.695	2673	2676	2679	rBV2	846	638	0.01%	0.004%
57	9.749	2689	2693	2696	rBV5	1144	821	0.02%	0.005%
58	9.965	2756	2760	2763	rBV5	1701	1505	0.03%	0.010%
59	10.077	2791	2795	2798	rBV4	925	624	0.01%	0.004%
60	10.096	2798	2801	2803	rBV3	1040	607	0.01%	0.004%
61	10.109	2803	2805	2811	rVB6	1313	1353	0.03%	0.009%
62	10.193	2828	2831	2833	rBV4	1486	1004	0.02%	0.007%
63	10.238	2833	2845	2867	rVV	428365	664394	14.37%	4.416%
64	10.334	2871	2875	2878	rBV5	1429	1086	0.02%	0.007%
65	10.354	2878	2881	2884	rVB4	1259	942	0.02%	0.006%
66	10.508	2925	2929	2931	rBV4	1453	1111	0.02%	0.007%
67	10.595	2952	2956	2958	rBV4	1438	1208	0.03%	0.008%
68	10.707	2989	2991	2995	rBV4	982	665	0.01%	0.004%
69	10.730	2995	2998	3001	rBV5	1391	826	0.02%	0.005%
70	11.113	3115	3117	3123	rVB6	1341	982	0.02%	0.007%
71	11.174	3133	3136	3138	rBV3	1001	655	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016596.D
 Acq On : 06 Jun 2020 17:39
 Operator : SY/MD
 Sample : L2895-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3183	rBV	677145	1042280	22.55%	6.927%
73	11.479	3227	3231	3234	rBV4	1116	1040	0.02%	0.007%
74	11.518	3240	3243	3244	rBV3	1097	624	0.01%	0.004%
75	11.556	3247	3255	3264	rVV3	11013	19851	0.43%	0.132%
76	11.646	3272	3283	3298	rBV	664552	1028832	22.26%	6.838%
77	12.000	3388	3393	3395	rBV5	1375	1208	0.03%	0.008%
78	12.138	3433	3436	3439	rBV5	1297	945	0.02%	0.006%
79	12.257	3471	3473	3474	rBV	1306	571	0.01%	0.004%
80	12.321	3490	3493	3495	rBV4	921	620	0.01%	0.004%
81	12.360	3502	3505	3506	rBV3	1716	841	0.02%	0.006%
82	12.595	3576	3578	3580	rBV3	1132	601	0.01%	0.004%
83	12.714	3614	3615	3619	rVB3	2120	1139	0.02%	0.008%
84	12.733	3619	3621	3623	rBV3	1532	1041	0.02%	0.007%
85	12.804	3642	3643	3646	rBV3	898	546	0.01%	0.004%
86	12.913	3675	3677	3680	rVB3	1526	608	0.01%	0.004%
87	13.045	3716	3718	3719	rBV2	1293	619	0.01%	0.004%
88	13.138	3743	3747	3748	rBV3	1213	931	0.02%	0.006%
89	13.167	3753	3756	3760	rVV4	1289	1203	0.03%	0.008%
90	13.186	3760	3762	3768	rVB7	1311	1196	0.03%	0.008%
91	13.611	3891	3894	3898	rVB4	1798	1194	0.03%	0.008%
92	13.926	3989	3992	3993	rBV3	830	549	0.01%	0.004%
93	13.981	4006	4009	4011	rVV3	1256	788	0.02%	0.005%
94	14.058	4031	4033	4034	rBV	1273	558	0.01%	0.004%
95	14.109	4045	4049	4051	rBV3	1472	1206	0.03%	0.008%
96	14.209	4077	4080	4082	rBV3	1770	1049	0.02%	0.007%
97	14.382	4132	4134	4136	rBV2	1194	534	0.01%	0.004%
98	14.444	4150	4153	4155	rBV3	1681	841	0.02%	0.006%
99	14.495	4167	4169	4172	rBV3	1289	947	0.02%	0.006%
100	15.122	4360	4364	4368	rBV7	1760	1650	0.04%	0.011%


Sum of corrected areas: 15046689

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016596.D
Acq On : 06 Jun 2020 17:39
Operator : SY/MD
Sample : L2895-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

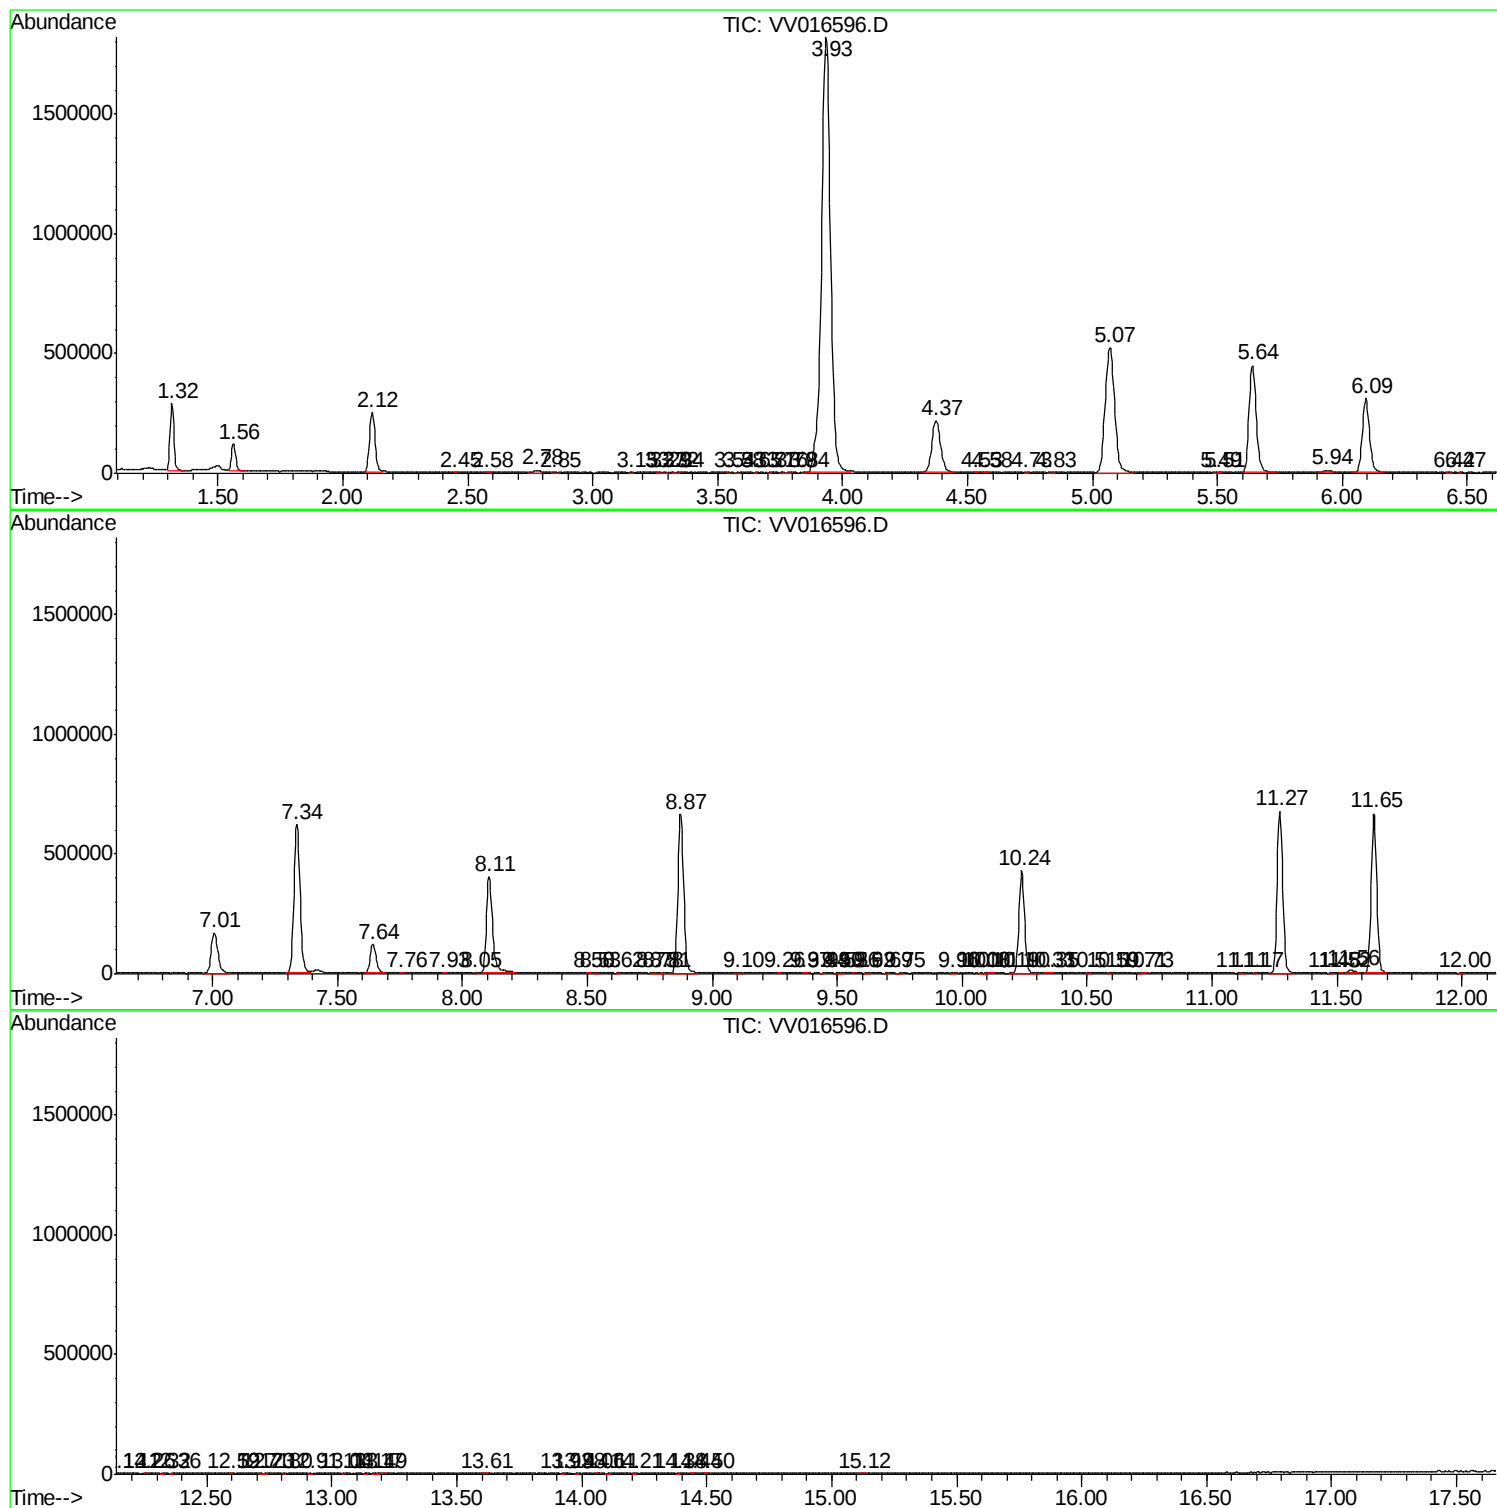

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016596.D
Acq On : 06 Jun 2020 17:39
Operator : SY/MD
Sample : L2895-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016596.D
Acq On : 06 Jun 2020 17:39
Operator : SY/MD
Sample : L2895-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc