

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016597.D
 Acq On : 06 Jun 2020 18:03
 Operator : SY/MD
 Sample : L2895-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB2	277435	291732	6.30%	1.957%
2	1.560	140	146	157	rVB	110028	129429	2.80%	0.868%
3	2.116	310	319	333	rVB	251768	374624	8.09%	2.512%
4	2.431	411	417	420	rBV8	1553	1513	0.03%	0.010%
5	2.453	420	424	426	rVV4	1492	1084	0.02%	0.007%
6	2.470	426	429	433	rVB5	1451	1140	0.02%	0.008%
7	2.598	465	469	471	rBV5	1402	1134	0.02%	0.008%
8	2.704	500	502	505	rVB4	1380	713	0.02%	0.005%
9	2.775	514	524	536	rBV3	9752	18301	0.40%	0.123%
10	2.855	545	549	550	rBV2	1358	839	0.02%	0.006%
11	2.978	583	587	588	rBV4	1488	835	0.02%	0.006%
12	3.177	643	649	651	rBV6	1968	2087	0.05%	0.014%
13	3.306	685	689	693	rBV4	833	675	0.01%	0.005%
14	3.470	737	740	743	rVB5	1620	996	0.02%	0.007%
15	3.495	743	748	751	rBV6	1429	1406	0.03%	0.009%
16	3.563	764	769	771	rBV3	833	783	0.02%	0.005%
17	3.582	771	775	776	rBV4	1072	648	0.01%	0.004%
18	3.653	793	797	801	rBV7	1014	735	0.02%	0.005%
19	3.933	862	884	916	rBV2	1822339	4630596	100.00%	31.056%
20	4.373	1004	1021	1045	rBV	214835	529161	11.43%	3.549%
21	4.650	1105	1107	1109	rBV3	1361	764	0.02%	0.005%
22	4.698	1118	1122	1123	rBV4	1502	1079	0.02%	0.007%
23	4.868	1173	1175	1180	rBV3	1166	965	0.02%	0.006%
24	4.900	1183	1185	1189	rVB3	1254	752	0.02%	0.005%
25	4.936	1193	1196	1200	rVB4	1172	768	0.02%	0.005%
26	5.071	1220	1238	1267	rBV2	513233	1342480	28.99%	9.003%
27	5.486	1364	1367	1370	rVB5	1625	1112	0.02%	0.007%
28	5.514	1372	1376	1377	rBV3	1215	906	0.02%	0.006%
29	5.595	1397	1401	1402	rBV3	1991	1199	0.03%	0.008%
30	5.640	1402	1415	1437	rVV	442332	872309	18.84%	5.850%
31	6.093	1542	1556	1575	rBV	302812	613231	13.24%	4.113%
32	6.315	1622	1625	1629	rVB5	1899	1274	0.03%	0.009%
33	6.363	1638	1640	1648	rVB8	1157	872	0.02%	0.006%
34	6.521	1684	1689	1690	rBV3	937	735	0.02%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016597.D
 Acq On : 06 Jun 2020 18:03
 Operator : SY/MD
 Sample : L2895-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.585	1706	1709	1711	rBV3	1187	850	0.02%	0.006%
36	6.868	1793	1797	1799	rBV4	995	880	0.02%	0.006%
37	7.006	1829	1840	1857	rBV	170577	304301	6.57%	2.041%
38	7.338	1931	1943	1959	rBV	619240	1050191	22.68%	7.043%
39	7.524	1999	2001	2003	rBV2	1088	640	0.01%	0.004%
40	7.640	2028	2037	2052	rBV	117757	200112	4.32%	1.342%
41	7.762	2071	2075	2080	rBV6	2289	2381	0.05%	0.016%
42	7.920	2121	2124	2127	rVB4	1484	965	0.02%	0.006%
43	7.997	2146	2148	2151	rBV4	1872	1121	0.02%	0.008%
44	8.106	2171	2182	2208	rBV	406550	704757	15.22%	4.727%
45	8.524	2310	2312	2318	rBV6	874	621	0.01%	0.004%
46	8.617	2339	2341	2344	rBV4	1410	805	0.02%	0.005%
47	8.871	2410	2420	2439	rBV	649994	1049662	22.67%	7.040%
48	9.170	2504	2513	2521	rBV	3664	5656	0.12%	0.038%
49	9.267	2538	2543	2547	rBV7	1023	1271	0.03%	0.009%
50	9.360	2566	2572	2576	rBV5	2120	2696	0.06%	0.018%
51	9.418	2588	2590	2592	rVB3	1628	653	0.01%	0.004%
52	9.434	2592	2595	2596	rBV3	1220	605	0.01%	0.004%
53	9.469	2601	2606	2607	rBV3	1296	1019	0.02%	0.007%
54	9.518	2618	2621	2623	rBV3	1399	964	0.02%	0.006%
55	9.633	2653	2657	2659	rBV3	1491	988	0.02%	0.007%
56	9.672	2666	2669	2672	rBV4	1354	906	0.02%	0.006%
57	9.804	2707	2710	2715	rVB6	1229	888	0.02%	0.006%
58	10.016	2774	2776	2780	rVB4	1508	899	0.02%	0.006%
59	10.099	2798	2802	2804	rBV5	1181	930	0.02%	0.006%
60	10.116	2804	2807	2809	rVV4	1763	1242	0.03%	0.008%
61	10.238	2832	2845	2863	rBV	417681	655752	14.16%	4.398%
62	10.463	2913	2915	2918	rVB3	1581	802	0.02%	0.005%
63	10.482	2918	2921	2924	rBV4	1128	888	0.02%	0.006%
64	10.643	2968	2971	2975	rBV4	923	751	0.02%	0.005%
65	10.788	3013	3016	3019	rBV5	1207	691	0.01%	0.005%
66	10.884	3044	3046	3052	rVB5	1407	1085	0.02%	0.007%
67	10.935	3057	3062	3069	rBV8	2243	2735	0.06%	0.018%
68	11.067	3101	3103	3106	rVB3	1266	647	0.01%	0.004%
69	11.161	3128	3132	3133	rBV3	1428	957	0.02%	0.006%
70	11.209	3145	3147	3152	rBV6	1212	1006	0.02%	0.007%
71	11.270	3155	3166	3181	rVV	663497	1012368	21.86%	6.790%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016597.D
 Acq On : 06 Jun 2020 18:03
 Operator : SY/MD
 Sample : L2895-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.472	3225	3229	3232	rBV6	1127	903	0.02%	0.006%
73	11.514	3239	3242	3246	rBV3	1398	1052	0.02%	0.007%
74	11.559	3249	3256	3261	rBV9	2741	4376	0.09%	0.029%
75	11.646	3269	3283	3301	rBV	670309	1036701	22.39%	6.953%
76	12.099	3419	3424	3431	rBV8	1679	2237	0.05%	0.015%
77	12.160	3441	3443	3447	rVB4	1896	1156	0.02%	0.008%
78	12.334	3494	3497	3500	rBV4	1748	930	0.02%	0.006%
79	12.421	3520	3524	3525	rBV3	1179	804	0.02%	0.005%
80	12.463	3534	3537	3542	rBV6	1416	1365	0.03%	0.009%
81	12.762	3626	3630	3631	rBV3	1149	787	0.02%	0.005%
82	12.816	3645	3647	3652	rVB5	1485	910	0.02%	0.006%
83	12.836	3652	3653	3658	rVB4	1346	990	0.02%	0.007%
84	12.878	3664	3666	3668	rBV3	1005	667	0.01%	0.004%
85	13.019	3706	3710	3712	rBV4	1270	788	0.02%	0.005%
86	13.038	3712	3716	3720	rVV5	1384	1332	0.03%	0.009%
87	13.086	3728	3731	3733	rBV3	988	699	0.02%	0.005%
88	13.215	3766	3771	3772	rBV3	1276	1045	0.02%	0.007%
89	13.250	3779	3782	3785	rBV5	1010	683	0.01%	0.005%
90	13.414	3830	3833	3835	rBV4	1408	854	0.02%	0.006%
91	13.607	3891	3893	3900	rVB5	1829	1772	0.04%	0.012%
92	13.649	3900	3906	3908	rBV6	1457	1562	0.03%	0.010%
93	13.900	3980	3984	3986	rBV5	1566	1195	0.03%	0.008%
94	14.058	4032	4033	4036	rBV3	1144	661	0.01%	0.004%
95	14.254	4090	4094	4095	rBV3	1590	914	0.02%	0.006%
96	14.382	4131	4134	4138	rBV6	1768	1394	0.03%	0.009%
97	14.434	4147	4150	4153	rBV4	1634	1379	0.03%	0.009%
98	14.675	4221	4225	4226	rBV2	1594	1184	0.03%	0.008%
99	14.746	4245	4247	4252	rBV6	1501	1013	0.02%	0.007%
100	14.932	4303	4305	4307	rBV3	1433	794	0.02%	0.005%


Sum of corrected areas: 14910709

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016597.D
Acq On : 06 Jun 2020 18:03
Operator : SY/MD
Sample : L2895-18
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

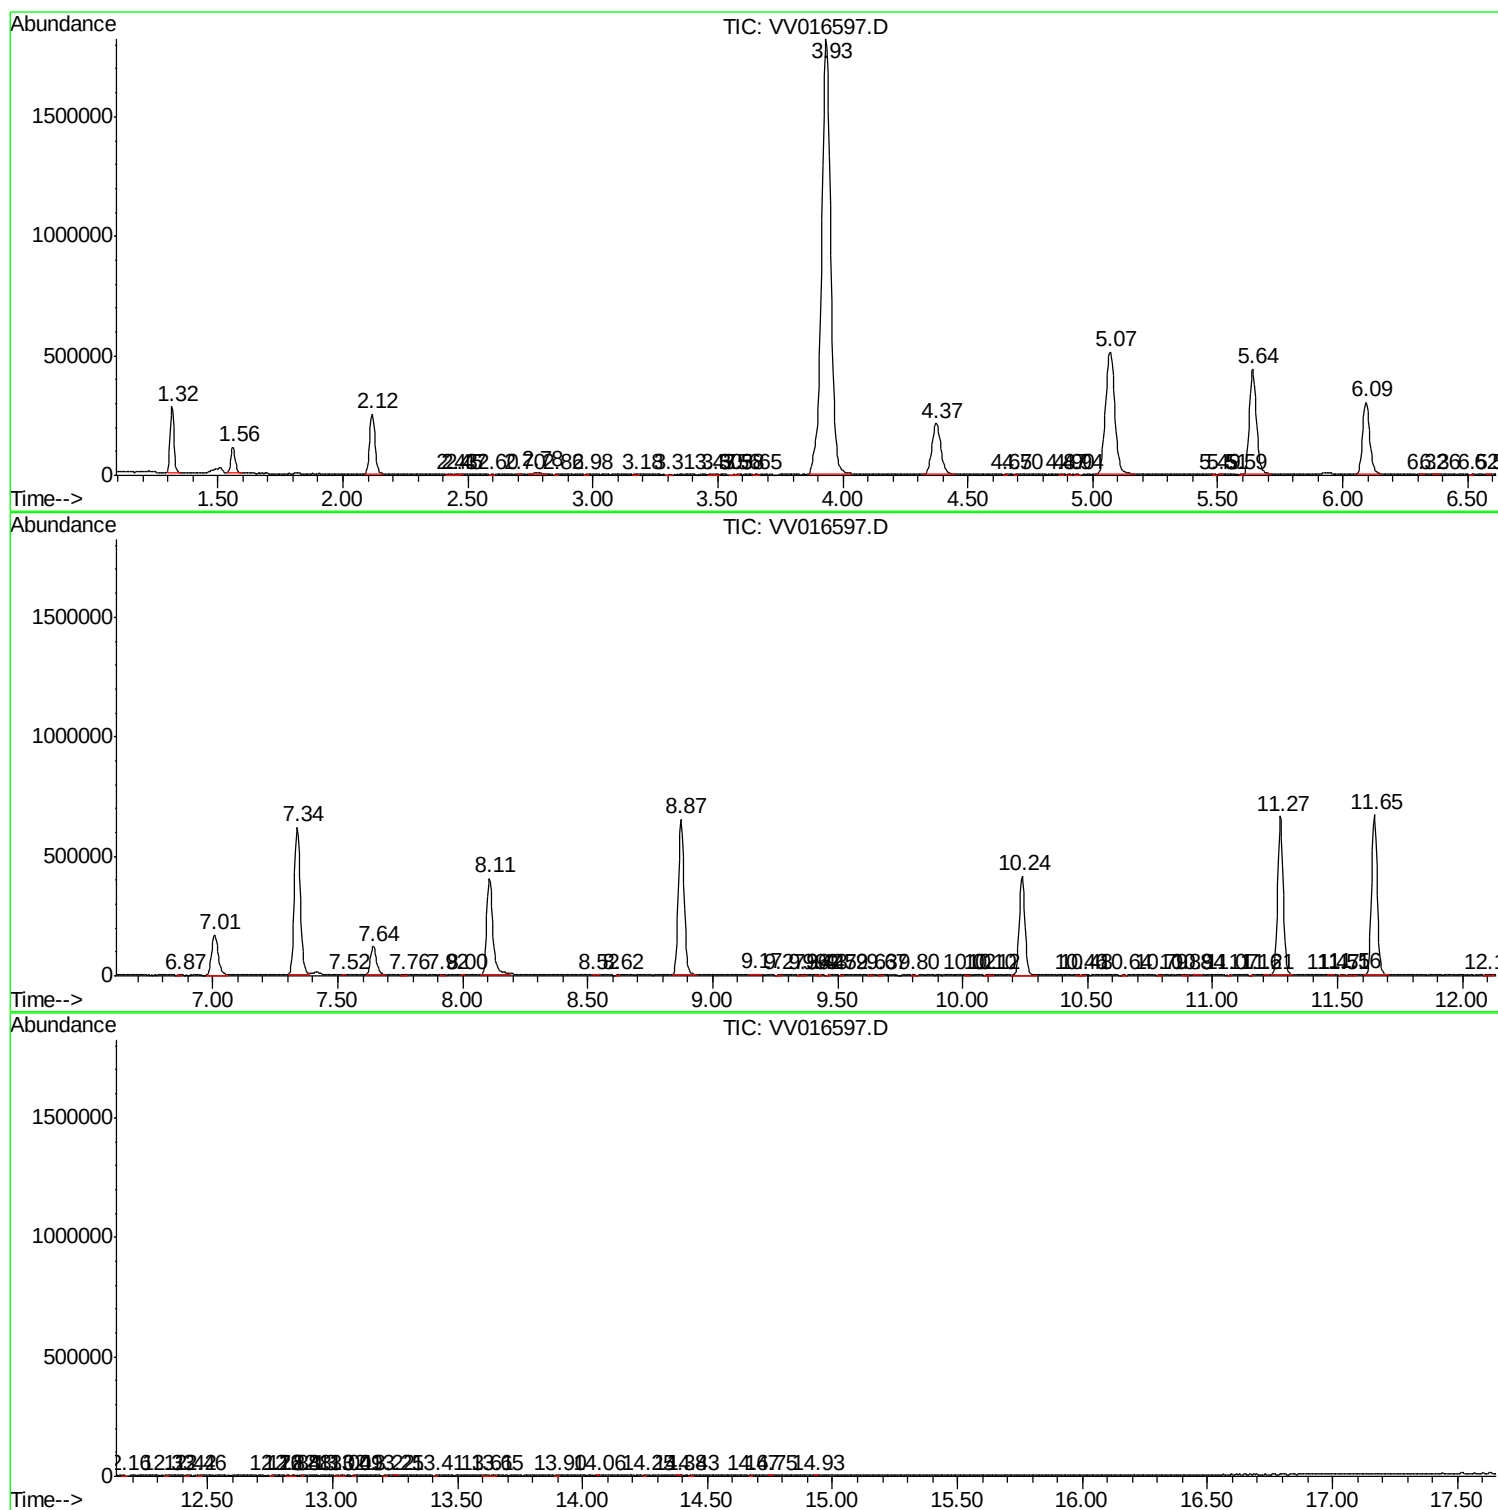

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016597.D
Acq On : 06 Jun 2020 18:03
Operator : SY/MD
Sample : L2895-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016597.D
Acq On : 06 Jun 2020 18:03
Operator : SY/MD
Sample : L2895-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc