

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016599.D
 Acq On : 06 Jun 2020 18:50
 Operator : SY/MD
 Sample : L2895-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB2	272581	288142	15.62%	2.288%
2	1.560	140	146	158	rVB	106474	122896	6.66%	0.976%
3	2.116	310	319	334	rBV	240363	356854	19.34%	2.834%
4	2.389	403	404	405	rBV	1259	435	0.02%	0.003%
5	2.888	557	559	561	rBV3	1265	575	0.03%	0.005%
6	2.923	568	570	573	rBV4	1218	797	0.04%	0.006%
7	3.110	625	628	634	rBV6	1351	1104	0.06%	0.009%
8	3.370	707	709	711	rBV3	1256	594	0.03%	0.005%
9	3.476	738	742	743	rBV3	1364	841	0.05%	0.007%
10	3.528	756	758	762	rVB3	1726	969	0.05%	0.008%
11	3.560	767	768	772	rVV3	1068	518	0.03%	0.004%
12	3.711	813	815	820	rVB6	763	446	0.02%	0.004%
13	3.827	849	851	854	rVB4	1090	455	0.02%	0.004%
14	3.856	856	860	861	rBV3	1056	679	0.04%	0.005%
15	3.933	862	884	913	rBV2	659325	1844945	100.00%	14.652%
16	4.373	1004	1021	1045	rBV	210627	516873	28.02%	4.105%
17	4.595	1086	1090	1091	rBV5	1134	794	0.04%	0.006%
18	4.724	1128	1130	1135	rBV4	1130	1010	0.05%	0.008%
19	4.827	1160	1162	1165	rBV3	1240	626	0.03%	0.005%
20	4.949	1199	1200	1202	rBV2	991	430	0.02%	0.003%
21	5.071	1221	1238	1263	rBV2	504759	1307333	70.86%	10.383%
22	5.566	1388	1392	1396	rVB6	940	783	0.04%	0.006%
23	5.589	1396	1399	1401	rBV3	1225	587	0.03%	0.005%
24	5.640	1401	1415	1434	rBV	418396	826033	44.77%	6.560%
25	5.875	1485	1488	1490	rBV4	1091	657	0.04%	0.005%
26	5.939	1499	1508	1526	rVB2	60264	119701	6.49%	0.951%
27	6.093	1543	1556	1579	rBV	293449	595495	32.28%	4.729%
28	6.296	1617	1619	1622	rBV3	1247	708	0.04%	0.006%
29	6.418	1656	1657	1660	rBV3	791	421	0.02%	0.003%
30	6.434	1660	1662	1663	rBV2	1049	424	0.02%	0.003%
31	6.463	1668	1671	1674	rVV5	1536	1058	0.06%	0.008%
32	6.492	1678	1680	1682	rBV3	1062	551	0.03%	0.004%
33	6.576	1703	1706	1709	rVB3	1191	595	0.03%	0.005%
34	6.611	1713	1717	1721	rVB6	1562	1165	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016599.D
 Acq On : 06 Jun 2020 18:50
 Operator : SY/MD
 Sample : L2895-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.630	1721	1723	1725	rBV3	1740	1111	0.06%	0.009%
36	6.852	1785	1792	1794	rBV8	1340	1678	0.09%	0.013%
37	6.936	1814	1818	1820	rBV3	860	622	0.03%	0.005%
38	7.007	1829	1840	1858	rBV	163058	290403	15.74%	2.306%
39	7.270	1918	1922	1927	rVB6	1559	1426	0.08%	0.011%
40	7.338	1931	1943	1960	rBV	605836	1030639	55.86%	8.185%
41	7.640	2025	2037	2059	rBV2	116509	203996	11.06%	1.620%
42	7.997	2137	2148	2164	rVB	421285	687471	37.26%	5.460%
43	8.106	2173	2182	2211	rBV	393086	664661	36.03%	5.279%
44	8.418	2277	2279	2282	rBV4	1182	704	0.04%	0.006%
45	8.640	2346	2348	2349	rBV2	1384	574	0.03%	0.005%
46	8.675	2356	2359	2360	rBV3	1388	824	0.04%	0.007%
47	8.775	2388	2390	2393	rVB4	1563	902	0.05%	0.007%
48	8.804	2393	2399	2400	rBV4	1449	1228	0.07%	0.010%
49	8.871	2408	2420	2440	rBV	627237	1015168	55.02%	8.062%
50	9.090	2486	2488	2490	rBV3	1091	474	0.03%	0.004%
51	9.254	2535	2539	2542	rVB5	1803	1302	0.07%	0.010%
52	9.273	2542	2545	2546	rBV3	1166	740	0.04%	0.006%
53	9.383	2575	2579	2580	rBV2	1690	1005	0.05%	0.008%
54	9.473	2605	2607	2610	rBV3	1765	1012	0.05%	0.008%
55	9.511	2616	2619	2620	rBV3	868	422	0.02%	0.003%
56	9.820	2713	2715	2718	rBV4	743	434	0.02%	0.003%
57	9.852	2721	2725	2729	rBV7	1561	1571	0.09%	0.012%
58	10.055	2785	2788	2791	rBV4	1117	871	0.05%	0.007%
59	10.087	2796	2798	2799	rBV2	1276	448	0.02%	0.004%
60	10.119	2806	2808	2814	rVB6	1564	1201	0.07%	0.010%
61	10.161	2819	2821	2823	rVB3	1540	628	0.03%	0.005%
62	10.238	2833	2845	2862	rBV	407152	636840	34.52%	5.058%
63	10.383	2887	2890	2891	rBV3	1013	549	0.03%	0.004%
64	10.444	2906	2909	2911	rBV2	2042	1408	0.08%	0.011%
65	10.688	2978	2985	2987	rBV6	1935	1858	0.10%	0.015%
66	10.781	3012	3014	3018	rBV4	1871	1161	0.06%	0.009%
67	10.852	3034	3036	3037	rBV2	1248	562	0.03%	0.004%
68	10.993	3078	3080	3082	rBV3	1389	784	0.04%	0.006%
69	11.042	3093	3095	3097	rBV3	1299	610	0.03%	0.005%
70	11.087	3107	3109	3113	rVB4	1263	926	0.05%	0.007%
71	11.106	3113	3115	3116	rBV2	1073	486	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016599.D
 Acq On : 06 Jun 2020 18:50
 Operator : SY/MD
 Sample : L2895-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3184	rBV	638880	984032	53.34%	7.815%
73	11.473	3227	3229	3230	rBV	1215	544	0.03%	0.004%
74	11.502	3236	3238	3241	rBV4	1347	794	0.04%	0.006%
75	11.556	3247	3255	3265	rBV8	9163	17664	0.96%	0.140%
76	11.646	3271	3283	3304	rBV	652702	1012808	54.90%	8.044%
77	11.913	3363	3366	3370	rBV5	1160	1002	0.05%	0.008%
78	12.180	3444	3449	3450	rBV4	1036	926	0.05%	0.007%
79	12.360	3503	3505	3509	rBV4	1075	905	0.05%	0.007%
80	12.456	3533	3535	3537	rBV3	1118	491	0.03%	0.004%
81	12.498	3545	3548	3553	rBV6	1352	1381	0.07%	0.011%
82	12.659	3595	3598	3600	rBV4	1201	961	0.05%	0.008%
83	12.768	3628	3632	3634	rVB4	1189	927	0.05%	0.007%
84	12.784	3634	3637	3638	rBV4	1463	684	0.04%	0.005%
85	12.823	3644	3649	3650	rBV4	1753	1363	0.07%	0.011%
86	12.932	3681	3683	3687	rBV4	831	709	0.04%	0.006%
87	12.993	3699	3702	3703	rBV3	1116	488	0.03%	0.004%
88	13.093	3730	3733	3734	rBV3	1400	625	0.03%	0.005%
89	13.154	3748	3752	3755	rBV6	1330	1129	0.06%	0.009%
90	13.260	3783	3785	3788	rBV3	1342	896	0.05%	0.007%
91	13.415	3830	3833	3835	rBV4	1360	760	0.04%	0.006%
92	13.772	3936	3944	3951	rBV10	1737	3110	0.17%	0.025%
93	13.852	3967	3969	3972	rVB4	2423	1204	0.07%	0.010%
94	13.984	4007	4010	4011	rBV3	1070	561	0.03%	0.004%
95	14.029	4022	4024	4026	rVB2	1177	493	0.03%	0.004%
96	14.042	4026	4028	4030	rBV3	1050	639	0.03%	0.005%
97	14.148	4059	4061	4065	rVB4	2012	1230	0.07%	0.010%
98	14.659	4215	4220	4222	rBV4	1478	1383	0.07%	0.011%
99	14.710	4232	4236	4238	rVB3	1355	807	0.04%	0.006%
100	14.775	4254	4256	4260	rVB4	1529	768	0.04%	0.006%


Sum of corrected areas: 12591477

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016599.D
Acq On : 06 Jun 2020 18:50
Operator : SY/MD
Sample : L2895-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
EW0M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

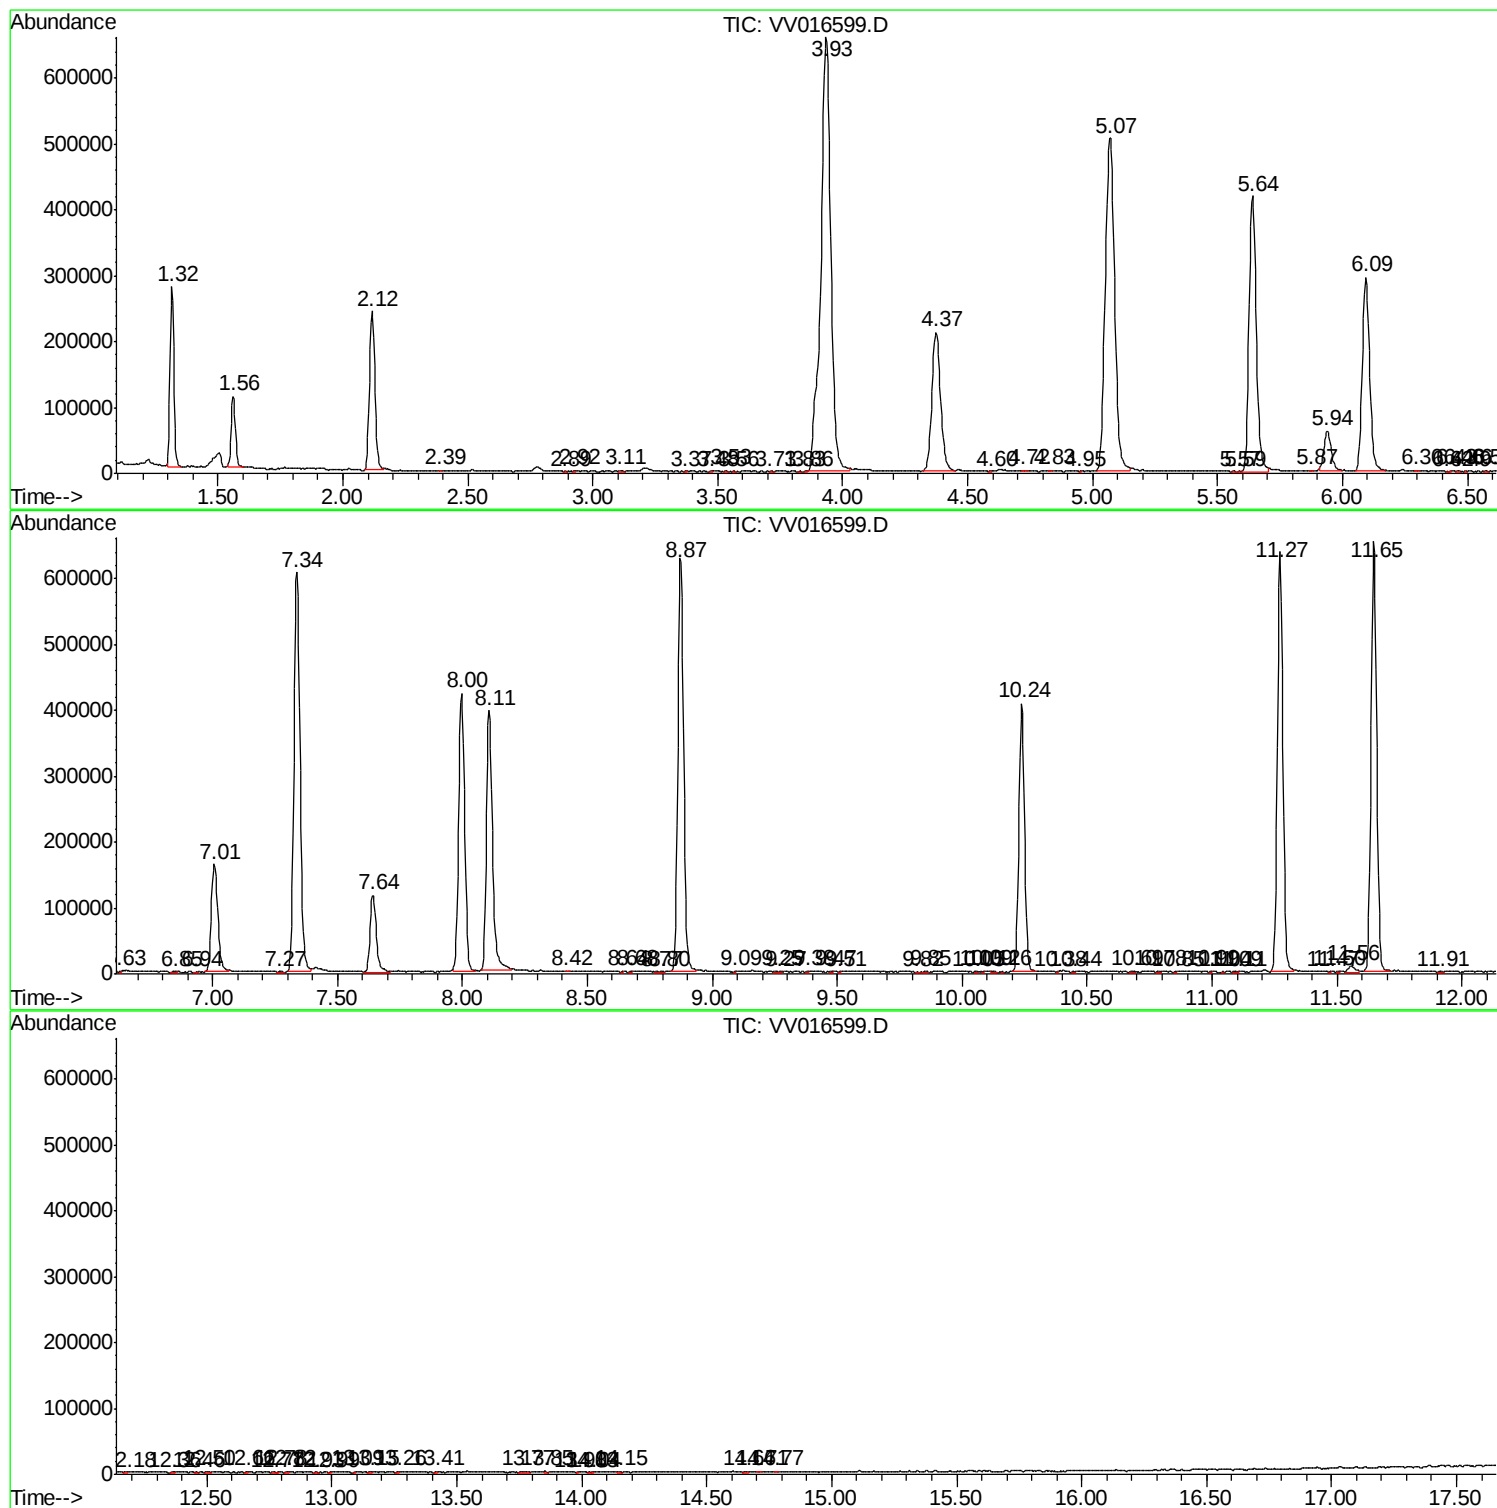

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016599.D
Acq On : 06 Jun 2020 18:50
Operator : SY/MD
Sample : L2895-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016599.D
Acq On : 06 Jun 2020 18:50
Operator : SY/MD
Sample : L2895-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc