

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016603.D
 Acq On : 06 Jun 2020 21:48
 Operator : SY/MD
 Sample : VV0606WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	171733	173050	11.71%	1.548%
2	1.560	140	146	158	rVB	127255	149904	10.15%	1.341%
3	2.116	310	319	340	rVB	280962	416554	28.20%	3.726%
4	2.479	430	432	437	rVB5	1578	791	0.05%	0.007%
5	2.769	518	522	526	rBV5	2238	1941	0.13%	0.017%
6	2.849	544	547	550	rVB4	1390	932	0.06%	0.008%
7	2.891	558	560	562	rBV3	1484	940	0.06%	0.008%
8	3.003	593	595	599	rVB3	935	601	0.04%	0.005%
9	3.032	602	604	609	rVB5	1432	910	0.06%	0.008%
10	3.087	617	621	625	rVV6	1383	1291	0.09%	0.012%
11	3.322	693	694	697	rBV2	1083	607	0.04%	0.005%
12	3.360	703	706	709	rVV3	1524	1014	0.07%	0.009%
13	3.486	743	745	749	rVB3	1230	964	0.07%	0.009%
14	3.508	749	752	753	rBV3	1158	619	0.04%	0.006%
15	3.540	758	762	764	rBV4	1104	631	0.04%	0.006%
16	3.621	783	787	792	rVB7	1242	1135	0.08%	0.010%
17	3.647	792	795	799	rVB6	1127	744	0.05%	0.007%
18	3.675	799	804	805	rBV4	1141	1110	0.08%	0.010%
19	3.749	824	827	829	rBV4	1317	937	0.06%	0.008%
20	3.894	862	872	902	rVV	116345	310656	21.03%	2.778%
21	4.286	991	994	997	rVB5	1219	793	0.05%	0.007%
22	4.306	997	1000	1003	rBV4	1209	1004	0.07%	0.009%
23	4.373	1004	1021	1046	rVV	241489	584788	39.59%	5.230%
24	4.717	1125	1128	1131	rVB5	2263	1412	0.10%	0.013%
25	5.071	1221	1238	1269	rBV2	564505	1477260	100.00%	13.212%
26	5.344	1321	1323	1328	rBV5	1175	641	0.04%	0.006%
27	5.576	1393	1395	1398	rVB4	1166	584	0.04%	0.005%
28	5.640	1400	1415	1433	rBV	445206	885752	59.96%	7.922%
29	5.920	1494	1502	1503	rBV6	6903	5713	0.39%	0.051%
30	6.000	1525	1527	1530	rBV3	1106	641	0.04%	0.006%
31	6.093	1539	1556	1580	rBV	329758	671879	45.48%	6.009%
32	7.007	1829	1840	1860	rBV	181213	319386	21.62%	2.857%
33	7.167	1888	1890	1892	rBV3	1829	1057	0.07%	0.009%
34	7.289	1924	1928	1931	rBV4	1214	1210	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016603.D
 Acq On : 06 Jun 2020 21:48
 Operator : SY/MD
 Sample : VV0606WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1962	rVV	680655	1169471	79.16%	10.460%
36	7.537	2002	2005	2008	rBV4	1578	1022	0.07%	0.009%
37	7.643	2026	2038	2060	rBV	126805	222850	15.09%	1.993%
38	7.826	2092	2095	2099	rBV6	1477	895	0.06%	0.008%
39	7.923	2121	2125	2126	rBV3	1019	644	0.04%	0.006%
40	7.952	2131	2134	2136	rBV3	1360	870	0.06%	0.008%
41	8.042	2158	2162	2170	rVB9	1498	2419	0.16%	0.022%
42	8.106	2170	2182	2214	rBV	432855	752563	50.94%	6.731%
43	8.646	2348	2350	2354	rBV4	1008	871	0.06%	0.008%
44	8.698	2364	2366	2369	rVB4	1163	591	0.04%	0.005%
45	8.714	2369	2371	2375	rBV4	1064	752	0.05%	0.007%
46	8.791	2392	2395	2398	rVB5	1169	576	0.04%	0.005%
47	8.814	2401	2402	2406	rVB4	1401	742	0.05%	0.007%
48	8.875	2409	2421	2440	rVV	662220	1073729	72.68%	9.603%
49	9.437	2593	2596	2598	rBV4	1552	1113	0.08%	0.010%
50	9.469	2604	2606	2609	rVB2	1755	888	0.06%	0.008%
51	9.498	2612	2615	2617	rBV3	1145	565	0.04%	0.005%
52	9.550	2627	2631	2634	rBV5	1549	1283	0.09%	0.011%
53	9.791	2702	2706	2708	rBV4	1048	782	0.05%	0.007%
54	10.087	2795	2798	2799	rVV3	1052	725	0.05%	0.006%
55	10.238	2833	2845	2859	rBV	455877	703126	47.60%	6.289%
56	10.463	2909	2915	2919	rVB7	1725	1625	0.11%	0.015%
57	10.492	2921	2924	2930	rBV5	1731	1603	0.11%	0.014%
58	10.547	2939	2941	2944	rBV4	1252	987	0.07%	0.009%
59	10.592	2952	2955	2956	rBV3	1174	633	0.04%	0.006%
60	10.633	2964	2968	2974	rBV8	1091	949	0.06%	0.008%
61	10.662	2974	2977	2979	rBV3	1547	1018	0.07%	0.009%
62	10.717	2992	2994	2996	rBV3	876	565	0.04%	0.005%
63	10.920	3053	3057	3060	rBV5	1183	976	0.07%	0.009%
64	11.048	3094	3097	3099	rVV3	1300	728	0.05%	0.007%
65	11.161	3129	3132	3136	rBV6	919	655	0.04%	0.006%
66	11.190	3136	3141	3142	rBV4	2462	1716	0.12%	0.015%
67	11.270	3155	3166	3184	rBV	671455	1037235	70.21%	9.277%
68	11.572	3254	3260	3265	rBV7	1455	1450	0.10%	0.013%
69	11.646	3271	3283	3299	rBV	723239	1127421	76.32%	10.084%
70	11.801	3328	3331	3333	rBV3	1334	788	0.05%	0.007%
71	11.913	3364	3366	3368	rBV3	1550	624	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016603.D
 Acq On : 06 Jun 2020 21:48
 Operator : SY/MD
 Sample : VV0606WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.968	3378	3383	3386	rBV6	1379	1224	0.08%	0.011%
73	12.003	3389	3394	3397	rBV6	903	972	0.07%	0.009%
74	12.035	3401	3404	3405	rBV3	1160	576	0.04%	0.005%
75	12.090	3419	3421	3424	rBV2	1045	655	0.04%	0.006%
76	12.174	3443	3447	3449	rBV4	1185	690	0.05%	0.006%
77	12.244	3465	3469	3472	rBV4	1183	963	0.07%	0.009%
78	12.354	3500	3503	3505	rBV3	988	601	0.04%	0.005%
79	12.495	3545	3547	3551	rBV4	1014	764	0.05%	0.007%
80	12.595	3576	3578	3582	rVB4	1636	1029	0.07%	0.009%
81	12.640	3584	3592	3595	rBV10	1182	1402	0.09%	0.013%
82	12.672	3595	3602	3610	rBV10	3547	6168	0.42%	0.055%
83	12.833	3646	3652	3654	rBV6	1311	1379	0.09%	0.012%
84	13.219	3768	3772	3775	rBV4	1280	1153	0.08%	0.010%
85	13.286	3785	3793	3800	rBV10	4930	7995	0.54%	0.072%
86	13.350	3811	3813	3817	rVB5	974	570	0.04%	0.005%
87	13.373	3817	3820	3826	rBV7	1104	1071	0.07%	0.010%
88	13.402	3826	3829	3832	rBV5	1440	1214	0.08%	0.011%
89	13.489	3853	3856	3861	rBV7	1335	1447	0.10%	0.013%
90	13.530	3862	3869	3870	rBV6	3908	3899	0.26%	0.035%
91	13.591	3885	3888	3891	rBV4	1621	1053	0.07%	0.009%
92	13.772	3940	3944	3951	rVB8	3487	4014	0.27%	0.036%
93	13.913	3986	3988	3991	rBV4	870	572	0.04%	0.005%
94	14.170	4062	4068	4071	rBV7	1871	2292	0.16%	0.020%
95	14.463	4157	4159	4161	rBV2	1144	577	0.04%	0.005%
96	14.575	4192	4194	4198	rVB3	927	698	0.05%	0.006%
97	14.630	4205	4211	4213	rVB5	2028	1994	0.13%	0.018%
98	14.649	4213	4217	4218	rBV3	1438	1095	0.07%	0.010%
99	14.955	4309	4312	4314	rBV3	1316	929	0.06%	0.008%
100	15.099	4355	4357	4361	rBV5	1581	916	0.06%	0.008%


Sum of corrected areas: 11180813

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016603.D
Acq On : 06 Jun 2020 21:48
Operator : SY/MD
Sample : VV0606WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

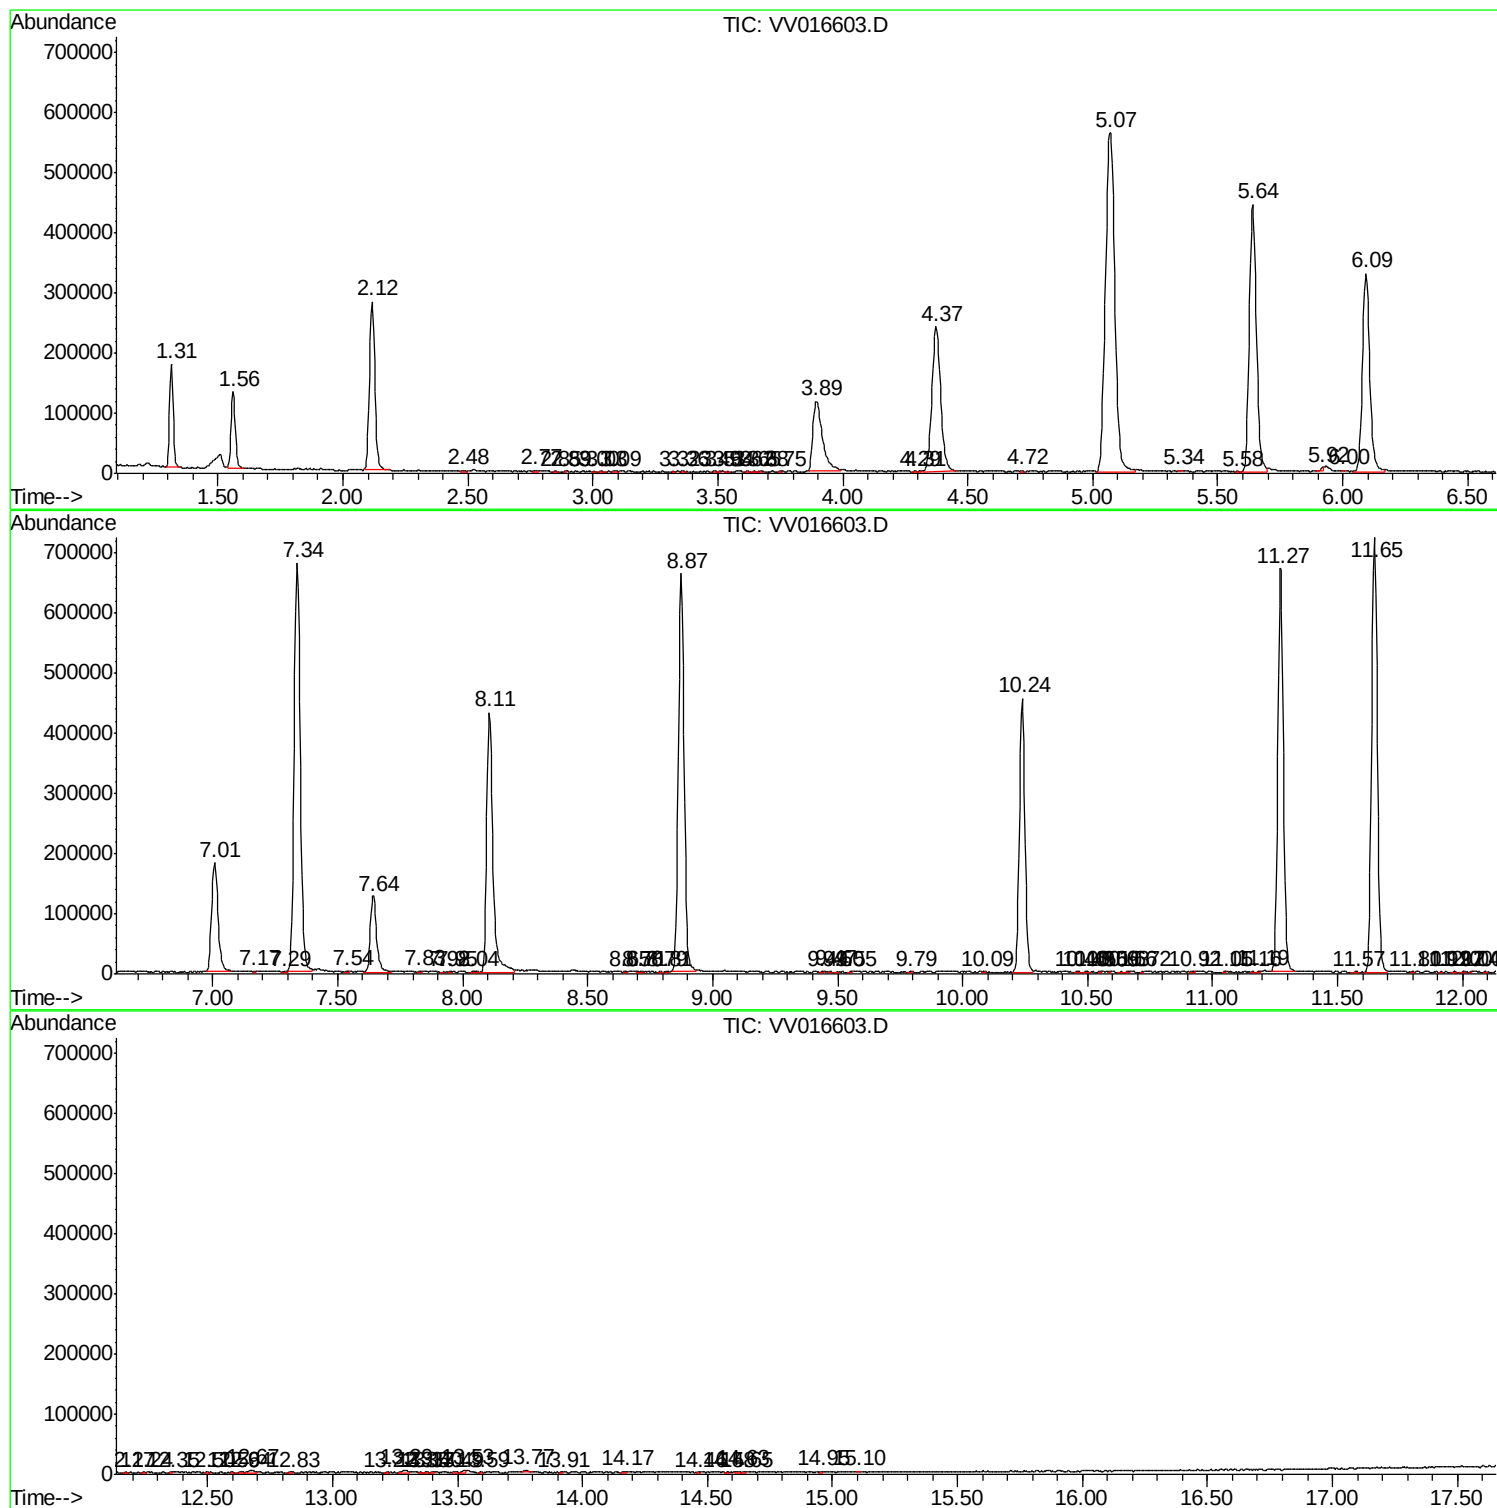

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016603.D
Acq On : 06 Jun 2020 21:48
Operator : SY/MD
Sample : VV0606WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016603.D
Acq On : 06 Jun 2020 21:48
Operator : SY/MD
Sample : VV0606WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc