

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016607.D
 Acq On : 06 Jun 2020 23:23
 Operator : SY/MD
 Sample : L2875-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	94	rBV	8337124	8935141	42.03%	21.705%
2	1.563	141	147	163	rVB	140626	169040	0.80%	0.411%
3	2.119	310	320	333	rBV	315310	469151	2.21%	1.140%
4	2.582	461	464	465	rBV4	1155	749	0.00%	0.002%
5	2.708	501	503	505	rBV3	1282	569	0.00%	0.001%
6	2.733	509	511	514	rBV3	1581	624	0.00%	0.002%
7	2.778	514	525	538	rVV2	33943	59851	0.28%	0.145%
8	2.862	547	551	553	rBV4	1103	765	0.00%	0.002%
9	2.929	568	572	574	rBV4	1145	1024	0.00%	0.002%
10	2.984	587	589	593	rVB3	1715	975	0.00%	0.002%
11	3.032	603	604	607	rBV3	1189	424	0.00%	0.001%
12	3.132	632	635	638	rBV4	1346	1245	0.01%	0.003%
13	3.273	675	679	683	rBV7	1308	1197	0.01%	0.003%
14	3.312	688	691	693	rBV3	1024	462	0.00%	0.001%
15	3.360	704	706	707	rBV2	700	257	0.00%	0.001%
16	3.508	748	752	755	rVB5	1764	1531	0.01%	0.004%
17	3.524	755	757	758	rBV2	1078	452	0.00%	0.001%
18	3.563	766	769	774	rBV6	1575	1553	0.01%	0.004%
19	3.589	774	777	778	rBV3	1179	497	0.00%	0.001%
20	3.685	805	807	810	rBV3	1077	862	0.00%	0.002%
21	3.714	814	816	817	rBV2	901	331	0.00%	0.001%
22	3.775	833	835	839	rBV3	1376	829	0.00%	0.002%
23	3.936	861	885	921	rBV	8685510	21260640	100.00%	51.646%
24	4.373	1008	1021	1045	rVB	248056	597808	2.81%	1.452%
25	4.881	1176	1179	1181	rBV4	1509	803	0.00%	0.002%
26	5.000	1214	1216	1217	rBV2	794	271	0.00%	0.001%
27	5.071	1220	1238	1258	rBV2	603950	1536984	7.23%	3.734%
28	5.640	1401	1415	1439	rBV	452832	898594	4.23%	2.183%
29	6.093	1544	1556	1580	rVB	344658	690355	3.25%	1.677%
30	6.521	1687	1689	1692	rBV3	1899	1182	0.01%	0.003%
31	7.006	1829	1840	1856	rBV	193298	340119	1.60%	0.826%
32	7.338	1931	1943	1961	rBV	718817	1225138	5.76%	2.976%
33	7.531	1999	2003	2005	rBV5	1360	1089	0.01%	0.003%
34	7.640	2028	2037	2054	rBV	134572	227527	1.07%	0.553%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016607.D
 Acq On : 06 Jun 2020 23:23
 Operator : SY/MD
 Sample : L2875-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.897	2116	2117	2121	rBV4	1341	814	0.00%	0.002%
36	8.051	2162	2165	2168	rBV4	1446	1077	0.01%	0.003%
37	8.106	2172	2182	2215	rVV	445657	773679	3.64%	1.879%
38	8.874	2409	2421	2445	rBV	674137	1083679	5.10%	2.632%
39	9.466	2604	2605	2606	rBV	1031	386	0.00%	0.001%
40	9.559	2627	2634	2635	rBV6	2355	2057	0.01%	0.005%
41	10.013	2773	2775	2777	rBV3	1064	492	0.00%	0.001%
42	10.238	2833	2845	2858	rBV	448996	706644	3.32%	1.717%
43	10.553	2940	2943	2949	rBV7	2148	2236	0.01%	0.005%
44	10.707	2989	2991	2994	rBV4	1026	605	0.00%	0.001%
45	11.016	3083	3087	3089	rBV3	1921	1060	0.00%	0.003%
46	11.270	3155	3166	3186	rBV	661223	1014231	4.77%	2.464%
47	11.646	3272	3283	3303	rBV	705953	1121108	5.27%	2.723%
48	11.910	3362	3365	3367	rBV4	1134	802	0.00%	0.002%
49	12.013	3395	3397	3398	rBV2	837	292	0.00%	0.001%
50	12.144	3436	3438	3439	rBV2	926	314	0.00%	0.001%
51	12.212	3455	3459	3460	rBV2	1469	925	0.00%	0.002%
52	12.238	3465	3467	3469	rBV3	1073	695	0.00%	0.002%
53	12.337	3495	3498	3499	rBV3	1788	915	0.00%	0.002%
54	12.440	3525	3530	3535	rBV8	2124	2282	0.01%	0.006%
55	12.460	3535	3536	3537	rBV	481	178	0.00%	0.000%
56	12.511	3550	3552	3555	rBV4	1208	794	0.00%	0.002%
57	12.633	3587	3590	3591	rBV	740	424	0.00%	0.001%
58	12.659	3595	3598	3599	rBV3	996	447	0.00%	0.001%
59	12.707	3610	3613	3614	rBV3	1097	605	0.00%	0.001%
60	12.771	3632	3633	3635	rBV	1005	426	0.00%	0.001%
61	12.810	3643	3645	3648	rBV4	805	394	0.00%	0.001%
62	12.861	3660	3661	3667	rVB4	1080	896	0.00%	0.002%
63	12.964	3692	3693	3695	rBV2	882	347	0.00%	0.001%
64	12.993	3700	3702	3704	rBV2	826	460	0.00%	0.001%
65	13.138	3742	3747	3751	rBV6	1549	1405	0.01%	0.003%
66	13.177	3757	3759	3761	rBV3	1362	817	0.00%	0.002%
67	13.206	3764	3768	3769	rBV3	1629	1275	0.01%	0.003%
68	13.360	3809	3816	3817	rBV6	1355	1501	0.01%	0.004%
69	13.488	3854	3856	3859	rBV3	965	482	0.00%	0.001%
70	13.537	3866	3871	3874	rBV7	2088	2006	0.01%	0.005%
71	13.604	3890	3892	3894	rBV2	1289	814	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016607.D
Acq On : 06 Jun 2020 23:23
Operator : SY/MD
Sample : L2875-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Title : VOC Analysis

72	13.717	3925	3927	3929	rBV2	1024	596	0.00%	0.001%
73	13.759	3935	3940	3945	rBV8	1860	1636	0.01%	0.004%
74	13.820	3956	3959	3960	rBV3	660	443	0.00%	0.001%
75	13.968	4001	4005	4007	rVB5	1761	792	0.00%	0.002%
76	13.980	4007	4009	4012	rBV4	731	387	0.00%	0.001%
77	13.993	4012	4013	4016	rBV2	1079	550	0.00%	0.001%
78	14.160	4062	4065	4070	rVB5	1798	1538	0.01%	0.004%
79	14.183	4070	4072	4075	rBV3	1881	1611	0.01%	0.004%
80	14.254	4092	4094	4096	rBV3	1062	427	0.00%	0.001%
81	14.267	4096	4098	4100	rBV3	1657	912	0.00%	0.002%
82	14.353	4122	4125	4127	rBV3	1558	864	0.00%	0.002%
83	14.437	4149	4151	4152	rBV2	867	323	0.00%	0.001%
84	14.617	4205	4207	4208	rBV2	1265	375	0.00%	0.001%




Sum of corrected areas: 41166057

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016607.D
Acq On : 06 Jun 2020 23:23
Operator : SY/MD
Sample : L2875-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

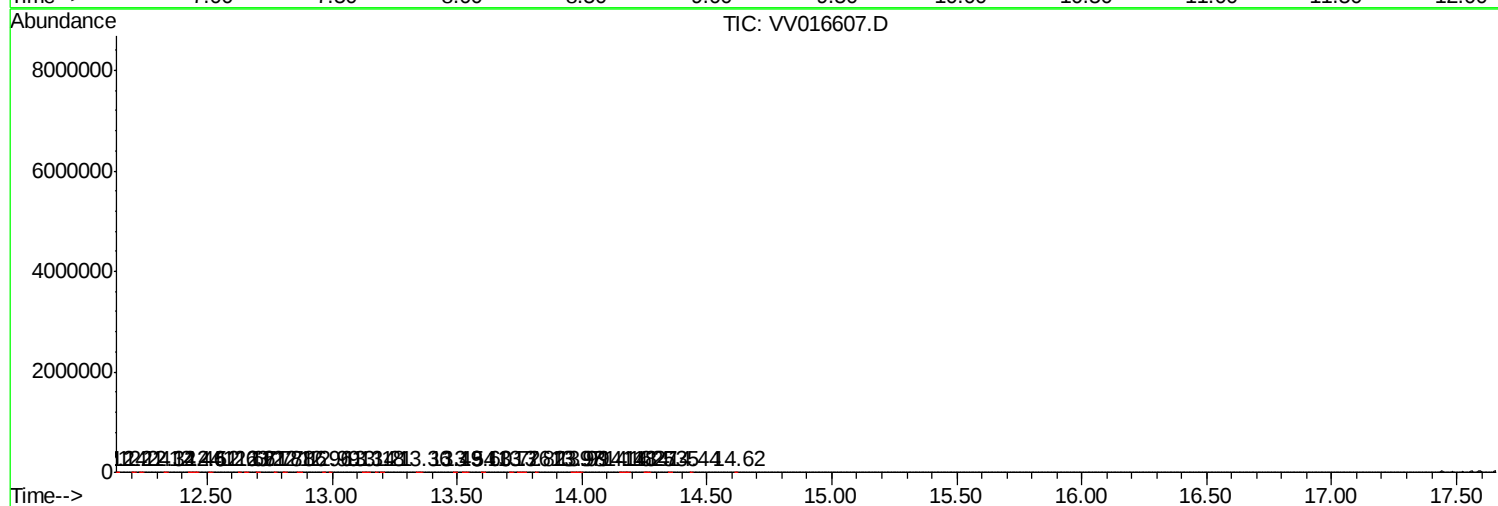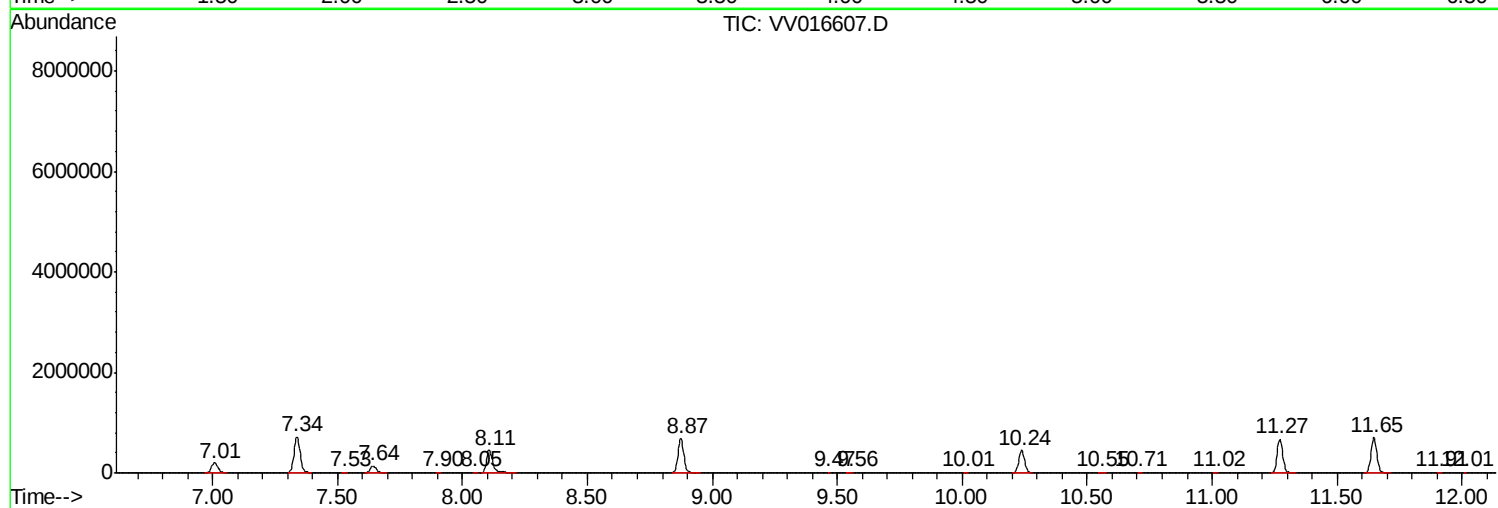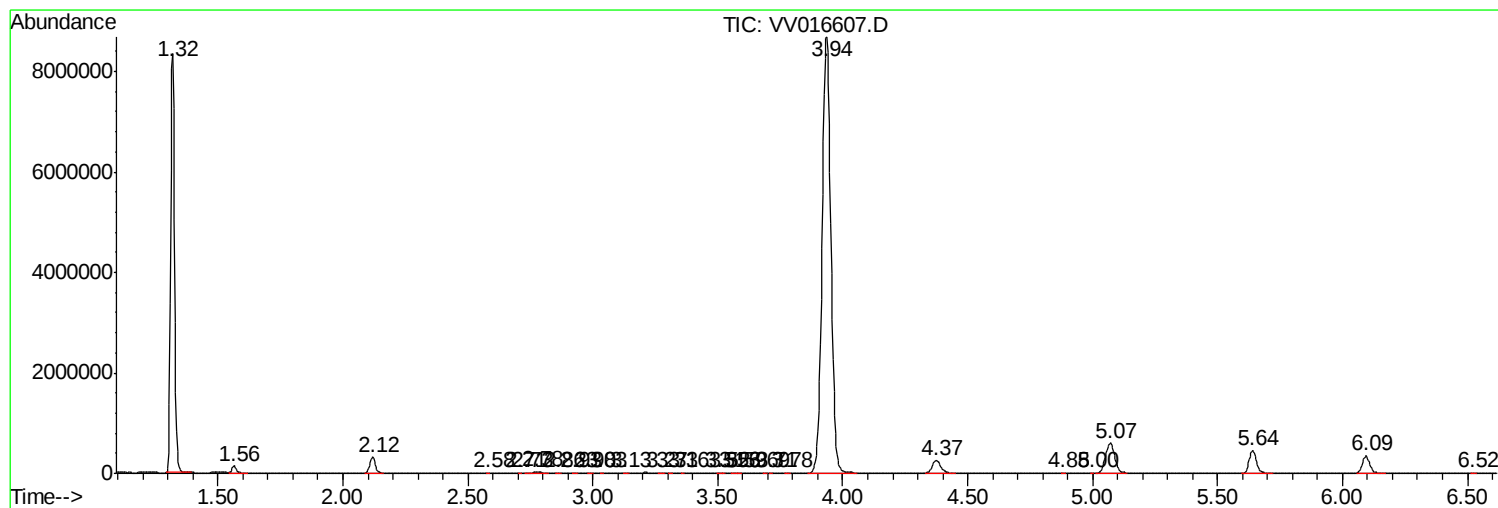

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016607.D
Acq On : 06 Jun 2020 23:23
Operator : SY/MD
Sample : L2875-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016607.D
Acq On : 06 Jun 2020 23:23
Operator : SY/MD
Sample : L2875-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc