

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016609.D
 Acq On : 07 Jun 2020 00:11
 Operator : SY/MD
 Sample : L2875-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	214226	214231	13.66%	1.853%
2	1.566	143	148	158	rVB	130783	150985	9.63%	1.306%
3	2.119	310	320	335	rBV	305419	451809	28.81%	3.907%
4	2.640	479	482	483	rBV3	949	587	0.04%	0.005%
5	2.753	514	517	519	rVB3	1728	988	0.06%	0.009%
6	2.775	519	524	526	rBV6	2237	2119	0.14%	0.018%
7	2.868	549	553	555	rBV4	1732	1219	0.08%	0.011%
8	2.900	560	563	567	rBV4	1347	1173	0.07%	0.010%
9	3.000	589	594	603	rBV9	1756	2825	0.18%	0.024%
10	3.129	631	634	638	rBV4	906	699	0.04%	0.006%
11	3.164	644	645	649	rVB3	1306	668	0.04%	0.006%
12	3.232	664	666	672	rVB6	2141	1253	0.08%	0.011%
13	3.267	673	677	680	rVB6	1376	1106	0.07%	0.010%
14	3.328	693	696	699	rBV4	1330	1077	0.07%	0.009%
15	3.450	729	734	739	rBV7	1374	1279	0.08%	0.011%
16	3.479	739	743	745	rBV5	1628	978	0.06%	0.008%
17	3.572	770	772	776	rVB4	1128	593	0.04%	0.005%
18	3.717	814	817	822	rBV5	873	921	0.06%	0.008%
19	3.855	856	860	862	rBV3	1134	620	0.04%	0.005%
20	3.897	862	873	904	rBV	119205	352763	22.49%	3.050%
21	4.257	981	985	994	rVB10	2257	2914	0.19%	0.025%
22	4.296	994	997	998	rBV3	1797	943	0.06%	0.008%
23	4.373	1007	1021	1040	rVV	246253	593766	37.86%	5.134%
24	4.511	1062	1064	1066	rBV3	1367	795	0.05%	0.007%
25	4.595	1087	1090	1095	rVB6	1453	1110	0.07%	0.010%
26	4.624	1095	1099	1100	rBV4	887	683	0.04%	0.006%
27	5.071	1219	1238	1268	rBV2	604565	1568375	100.00%	13.562%
28	5.273	1296	1301	1305	rBV7	1540	1722	0.11%	0.015%
29	5.479	1362	1365	1367	rBV3	1340	748	0.05%	0.006%
30	5.508	1372	1374	1378	rBV3	1039	731	0.05%	0.006%
31	5.588	1396	1399	1401	rBV3	880	668	0.04%	0.006%
32	5.640	1401	1415	1438	rVV	476789	942147	60.07%	8.147%
33	6.093	1544	1556	1578	rVB	350252	697180	44.45%	6.029%
34	6.334	1628	1631	1632	rBV4	1419	646	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016609.D
 Acq On : 07 Jun 2020 00:11
 Operator : SY/MD
 Sample : L2875-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.373	1641	1643	1645	rBV4	1457	642	0.04%	0.006%
36	6.521	1686	1689	1690	rBV2	1464	780	0.05%	0.007%
37	6.617	1716	1719	1720	rBV3	1513	819	0.05%	0.007%
38	7.006	1829	1840	1857	rBV	186505	332994	21.23%	2.879%
39	7.228	1905	1909	1911	rVB6	1157	836	0.05%	0.007%
40	7.338	1931	1943	1961	rBV	729016	1231236	78.50%	10.647%
41	7.643	2027	2038	2056	rBV	132866	228798	14.59%	1.978%
42	7.801	2084	2087	2091	rBV6	1221	1009	0.06%	0.009%
43	7.826	2091	2095	2096	rBV3	2314	1519	0.10%	0.013%
44	8.106	2170	2182	2215	rBV	435687	761547	48.56%	6.585%
45	8.733	2374	2377	2382	rBV6	1887	1411	0.09%	0.012%
46	8.874	2406	2421	2444	rBV	704821	1132286	72.19%	9.791%
47	9.222	2526	2529	2533	rVB4	1434	1002	0.06%	0.009%
48	9.321	2557	2560	2562	rBV4	927	794	0.05%	0.007%
49	9.376	2572	2577	2578	rBV6	1614	1330	0.08%	0.012%
50	9.598	2644	2646	2650	rBV4	1059	663	0.04%	0.006%
51	9.707	2678	2680	2683	rBV4	1112	703	0.04%	0.006%
52	9.823	2714	2716	2720	rVB4	1585	1004	0.06%	0.009%
53	9.846	2720	2723	2726	rBV5	1941	1372	0.09%	0.012%
54	9.955	2752	2757	2760	rBV5	1237	1285	0.08%	0.011%
55	10.177	2824	2826	2831	rVB5	1748	1266	0.08%	0.011%
56	10.238	2831	2845	2860	rBV	445379	693528	44.22%	5.997%
57	10.440	2905	2908	2911	rBV5	1520	1220	0.08%	0.011%
58	10.482	2916	2921	2923	rBV4	1272	1060	0.07%	0.009%
59	10.563	2941	2946	2951	rBV7	2001	2151	0.14%	0.019%
60	10.636	2967	2969	2972	rBV3	1296	675	0.04%	0.006%
61	10.820	3021	3026	3031	rBV10	1566	1732	0.11%	0.015%
62	10.871	3037	3042	3043	rBV5	1311	1164	0.07%	0.010%
63	11.080	3105	3107	3111	rVB3	1308	757	0.05%	0.007%
64	11.183	3136	3139	3140	rBV3	1326	872	0.06%	0.008%
65	11.270	3155	3166	3185	rBV	679369	1027754	65.53%	8.887%
66	11.508	3236	3240	3243	rBV4	1968	1351	0.09%	0.012%
67	11.556	3245	3255	3263	rBV4	4419	8420	0.54%	0.073%
68	11.646	3272	3283	3300	rBV	691214	1087110	69.31%	9.400%
69	12.058	3405	3411	3412	rBV4	1864	1716	0.11%	0.015%
70	12.103	3420	3425	3426	rBV5	1409	978	0.06%	0.008%
71	12.202	3453	3456	3458	rVB4	1278	594	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016609.D
 Acq On : 07 Jun 2020 00:11
 Operator : SY/MD
 Sample : L2875-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.267	3470	3476	3478	rBV7	2030	2378	0.15%	0.021%
73	12.357	3501	3504	3507	rBV5	1029	733	0.05%	0.006%
74	12.421	3522	3524	3528	rBV4	1258	994	0.06%	0.009%
75	12.559	3565	3567	3572	rVB6	1922	1347	0.09%	0.012%
76	12.604	3579	3581	3583	rBV3	1600	695	0.04%	0.006%
77	12.678	3601	3604	3609	rBV6	1409	1624	0.10%	0.014%
78	12.794	3638	3640	3644	rVB5	1073	685	0.04%	0.006%
79	12.829	3650	3651	3654	rBV3	1275	912	0.06%	0.008%
80	12.878	3664	3666	3671	rVV6	1188	1072	0.07%	0.009%
81	13.000	3697	3704	3705	rBV6	1164	1090	0.07%	0.009%
82	13.058	3720	3722	3723	rBV2	1311	612	0.04%	0.005%
83	13.138	3743	3747	3749	rBV4	1581	1259	0.08%	0.011%
84	13.244	3777	3780	3783	rBV3	1298	1213	0.08%	0.010%
85	13.411	3828	3832	3835	rBV6	978	866	0.06%	0.007%
86	13.697	3918	3921	3925	rBV5	1012	797	0.05%	0.007%
87	13.739	3931	3934	3937	rBV4	1046	791	0.05%	0.007%
88	13.771	3941	3944	3947	rBV5	1953	1261	0.08%	0.011%
89	13.813	3955	3957	3960	rBV3	1750	718	0.05%	0.006%
90	13.839	3963	3965	3969	rVB3	1200	866	0.06%	0.007%
91	13.984	4005	4010	4017	rVB9	1770	1973	0.13%	0.017%
92	14.013	4017	4019	4022	rBV3	933	645	0.04%	0.006%
93	14.086	4039	4042	4048	rBV6	994	914	0.06%	0.008%
94	14.138	4055	4058	4060	rBV4	1291	813	0.05%	0.007%
95	14.302	4107	4109	4111	rBV2	1424	738	0.05%	0.006%
96	14.344	4120	4122	4125	rBV4	1438	732	0.05%	0.006%
97	14.392	4133	4137	4140	rBV3	817	832	0.05%	0.007%
98	14.411	4140	4143	4147	rBV5	1829	1522	0.10%	0.013%
99	14.543	4181	4184	4188	rBV3	1072	892	0.06%	0.008%
100	15.791	4570	4572	4575	rVB2	2021	746	0.05%	0.006%


Sum of corrected areas: 11564419

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016609.D
Acq On : 07 Jun 2020 00:11
Operator : SY/MD
Sample : L2875-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

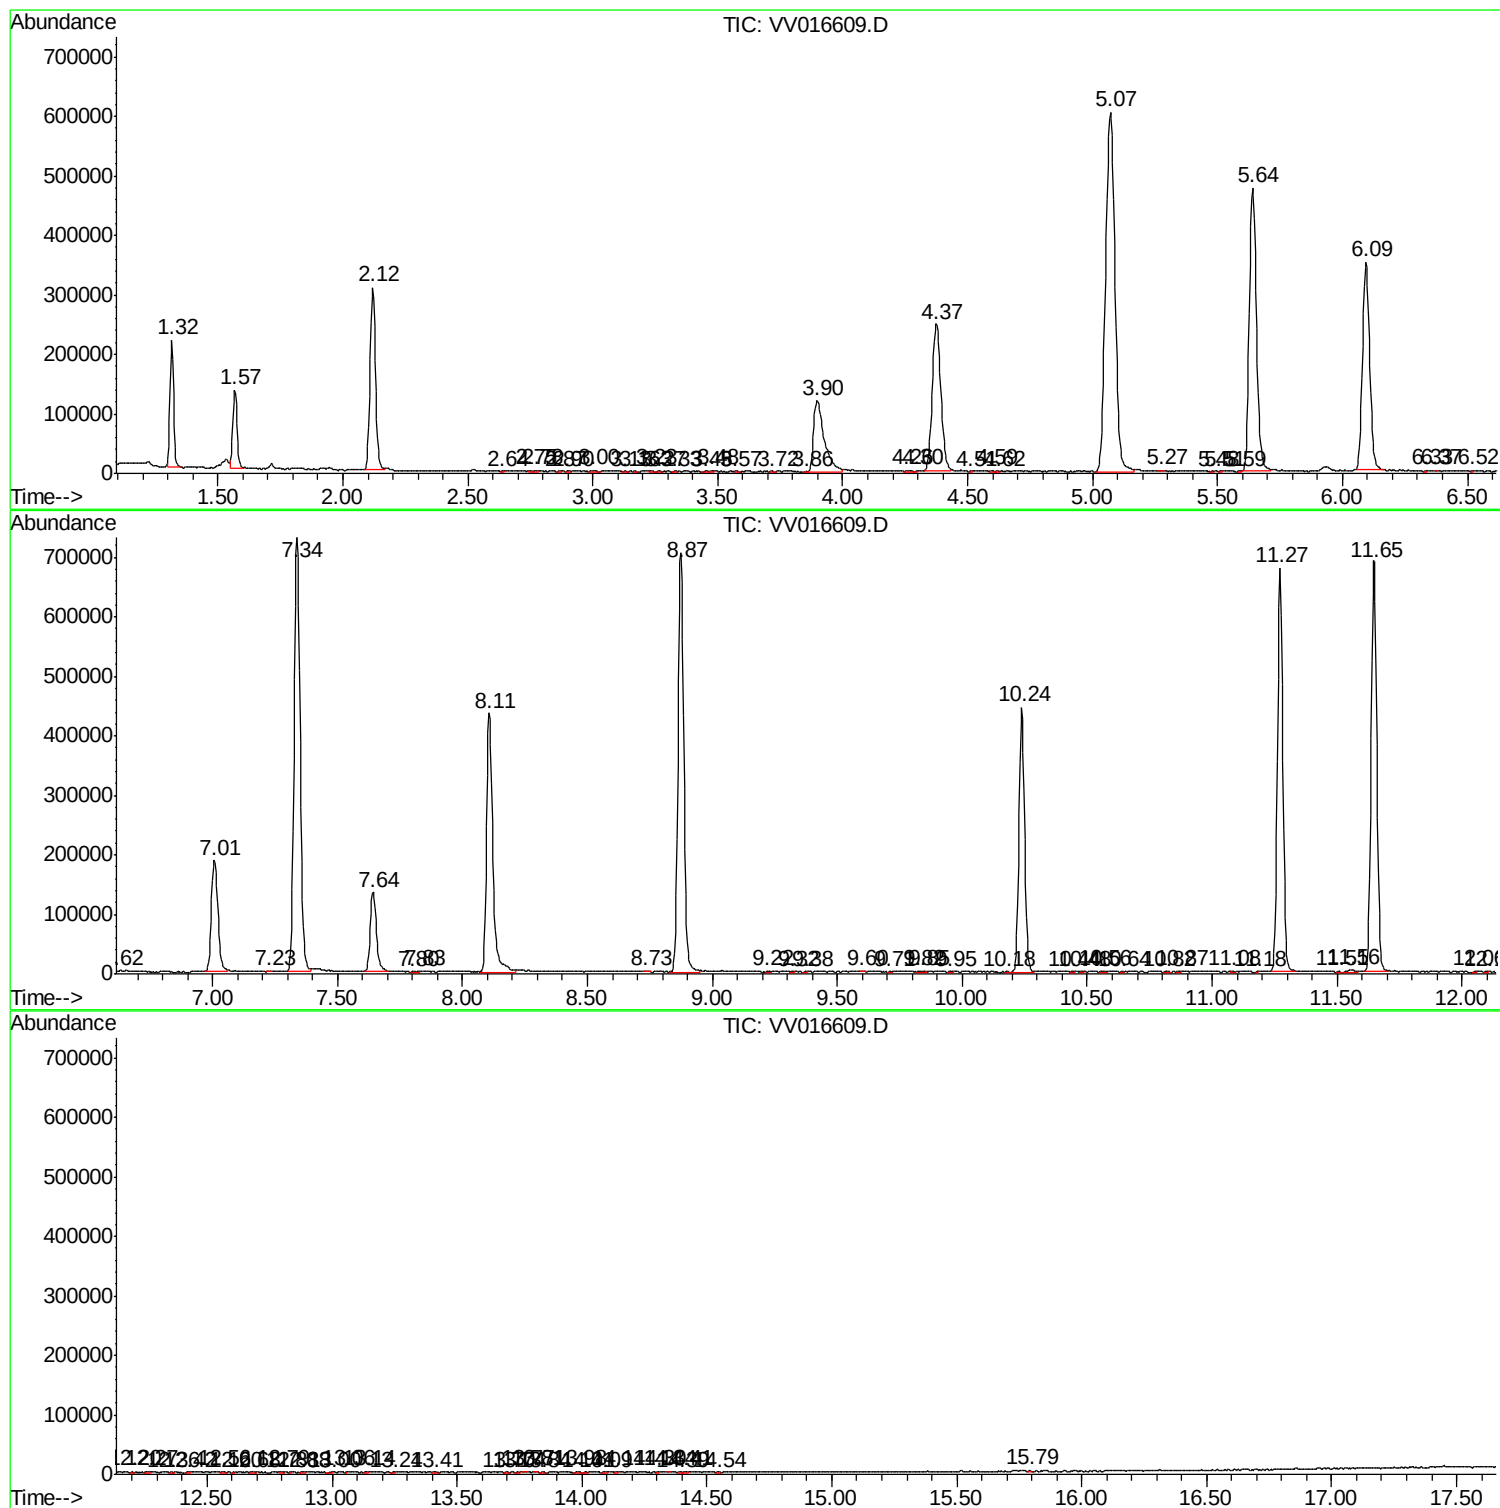

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016609.D
Acq On : 07 Jun 2020 00:11
Operator : SY/MD
Sample : L2875-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016609.D
Acq On : 07 Jun 2020 00:11
Operator : SY/MD
Sample : L2875-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc