

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016612.D
 Acq On : 07 Jun 2020 01:22
 Operator : SY/MD
 Sample : L2875-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	204698	203534	13.50%	1.823%
2	1.563	141	147	160	rVB	132788	155719	10.33%	1.395%
3	2.119	310	320	336	rBV	292543	434367	28.80%	3.891%
4	2.441	418	420	423	rBV4	890	620	0.04%	0.006%
5	2.505	437	440	442	rBV4	1352	982	0.07%	0.009%
6	2.736	509	512	513	rBV2	1293	584	0.04%	0.005%
7	2.769	513	522	533	rVV2	2505	5617	0.37%	0.050%
8	2.826	537	540	542	rVB3	1394	784	0.05%	0.007%
9	2.852	546	548	551	rBV3	1040	586	0.04%	0.005%
10	2.978	583	587	588	rBV3	1100	625	0.04%	0.006%
11	3.019	598	600	602	rBV3	1258	582	0.04%	0.005%
12	3.087	617	621	625	rVB7	891	715	0.05%	0.006%
13	3.106	625	627	630	rBV3	1692	670	0.04%	0.006%
14	3.318	690	693	698	rBV6	909	894	0.06%	0.008%
15	3.341	698	700	705	rVB5	858	563	0.04%	0.005%
16	3.367	705	708	713	rVB5	1157	969	0.06%	0.009%
17	3.392	713	716	720	rBV4	1054	1010	0.07%	0.009%
18	3.482	740	744	747	rBV5	1632	1524	0.10%	0.014%
19	3.498	747	749	752	rVB5	1617	898	0.06%	0.008%
20	3.605	779	782	786	rBV5	1035	762	0.05%	0.007%
21	3.634	788	791	794	rVB5	1268	850	0.06%	0.008%
22	3.650	794	796	798	rBV3	1308	672	0.04%	0.006%
23	3.666	798	801	803	rBV4	898	612	0.04%	0.005%
24	3.746	824	826	829	rVB4	1619	983	0.07%	0.009%
25	3.781	833	837	839	rBV5	1137	803	0.05%	0.007%
26	3.814	844	847	849	rBV4	980	759	0.05%	0.007%
27	3.897	863	873	902	rBV	116677	331017	21.95%	2.965%
28	4.280	990	992	995	rVB4	1487	814	0.05%	0.007%
29	4.306	995	1000	1001	rBV5	959	701	0.05%	0.006%
30	4.373	1007	1021	1045	rVB2	240985	577931	38.32%	5.177%
31	4.547	1072	1075	1080	rBV7	1587	1633	0.11%	0.015%
32	4.781	1144	1148	1149	rBV4	1449	1023	0.07%	0.009%
33	4.846	1164	1168	1174	rBV6	1789	1722	0.11%	0.015%
34	4.875	1174	1177	1180	rVB3	1149	748	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016612.D
 Acq On : 07 Jun 2020 01:22
 Operator : SY/MD
 Sample : L2875-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.071	1221	1238	1263	rVV2	593799	1508139	100.00%	13.509%
36	5.515	1374	1376	1378	rBV3	1716	1021	0.07%	0.009%
37	5.579	1393	1396	1397	rBV3	1483	668	0.04%	0.006%
38	5.640	1402	1415	1437	rBV	449583	875335	58.04%	7.841%
39	5.891	1489	1493	1496	rBV5	1917	931	0.06%	0.008%
40	5.926	1496	1504	1518	rVV5	7625	16867	1.12%	0.151%
41	6.093	1542	1556	1581	rBV	343437	689415	45.71%	6.175%
42	6.453	1664	1668	1670	rBV5	911	679	0.05%	0.006%
43	6.630	1721	1723	1728	rBV5	1693	1237	0.08%	0.011%
44	6.920	1810	1813	1815	rBV4	1113	571	0.04%	0.005%
45	6.955	1822	1824	1828	rVB5	1035	720	0.05%	0.006%
46	7.006	1828	1840	1856	rBV	187209	332070	22.02%	2.975%
47	7.174	1886	1892	1897	rBV9	2354	2771	0.18%	0.025%
48	7.338	1931	1943	1964	rBV	701976	1199128	79.51%	10.741%
49	7.643	2027	2038	2051	rBV	129908	218347	14.48%	1.956%
50	7.826	2091	2095	2097	rBV3	1791	995	0.07%	0.009%
51	7.932	2124	2128	2131	rBV4	1328	1277	0.08%	0.011%
52	8.106	2171	2182	2207	rBV	412695	734390	48.70%	6.578%
53	8.511	2301	2308	2311	rBV7	1384	1566	0.10%	0.014%
54	8.871	2409	2420	2438	rBV	658862	1054995	69.95%	9.450%
55	9.190	2517	2519	2523	rBV4	1700	1175	0.08%	0.011%
56	9.315	2553	2558	2561	rBV6	2573	2298	0.15%	0.021%
57	9.495	2610	2614	2617	rBV5	1184	1166	0.08%	0.010%
58	9.662	2662	2666	2671	rBV7	1834	1430	0.09%	0.013%
59	9.714	2679	2682	2683	rBV3	1341	681	0.05%	0.006%
60	9.739	2687	2690	2691	rVV3	1475	817	0.05%	0.007%
61	9.759	2694	2696	2702	rVV7	845	864	0.06%	0.008%
62	9.939	2748	2752	2754	rBV5	1272	1014	0.07%	0.009%
63	10.116	2804	2807	2811	rBV5	1679	957	0.06%	0.009%
64	10.238	2834	2845	2859	rVB	429703	667670	44.27%	5.981%
65	10.476	2916	2919	2922	rBV5	851	698	0.05%	0.006%
66	10.514	2927	2931	2933	rBV4	1623	1044	0.07%	0.009%
67	10.575	2946	2950	2951	rBV4	2413	1346	0.09%	0.012%
68	10.675	2979	2981	2984	rBV4	1302	888	0.06%	0.008%
69	10.698	2984	2988	2990	rVV5	1446	816	0.05%	0.007%
70	10.794	3015	3018	3024	rVB7	1701	1565	0.10%	0.014%
71	11.177	3134	3137	3139	rBV3	1660	1211	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016612.D
 Acq On : 07 Jun 2020 01:22
 Operator : SY/MD
 Sample : L2875-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3181	rBV	639892	992383	65.80%	8.889%
73	11.434	3213	3217	3220	rBV5	1339	1066	0.07%	0.010%
74	11.527	3244	3246	3249	rVB3	1161	727	0.05%	0.007%
75	11.646	3271	3283	3300	rBV	691695	1085919	72.00%	9.727%
76	11.894	3357	3360	3363	rBV3	1160	782	0.05%	0.007%
77	12.125	3427	3432	3436	rBV6	1324	1373	0.09%	0.012%
78	12.360	3500	3505	3507	rBV4	1572	1451	0.10%	0.013%
79	12.408	3516	3520	3524	rVB6	1357	1343	0.09%	0.012%
80	12.498	3545	3548	3550	rBV3	1846	1306	0.09%	0.012%
81	12.624	3585	3587	3588	rBV2	1089	612	0.04%	0.005%
82	12.665	3597	3600	3602	rBV5	1206	724	0.05%	0.006%
83	12.839	3648	3654	3655	rBV4	1649	1355	0.09%	0.012%
84	12.932	3681	3683	3686	rBV4	1176	740	0.05%	0.007%
85	13.035	3713	3715	3717	rBV3	1329	696	0.05%	0.006%
86	13.048	3717	3719	3720	rVV2	1685	614	0.04%	0.005%
87	13.070	3724	3726	3728	rVB3	1524	800	0.05%	0.007%
88	13.099	3732	3735	3738	rVV5	1481	1124	0.07%	0.010%
89	13.148	3746	3750	3751	rBV3	1122	662	0.04%	0.006%
90	13.366	3815	3818	3819	rBV3	921	647	0.04%	0.006%
91	13.759	3938	3940	3942	rBV3	1160	707	0.05%	0.006%
92	13.923	3986	3991	3993	rBV4	1510	1190	0.08%	0.011%
93	14.132	4053	4056	4057	rBV2	1194	685	0.05%	0.006%
94	14.286	4099	4104	4107	rBV7	1922	2120	0.14%	0.019%
95	14.363	4126	4128	4135	rVB7	1010	871	0.06%	0.008%
96	14.521	4172	4177	4181	rBV7	1436	1719	0.11%	0.015%
97	14.871	4284	4286	4289	rBV4	1289	696	0.05%	0.006%
98	14.955	4310	4312	4316	rBV3	953	827	0.05%	0.007%
99	15.151	4371	4373	4375	rBV2	1701	836	0.06%	0.007%
100	15.713	4546	4548	4550	rBV3	1790	865	0.06%	0.008%


Sum of corrected areas: 11163875

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016612.D
Acq On : 07 Jun 2020 01:22
Operator : SY/MD
Sample : L2875-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

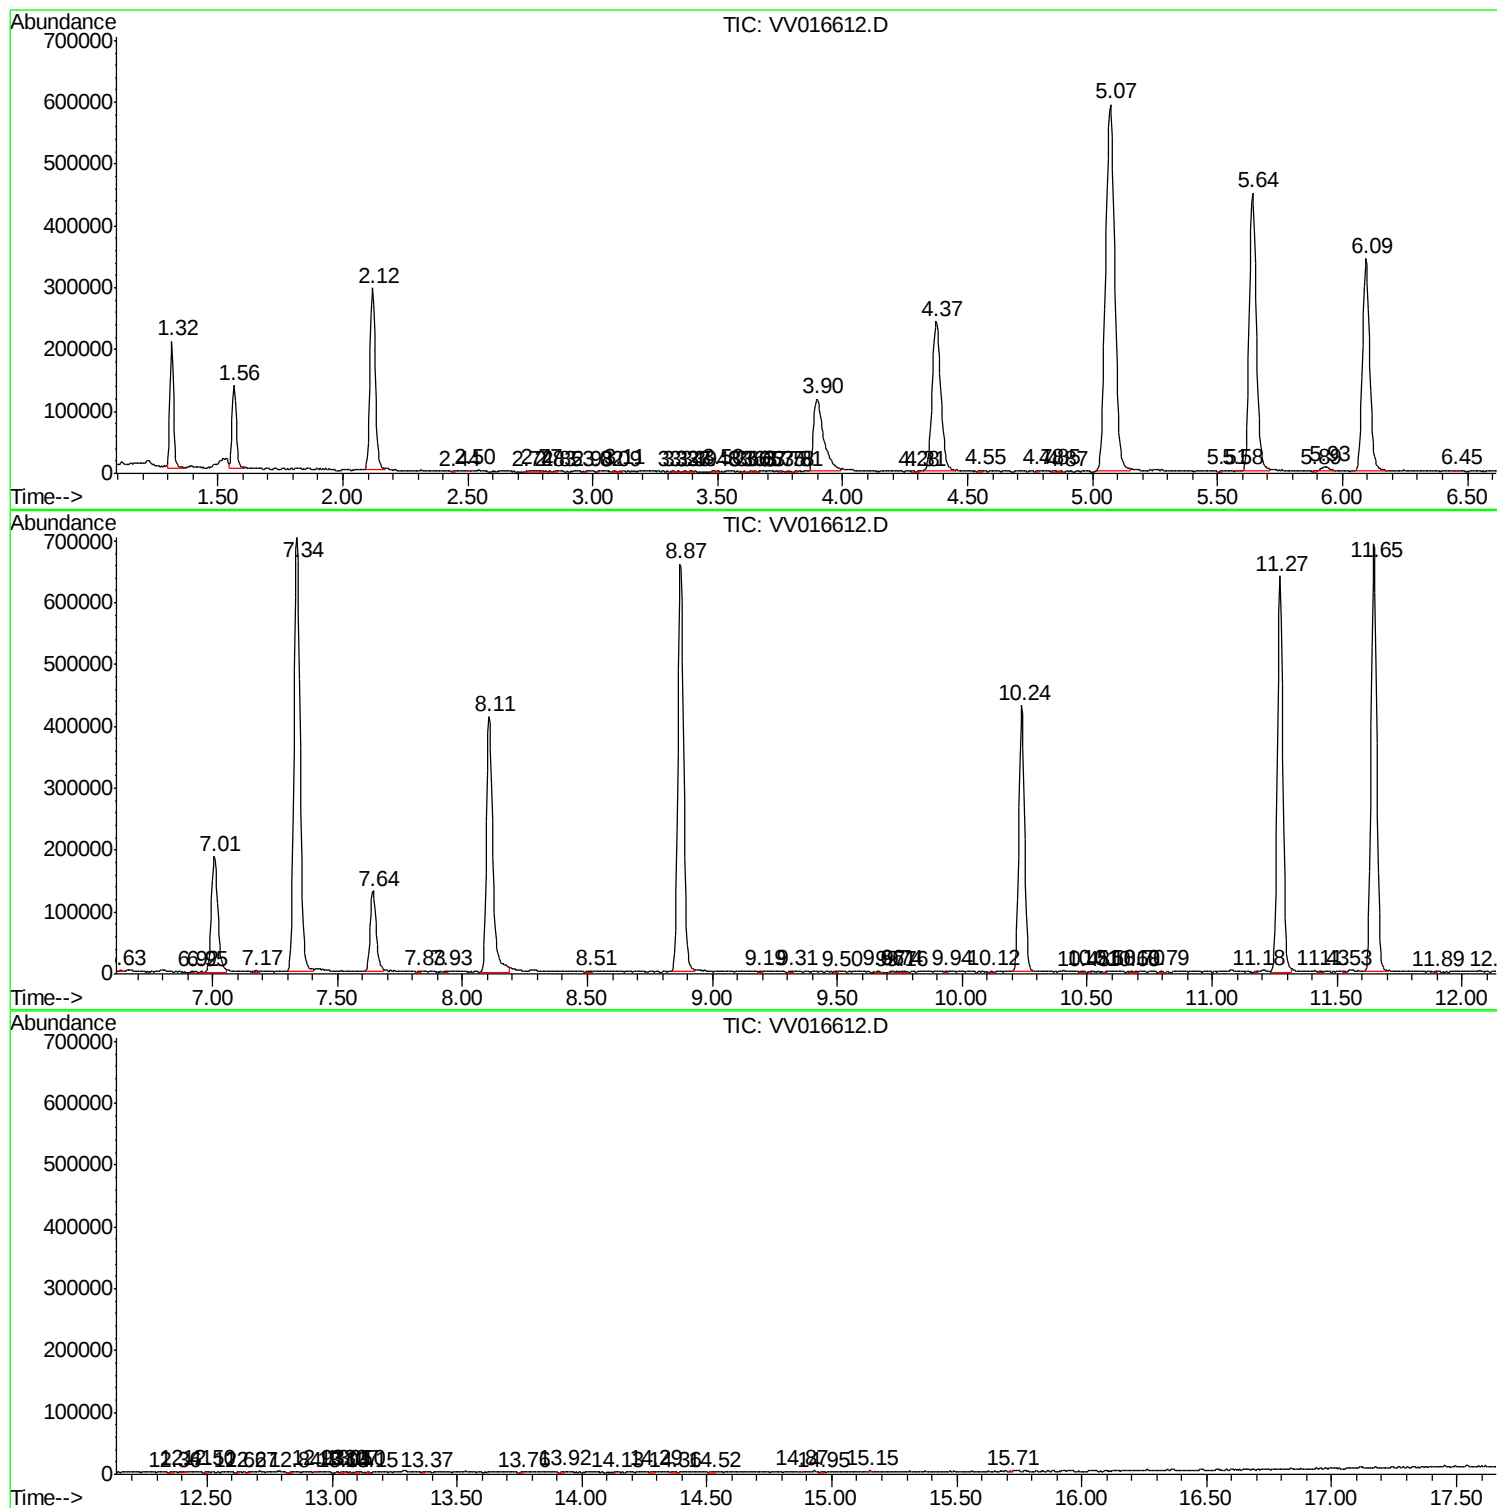

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016612.D
Acq On : 07 Jun 2020 01:22
Operator : SY/MD
Sample : L2875-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016612.D
Acq On : 07 Jun 2020 01:22
Operator : SY/MD
Sample : L2875-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc