

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016613.D
 Acq On : 07 Jun 2020 01:45
 Operator : SY/MD
 Sample : L2875-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	207729	209501	3.22%	1.204%
2	1.563	141	147	158	rVB	131948	152276	2.34%	0.875%
3	2.119	310	320	335	rBV	295053	437040	6.71%	2.512%
4	2.630	477	479	482	rBV3	1367	802	0.01%	0.005%
5	2.666	488	490	491	rBV2	1466	712	0.01%	0.004%
6	2.778	513	525	539	rBV	46137	83730	1.29%	0.481%
7	2.923	565	570	571	rBV4	1857	1548	0.02%	0.009%
8	3.036	601	605	610	rVV7	1586	1190	0.02%	0.007%
9	3.090	620	622	624	rBV3	1096	665	0.01%	0.004%
10	3.122	630	632	635	rVB3	2105	1017	0.02%	0.006%
11	3.138	635	637	640	rBV3	1529	1179	0.02%	0.007%
12	3.200	652	656	658	rBV4	2198	1698	0.03%	0.010%
13	3.322	692	694	697	rBV4	1562	1040	0.02%	0.006%
14	3.412	719	722	725	rVV4	1473	927	0.01%	0.005%
15	3.572	769	772	775	rVB4	1286	823	0.01%	0.005%
16	3.592	775	778	779	rBV2	1157	659	0.01%	0.004%
17	3.637	790	792	798	rVB7	1454	914	0.01%	0.005%
18	3.727	815	820	821	rBV4	1006	808	0.01%	0.005%
19	3.794	837	841	843	rBV4	1717	1186	0.02%	0.007%
20	3.836	851	854	858	rVB5	1113	802	0.01%	0.005%
21	3.936	858	885	918	rBV	2607851	6511008	100.00%	37.416%
22	4.373	1008	1021	1043	rVB	235423	564287	8.67%	3.243%
23	4.974	1206	1208	1212	rVB4	1614	1116	0.02%	0.006%
24	5.000	1212	1216	1219	rBV5	2072	1787	0.03%	0.010%
25	5.071	1221	1238	1265	rVV2	581338	1485773	22.82%	8.538%
26	5.354	1324	1326	1330	rVB5	1551	923	0.01%	0.005%
27	5.473	1362	1363	1370	rVB8	1587	1085	0.02%	0.006%
28	5.553	1385	1388	1389	rVV3	1556	817	0.01%	0.005%
29	5.640	1402	1415	1437	rBV	452367	892258	13.70%	5.127%
30	5.929	1492	1505	1516	rBV	8310	19674	0.30%	0.113%
31	6.023	1532	1534	1536	rBV3	1235	660	0.01%	0.004%
32	6.093	1542	1556	1578	rBV	331348	667020	10.24%	3.833%
33	6.463	1667	1671	1674	rBV4	1144	942	0.01%	0.005%
34	6.637	1719	1725	1731	rBV8	2438	3261	0.05%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016613.D
 Acq On : 07 Jun 2020 01:45
 Operator : SY/MD
 Sample : L2875-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.769	1763	1766	1769	rBV4	1380	1041	0.02%	0.006%
36	6.785	1769	1771	1776	rVB4	1171	756	0.01%	0.004%
37	6.836	1785	1787	1790	rBV3	1685	1043	0.02%	0.006%
38	6.894	1802	1805	1809	rBV4	1164	847	0.01%	0.005%
39	6.952	1820	1823	1825	rBV3	1251	902	0.01%	0.005%
40	7.006	1825	1840	1859	rVV	180018	322132	4.95%	1.851%
41	7.170	1887	1891	1893	rBV4	1827	1619	0.02%	0.009%
42	7.338	1927	1943	1961	rBV	686531	1186884	18.23%	6.821%
43	7.643	2028	2038	2057	rBV	126542	211620	3.25%	1.216%
44	7.823	2091	2094	2098	rBV5	2051	2020	0.03%	0.012%
45	7.942	2127	2131	2132	rBV4	1013	704	0.01%	0.004%
46	8.106	2172	2182	2211	rBV	412019	724441	11.13%	4.163%
47	8.714	2368	2371	2375	rVV6	957	755	0.01%	0.004%
48	8.830	2405	2407	2409	rBV3	1334	896	0.01%	0.005%
49	8.875	2409	2421	2437	rVV	666455	1067554	16.40%	6.135%
50	9.276	2544	2546	2551	rBV5	786	868	0.01%	0.005%
51	9.350	2565	2569	2571	rBV3	1201	901	0.01%	0.005%
52	9.424	2588	2592	2596	rVB6	1016	997	0.02%	0.006%
53	9.450	2596	2600	2602	rBV5	1188	948	0.01%	0.005%
54	9.637	2656	2658	2661	rVB4	1466	734	0.01%	0.004%
55	9.659	2661	2665	2669	rBV6	1210	1414	0.02%	0.008%
56	9.826	2711	2717	2719	rBV5	1463	1755	0.03%	0.010%
57	9.955	2748	2757	2758	rBV7	1454	1430	0.02%	0.008%
58	10.141	2812	2815	2817	rBV3	1163	727	0.01%	0.004%
59	10.238	2832	2845	2862	rBV	425242	670159	10.29%	3.851%
60	10.328	2869	2873	2876	rVB4	1663	1320	0.02%	0.008%
61	10.505	2925	2928	2931	rBV4	2278	1476	0.02%	0.008%
62	10.527	2931	2935	2939	rVV5	1169	1231	0.02%	0.007%
63	10.572	2944	2949	2952	rBV6	1489	1311	0.02%	0.008%
64	10.588	2952	2954	2959	rVB5	1341	1007	0.02%	0.006%
65	10.682	2981	2983	2986	rBV4	1511	955	0.01%	0.005%
66	10.781	3011	3014	3018	rBV5	1427	1243	0.02%	0.007%
67	10.829	3027	3029	3032	rVB3	2029	943	0.01%	0.005%
68	10.929	3057	3060	3064	rBV5	1453	1320	0.02%	0.008%
69	11.074	3103	3105	3109	rVV5	1061	657	0.01%	0.004%
70	11.270	3155	3166	3182	rBV	661451	1016032	15.60%	5.839%
71	11.444	3218	3220	3226	rVB6	1658	1065	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016613.D
 Acq On : 07 Jun 2020 01:45
 Operator : SY/MD
 Sample : L2875-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.485	3230	3233	3236	rBV5	2092	1455	0.02%	0.008%
73	11.505	3236	3239	3243	rVB4	1475	893	0.01%	0.005%
74	11.646	3271	3283	3303	rBV	705582	1088763	16.72%	6.257%
75	11.913	3364	3366	3371	rVB5	1437	1049	0.02%	0.006%
76	11.993	3388	3391	3394	rBV5	1228	739	0.01%	0.004%
77	12.112	3426	3428	3431	rBV4	999	712	0.01%	0.004%
78	12.144	3436	3438	3445	rVB7	1112	998	0.02%	0.006%
79	12.177	3445	3448	3454	rBV6	954	1027	0.02%	0.006%
80	12.556	3562	3566	3568	rBV5	1334	936	0.01%	0.005%
81	12.974	3693	3696	3699	rBV3	862	800	0.01%	0.005%
82	13.000	3701	3704	3707	rBV4	1401	927	0.01%	0.005%
83	13.016	3707	3709	3714	rVB6	1648	1291	0.02%	0.007%
84	13.038	3714	3716	3719	rBV3	1057	699	0.01%	0.004%
85	13.193	3760	3764	3766	rBV5	1772	1073	0.02%	0.006%
86	13.292	3789	3795	3802	rBV10	2368	3659	0.06%	0.021%
87	13.334	3806	3808	3811	rBV3	1243	743	0.01%	0.004%
88	13.411	3827	3832	3834	rBV5	1222	923	0.01%	0.005%
89	13.460	3844	3847	3852	rBV5	1979	1985	0.03%	0.011%
90	13.598	3883	3890	3897	rBV5	1198	1819	0.03%	0.010%
91	13.897	3980	3983	3985	rBV4	1779	870	0.01%	0.005%
92	13.961	4001	4003	4006	rBV3	1576	1043	0.02%	0.006%
93	14.042	4026	4028	4032	rBV5	1261	988	0.02%	0.006%
94	14.170	4065	4068	4070	rBV4	1451	918	0.01%	0.005%
95	14.498	4166	4170	4172	rBV4	1704	1235	0.02%	0.007%
96	14.566	4189	4191	4194	rBV4	1228	824	0.01%	0.005%
97	14.611	4200	4205	4207	rBV6	1624	1449	0.02%	0.008%
98	14.659	4218	4220	4225	rBV6	1202	935	0.01%	0.005%
99	14.791	4260	4261	4266	rVB4	1616	873	0.01%	0.005%
100	15.045	4337	4340	4343	rBV4	1569	1068	0.02%	0.006%


Sum of corrected areas: 17401529

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016613.D
Acq On : 07 Jun 2020 01:45
Operator : SY/MD
Sample : L2875-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

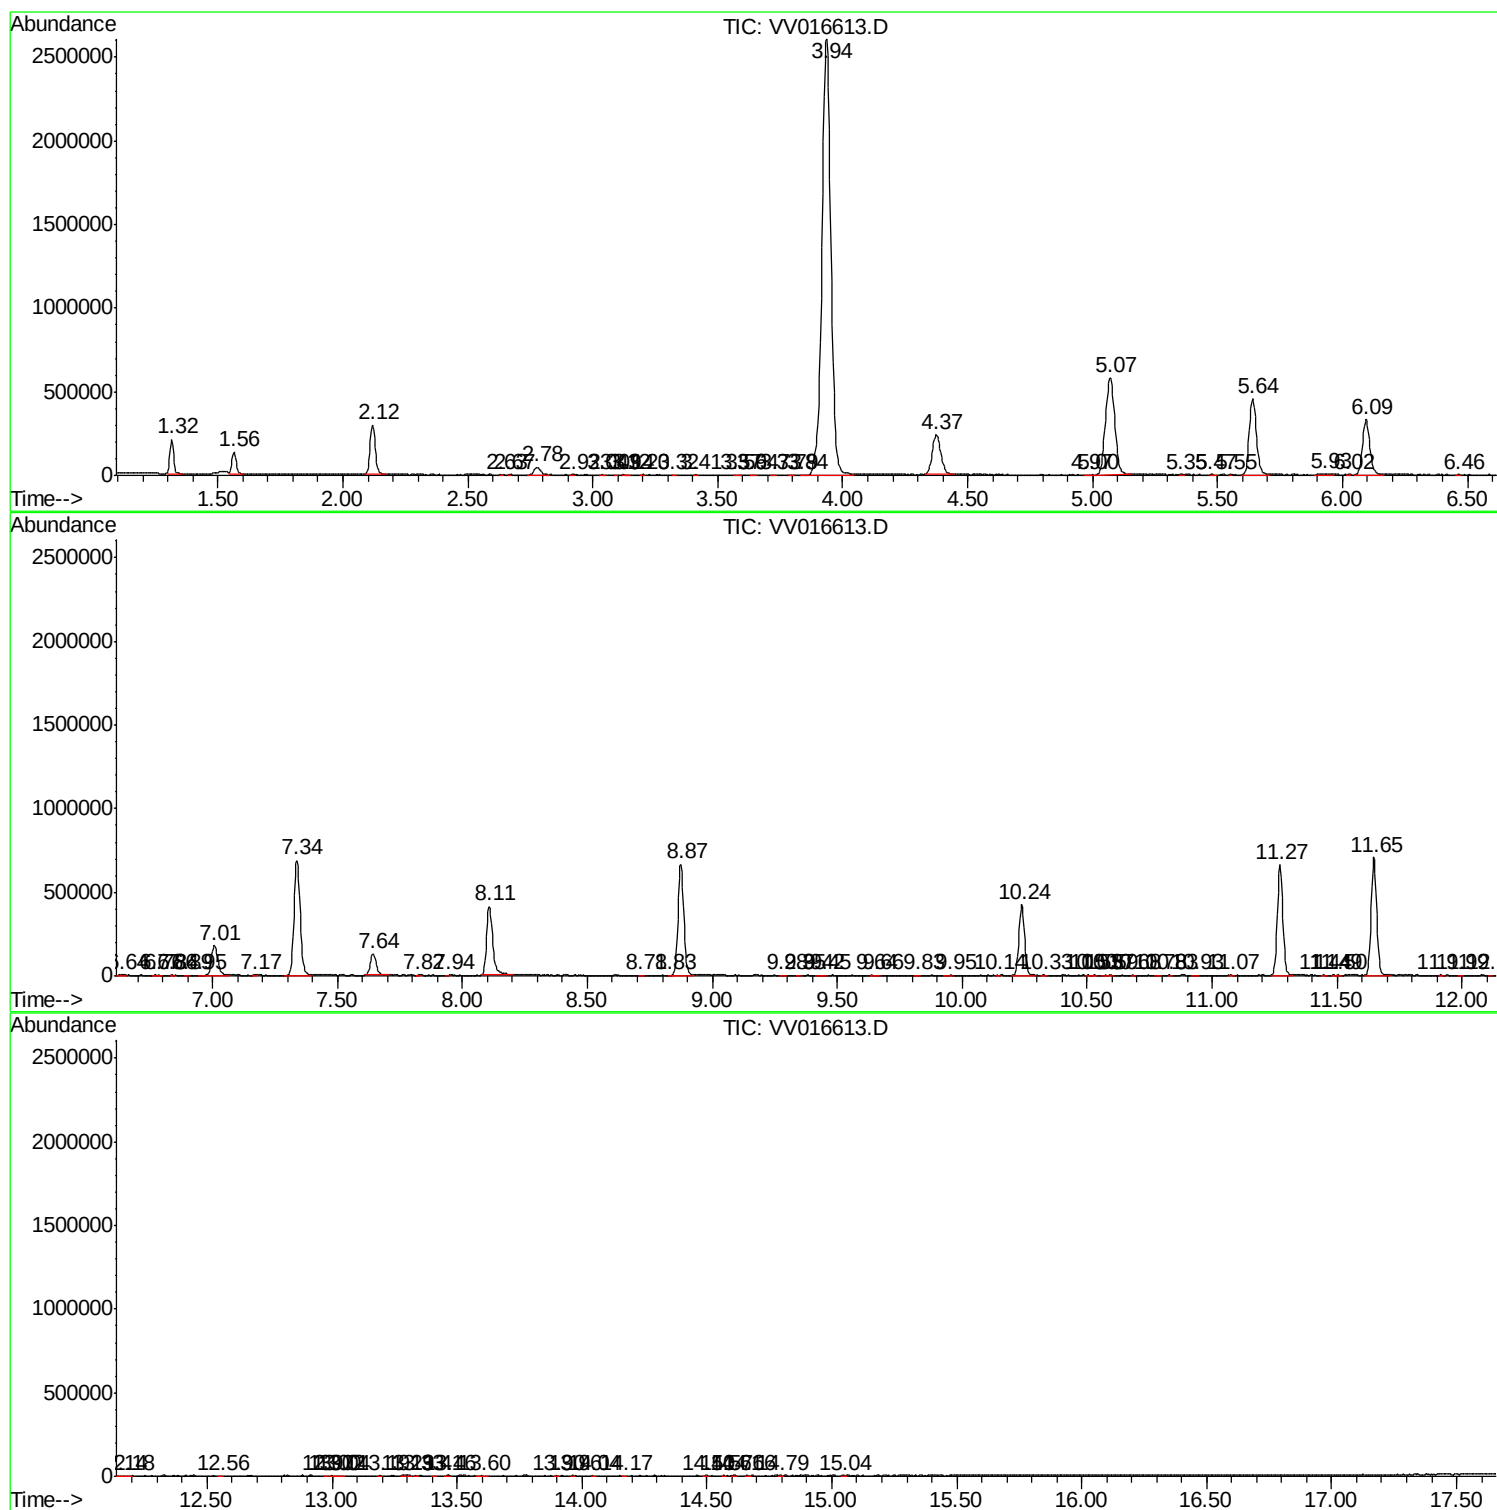

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016613.D
Acq On : 07 Jun 2020 01:45
Operator : SY/MD
Sample : L2875-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016613.D
Acq On : 07 Jun 2020 01:45
Operator : SY/MD
Sample : L2875-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc