

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016615.D
 Acq On : 07 Jun 2020 02:33
 Operator : SY/MD
 Sample : L2875-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	186085	191980	13.23%	1.766%
2	1.563	141	147	160	rVB	127074	152619	10.52%	1.404%
3	2.119	310	320	336	rBV	288372	424239	29.24%	3.903%
4	2.810	533	535	537	rBV3	1123	548	0.04%	0.005%
5	2.836	541	543	544	rBV2	1002	428	0.03%	0.004%
6	2.952	577	579	582	rVV4	826	427	0.03%	0.004%
7	3.064	612	614	617	rVB4	1323	501	0.03%	0.005%
8	3.113	624	629	632	rVB7	953	840	0.06%	0.008%
9	3.129	632	634	638	rBV4	939	846	0.06%	0.008%
10	3.183	647	651	655	rVB6	1587	1241	0.09%	0.011%
11	3.216	656	661	663	rBV5	1243	1036	0.07%	0.010%
12	3.338	696	699	702	rVB4	1358	769	0.05%	0.007%
13	3.360	702	706	708	rBV5	1505	1246	0.09%	0.011%
14	3.383	711	713	715	rVB3	868	362	0.02%	0.003%
15	3.415	720	723	726	rBV3	1483	1290	0.09%	0.012%
16	3.544	762	763	765	rBV2	742	351	0.02%	0.003%
17	3.627	784	789	791	rBV5	1347	1250	0.09%	0.011%
18	3.685	802	807	810	rBV7	1181	674	0.05%	0.006%
19	3.714	813	816	817	rBV4	763	406	0.03%	0.004%
20	3.897	862	873	902	rBV	110743	303844	20.95%	2.795%
21	4.373	1002	1021	1045	rBV	234286	579805	39.97%	5.334%
22	4.650	1104	1107	1111	rBV5	1521	1381	0.10%	0.013%
23	4.807	1154	1156	1158	rVB3	1185	344	0.02%	0.003%
24	5.071	1221	1238	1267	rBV2	567066	1450644	100.00%	13.345%
25	5.640	1403	1415	1435	rBV	452955	893140	61.57%	8.216%
26	6.093	1543	1556	1578	rBV	329072	656984	45.29%	6.044%
27	6.441	1662	1664	1667	rBV3	1312	839	0.06%	0.008%
28	6.633	1717	1724	1728	rBV8	2664	3493	0.24%	0.032%
29	6.775	1766	1768	1772	rBV4	1215	847	0.06%	0.008%
30	7.006	1828	1840	1858	rBV2	175658	312980	21.58%	2.879%
31	7.338	1931	1943	1960	rBV	667178	1155336	79.64%	10.628%
32	7.643	2028	2038	2053	rBV	121160	207005	14.27%	1.904%
33	7.929	2125	2127	2131	rBV4	2116	1222	0.08%	0.011%
34	8.106	2172	2182	2217	rBV	385225	694952	47.91%	6.393%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016615.D
 Acq On : 07 Jun 2020 02:33
 Operator : SY/MD
 Sample : L2875-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	8.405	2271	2275	2276	rBV4	1898	1094	0.08%	0.010%
36	8.495	2301	2303	2304	rBV2	971	366	0.03%	0.003%
37	8.601	2331	2336	2339	rBV7	1471	1574	0.11%	0.014%
38	8.621	2340	2342	2344	rVV3	1118	424	0.03%	0.004%
39	8.682	2357	2361	2362	rBV3	975	633	0.04%	0.006%
40	8.727	2373	2375	2378	rBV4	1374	1003	0.07%	0.009%
41	8.756	2382	2384	2387	rVB4	831	503	0.03%	0.005%
42	8.875	2409	2421	2442	rBV	659792	1068211	73.64%	9.827%
43	9.151	2504	2507	2508	rBV3	1895	1089	0.08%	0.010%
44	9.228	2526	2531	2532	rBV4	2020	1532	0.11%	0.014%
45	9.280	2544	2547	2550	rBV4	824	798	0.06%	0.007%
46	9.299	2550	2553	2559	rVV7	1481	1364	0.09%	0.013%
47	9.479	2605	2609	2613	rBV6	1348	1368	0.09%	0.013%
48	9.524	2620	2623	2626	rBV4	1574	1014	0.07%	0.009%
49	9.643	2658	2660	2664	rBV4	931	589	0.04%	0.005%
50	9.807	2709	2711	2714	rBV3	830	616	0.04%	0.006%
51	9.923	2744	2747	2751	rVB6	1370	1115	0.08%	0.010%
52	9.952	2751	2756	2760	rBV7	1866	1787	0.12%	0.016%
53	10.006	2770	2773	2774	rBV4	1092	481	0.03%	0.004%
54	10.071	2791	2793	2795	rVB3	1042	404	0.03%	0.004%
55	10.083	2795	2797	2799	rBV2	713	429	0.03%	0.004%
56	10.096	2799	2801	2804	rVV4	1012	458	0.03%	0.004%
57	10.154	2816	2819	2822	rBV4	1072	832	0.06%	0.008%
58	10.238	2833	2845	2861	rBV	415314	637385	43.94%	5.864%
59	10.466	2913	2916	2918	rBV5	1084	850	0.06%	0.008%
60	10.592	2953	2955	2963	rBV8	1737	1842	0.13%	0.017%
61	10.672	2976	2980	2981	rBV3	743	493	0.03%	0.005%
62	10.688	2981	2985	2987	rBV3	1038	812	0.06%	0.007%
63	10.736	2995	3000	3002	rBV4	1417	1299	0.09%	0.012%
64	10.826	3023	3028	3030	rBV4	1321	1219	0.08%	0.011%
65	10.852	3034	3036	3040	rVB4	1277	754	0.05%	0.007%
66	10.913	3053	3055	3056	rBV3	1097	602	0.04%	0.006%
67	11.122	3116	3120	3125	rVB5	1212	1101	0.08%	0.010%
68	11.161	3130	3132	3134	rBV3	1805	1060	0.07%	0.010%
69	11.270	3153	3166	3181	rBV	644429	992198	68.40%	9.128%
70	11.492	3232	3235	3238	rBV3	1037	840	0.06%	0.008%
71	11.556	3247	3255	3271	rBV7	10393	21248	1.46%	0.195%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016615.D
 Acq On : 07 Jun 2020 02:33
 Operator : SY/MD
 Sample : L2875-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3301	rVV	671067	1052950	72.59%	9.686%
73	11.817	3334	3336	3338	rBV3	1618	958	0.07%	0.009%
74	11.862	3349	3350	3352	rBV2	904	440	0.03%	0.004%
75	11.923	3367	3369	3370	rBV2	1187	592	0.04%	0.005%
76	12.038	3402	3405	3408	rBV5	1618	1026	0.07%	0.009%
77	12.109	3422	3427	3430	rBV5	1729	1567	0.11%	0.014%
78	12.321	3492	3493	3496	rBV2	1197	474	0.03%	0.004%
79	12.363	3500	3506	3507	rBV5	2836	2338	0.16%	0.022%
80	12.440	3527	3530	3533	rBV4	1943	1442	0.10%	0.013%
81	12.521	3553	3555	3557	rBV4	1011	512	0.04%	0.005%
82	12.569	3568	3570	3573	rBV3	1158	689	0.05%	0.006%
83	12.633	3587	3590	3591	rBV3	962	481	0.03%	0.004%
84	12.984	3697	3699	3702	rVB2	1632	879	0.06%	0.008%
85	13.064	3722	3724	3728	rVB5	1601	904	0.06%	0.008%
86	13.087	3729	3731	3734	rBV3	1148	643	0.04%	0.006%
87	13.312	3798	3801	3803	rBV4	1314	921	0.06%	0.008%
88	13.341	3807	3810	3812	rBV4	865	739	0.05%	0.007%
89	13.379	3820	3822	3826	rVB5	1325	778	0.05%	0.007%
90	13.424	3834	3836	3839	rBV3	1054	584	0.04%	0.005%
91	13.443	3839	3842	3845	rBV3	1190	978	0.07%	0.009%
92	13.495	3856	3858	3860	rBV2	1001	586	0.04%	0.005%
93	13.527	3863	3868	3869	rBV4	1852	1409	0.10%	0.013%
94	13.591	3886	3888	3890	rBV2	759	454	0.03%	0.004%
95	13.704	3921	3923	3927	rVB4	1610	958	0.07%	0.009%
96	13.884	3977	3979	3982	rBV3	1431	808	0.06%	0.007%
97	13.939	3993	3996	4000	rBV5	1215	1155	0.08%	0.011%
98	14.353	4122	4125	4126	rBV3	1091	634	0.04%	0.006%
99	14.566	4189	4191	4195	rBV4	1010	683	0.05%	0.006%
100	14.755	4248	4250	4252	rBV3	1113	470	0.03%	0.004%


Sum of corrected areas: 10870308

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016615.D
Acq On : 07 Jun 2020 02:33
Operator : SY/MD
Sample : L2875-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

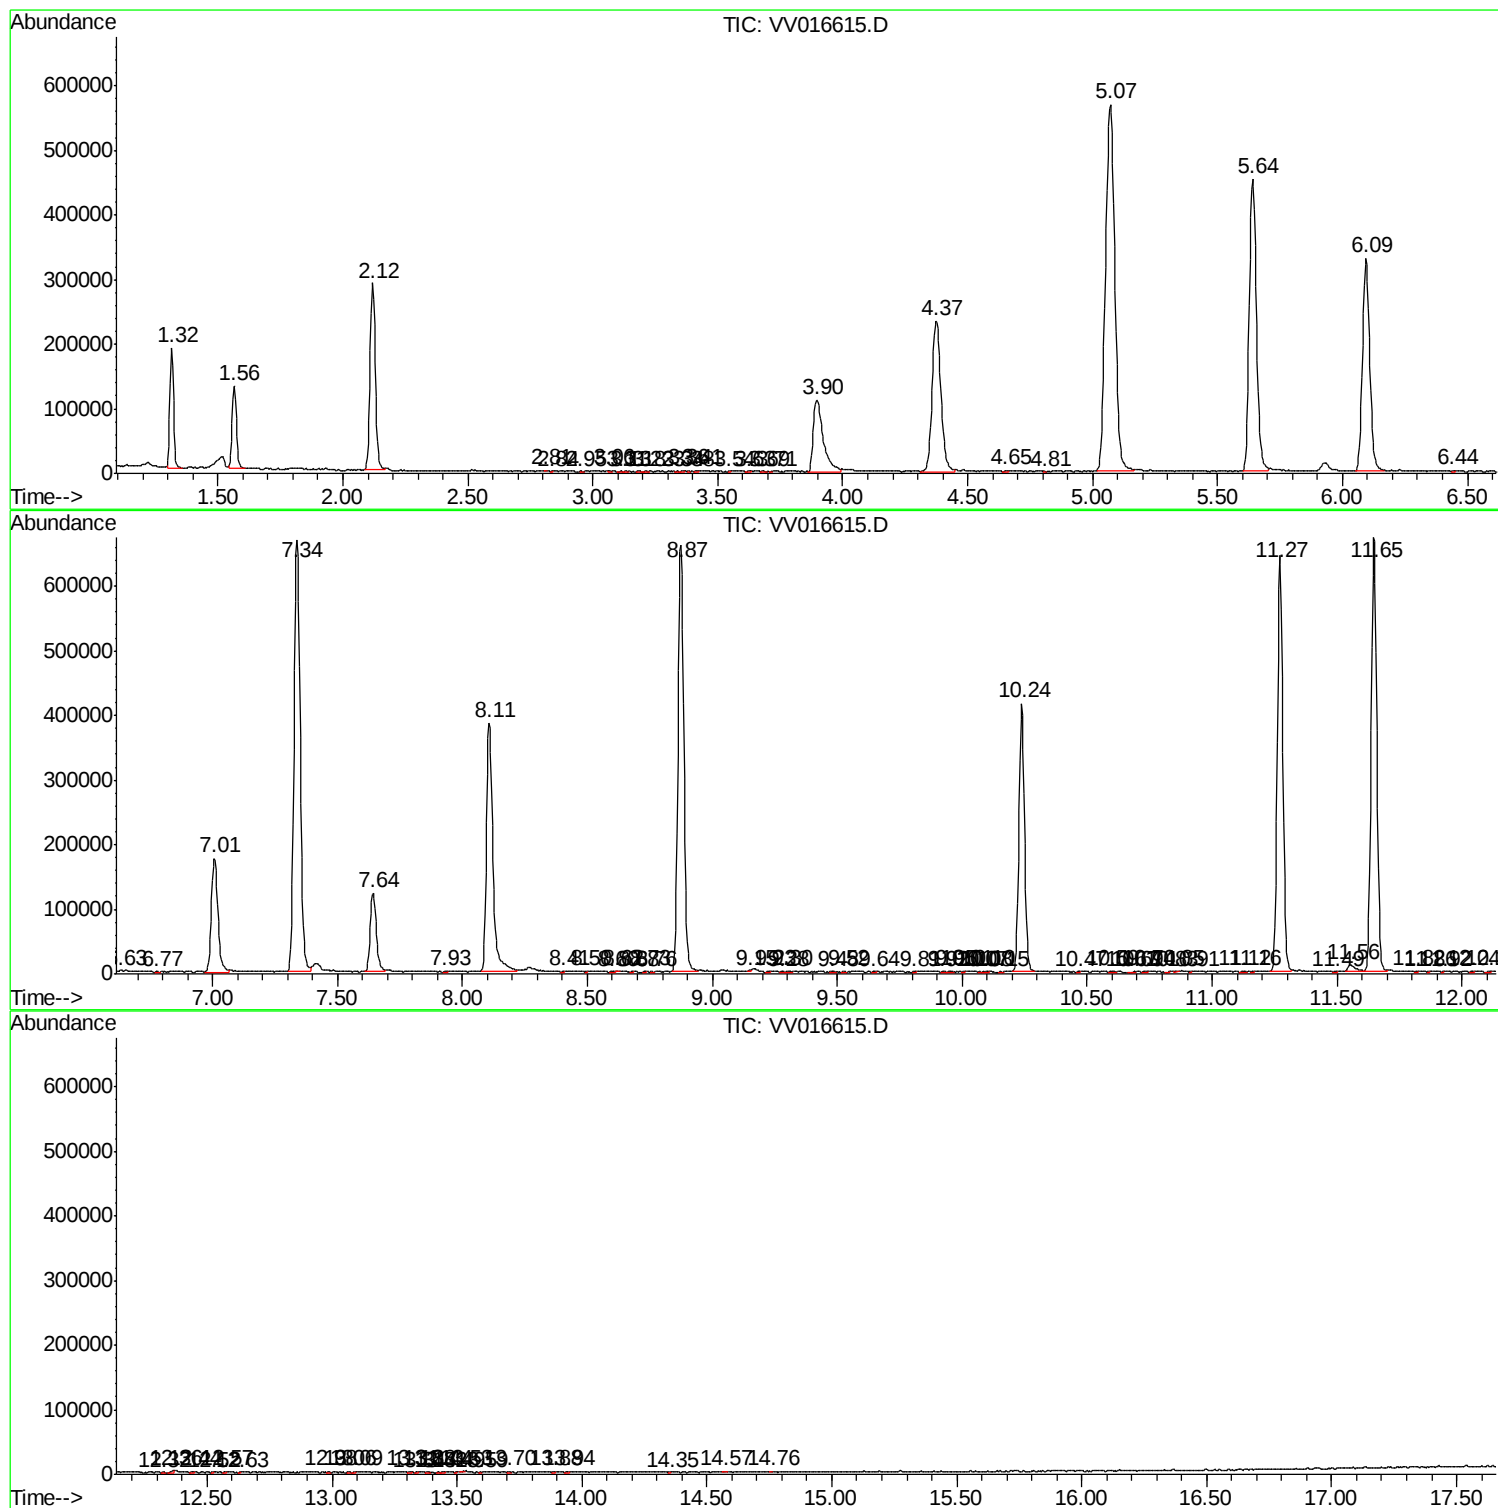

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016615.D
Acq On : 07 Jun 2020 02:33
Operator : SY/MD
Sample : L2875-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016615.D
Acq On : 07 Jun 2020 02:33
Operator : SY/MD
Sample : L2875-14
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc