

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016618.D
 Acq On : 07 Jun 2020 03:44
 Operator : SY/MD
 Sample : L2875-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	189434	196913	13.42%	1.813%
2	1.563	141	147	159	rVB	120532	145969	9.95%	1.344%
3	2.119	309	320	335	rBV	282012	423061	28.83%	3.894%
4	2.502	436	439	440	rBV3	1206	749	0.05%	0.007%
5	2.846	544	546	548	rBV3	1380	903	0.06%	0.008%
6	2.952	577	579	581	rBV3	1392	644	0.04%	0.006%
7	2.968	581	584	585	rBV2	1496	739	0.05%	0.007%
8	3.139	634	637	640	rBV3	1127	796	0.05%	0.007%
9	3.283	679	682	686	rBV5	1109	709	0.05%	0.007%
10	3.312	686	691	693	rBV5	1257	1059	0.07%	0.010%
11	3.521	753	756	760	rBV5	1101	1040	0.07%	0.010%
12	3.682	804	806	810	rVB4	1667	862	0.06%	0.008%
13	3.701	810	812	815	rBV4	1062	616	0.04%	0.006%
14	3.743	819	825	828	rBV8	1238	1226	0.08%	0.011%
15	3.759	828	830	833	rVV3	1065	670	0.05%	0.006%
16	3.778	833	836	839	rVB4	1272	717	0.05%	0.007%
17	3.849	854	858	860	rVB3	1024	664	0.05%	0.006%
18	3.894	860	872	903	rBV	113289	313134	21.34%	2.883%
19	4.167	954	957	959	rBV4	1699	1031	0.07%	0.009%
20	4.206	966	969	972	rBV4	1461	1357	0.09%	0.012%
21	4.309	997	1001	1003	rBV4	1294	926	0.06%	0.009%
22	4.373	1006	1021	1049	rVV	232353	570709	38.89%	5.254%
23	4.524	1064	1068	1070	rBV5	1594	1366	0.09%	0.013%
24	4.778	1145	1147	1150	rVB4	1682	812	0.06%	0.007%
25	4.881	1177	1179	1182	rBV4	1257	689	0.05%	0.006%
26	4.958	1201	1203	1206	rVB4	1336	745	0.05%	0.007%
27	4.981	1208	1210	1213	rVV4	1370	618	0.04%	0.006%
28	5.071	1220	1238	1266	rBV3	572633	1467424	100.00%	13.508%
29	5.322	1313	1316	1319	rBV4	1006	709	0.05%	0.007%
30	5.338	1319	1321	1324	rBV4	1540	1289	0.09%	0.012%
31	5.450	1354	1356	1357	rBV2	1336	609	0.04%	0.006%
32	5.479	1363	1365	1367	rBV3	1422	955	0.07%	0.009%
33	5.502	1370	1372	1374	rVV3	1370	554	0.04%	0.005%
34	5.569	1390	1393	1395	rBV3	1992	1159	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016618.D
 Acq On : 07 Jun 2020 03:44
 Operator : SY/MD
 Sample : L2875-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.640	1400	1415	1438	rBV	441349	874124	59.57%	8.047%
36	5.923	1495	1503	1505	rBV7	7145	9113	0.62%	0.084%
37	5.997	1523	1526	1527	rBV3	1558	946	0.06%	0.009%
38	6.093	1541	1556	1578	rBV	322919	666050	45.39%	6.131%
39	6.386	1645	1647	1649	rBV4	1213	663	0.05%	0.006%
40	6.524	1688	1690	1693	rVV3	1195	658	0.04%	0.006%
41	6.592	1706	1711	1712	rBV5	1216	855	0.06%	0.008%
42	6.891	1801	1804	1808	rBV5	1466	1083	0.07%	0.010%
43	6.942	1817	1820	1822	rBV4	1234	751	0.05%	0.007%
44	7.007	1827	1840	1864	rBV	176753	316744	21.59%	2.916%
45	7.248	1911	1915	1921	rVB7	2072	2186	0.15%	0.020%
46	7.338	1929	1943	1959	rBV	668004	1153819	78.63%	10.622%
47	7.640	2027	2037	2057	rVV	123974	216250	14.74%	1.991%
48	7.772	2076	2078	2083	rVB5	1946	809	0.06%	0.007%
49	8.058	2164	2167	2170	rVV4	1327	872	0.06%	0.008%
50	8.106	2172	2182	2223	rVV	408074	720617	49.11%	6.634%
51	8.550	2318	2320	2324	rBV3	1029	646	0.04%	0.006%
52	8.830	2404	2407	2409	rBV4	1150	862	0.06%	0.008%
53	8.875	2409	2421	2441	rVV	644345	1047661	71.39%	9.644%
54	9.071	2480	2482	2484	rBV2	1034	619	0.04%	0.006%
55	9.376	2571	2577	2579	rBV5	1421	1356	0.09%	0.012%
56	9.447	2597	2599	2602	rVV4	1010	581	0.04%	0.005%
57	9.621	2650	2653	2655	rBV3	1573	1030	0.07%	0.009%
58	9.685	2670	2673	2675	rBV4	1377	913	0.06%	0.008%
59	9.849	2721	2724	2728	rVB5	1022	719	0.05%	0.007%
60	10.058	2788	2789	2793	rBV4	997	693	0.05%	0.006%
61	10.199	2829	2833	2834	rBV2	1780	970	0.07%	0.009%
62	10.238	2834	2845	2860	rVB	417439	652123	44.44%	6.003%
63	10.576	2945	2950	2951	rBV4	1159	883	0.06%	0.008%
64	10.871	3038	3042	3046	rBV7	1264	1096	0.07%	0.010%
65	11.016	3083	3087	3090	rBV6	1465	1575	0.11%	0.014%
66	11.084	3104	3108	3109	rBV4	1314	970	0.07%	0.009%
67	11.135	3121	3124	3125	rBV3	1286	728	0.05%	0.007%
68	11.180	3136	3138	3139	rBV2	1400	552	0.04%	0.005%
69	11.270	3154	3166	3187	rBV	627090	961571	65.53%	8.852%
70	11.389	3202	3203	3208	rVB5	1191	810	0.06%	0.007%
71	11.498	3231	3237	3241	rBV7	1624	1935	0.13%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016618.D
 Acq On : 07 Jun 2020 03:44
 Operator : SY/MD
 Sample : L2875-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.595	3265	3267	3271	rBV3	906	613	0.04%	0.006%
73	11.646	3271	3283	3301	rVV	666838	1052483	71.72%	9.689%
74	11.784	3325	3326	3331	rVB3	1152	568	0.04%	0.005%
75	11.849	3343	3346	3348	rBV3	1072	563	0.04%	0.005%
76	11.929	3368	3371	3372	rBV3	1441	819	0.06%	0.008%
77	12.080	3415	3418	3419	rBV3	1473	825	0.06%	0.008%
78	12.299	3484	3486	3487	rBV	1362	623	0.04%	0.006%
79	12.640	3589	3592	3596	rVV5	1181	828	0.06%	0.008%
80	12.788	3635	3638	3640	rBV4	1847	982	0.07%	0.009%
81	12.871	3662	3664	3671	rVB8	1337	1105	0.08%	0.010%
82	12.900	3671	3673	3675	rBV2	997	577	0.04%	0.005%
83	12.981	3697	3698	3702	rBV4	928	616	0.04%	0.006%
84	13.280	3789	3791	3796	rBV4	1700	1388	0.09%	0.013%
85	13.354	3810	3814	3817	rBV4	1427	1466	0.10%	0.013%
86	13.418	3832	3834	3837	rBV4	1008	610	0.04%	0.006%
87	13.460	3844	3847	3851	rBV4	1481	1187	0.08%	0.011%
88	13.704	3919	3923	3924	rBV5	939	670	0.05%	0.006%
89	13.887	3978	3980	3983	rBV4	1158	776	0.05%	0.007%
90	13.936	3991	3995	3996	rBV3	1396	934	0.06%	0.009%
91	14.000	4011	4015	4016	rBV3	1610	902	0.06%	0.008%
92	14.045	4025	4029	4030	rBV4	1275	804	0.05%	0.007%
93	14.190	4068	4074	4076	rBV6	1556	1302	0.09%	0.012%
94	14.328	4115	4117	4121	rBV5	1292	767	0.05%	0.007%
95	14.427	4146	4148	4154	rVB5	1381	1041	0.07%	0.010%
96	14.456	4154	4157	4159	rBV3	1642	986	0.07%	0.009%
97	14.653	4214	4218	4220	rBV4	1813	1508	0.10%	0.014%
98	14.919	4298	4301	4303	rBV4	1278	682	0.05%	0.006%
99	15.103	4355	4358	4362	rBV6	1591	1516	0.10%	0.014%
100	15.315	4422	4424	4426	rBV3	1517	647	0.04%	0.006%


Sum of corrected areas: 10863044

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016618.D
Acq On : 07 Jun 2020 03:44
Operator : SY/MD
Sample : L2875-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

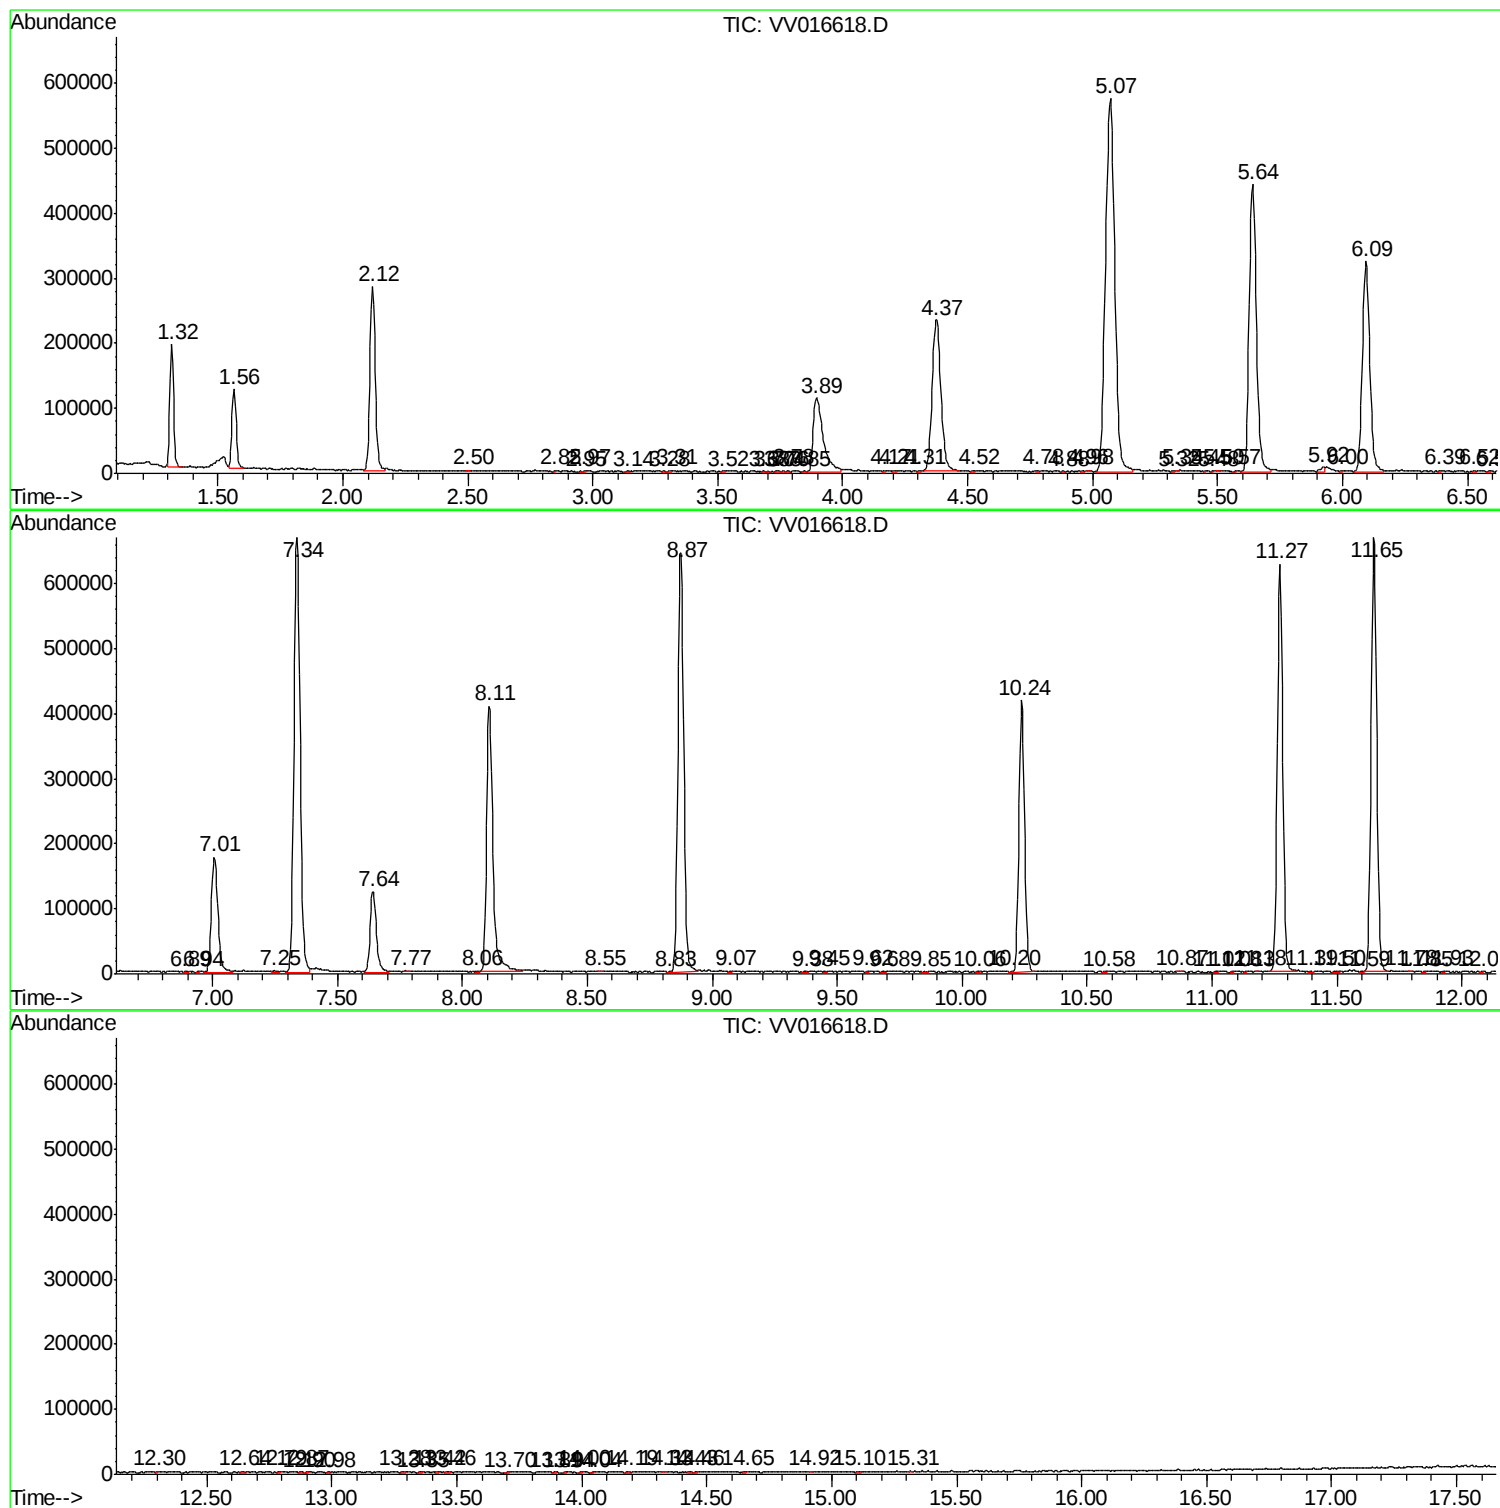

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016618.D
Acq On : 07 Jun 2020 03:44
Operator : SY/MD
Sample : L2875-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016618.D
Acq On : 07 Jun 2020 03:44
Operator : SY/MD
Sample : L2875-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc