

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016621.D
 Acq On : 07 Jun 2020 04:55
 Operator : SY/MD
 Sample : L2875-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	181625	189259	12.86%	1.743%
2	1.563	143	147	157	rVB	126213	140106	9.52%	1.291%
3	2.119	310	320	336	rBV	288070	425099	28.88%	3.916%
4	2.248	356	360	363	rVB5	1338	883	0.06%	0.008%
5	2.441	416	420	422	rBV4	1792	1146	0.08%	0.011%
6	2.762	514	520	521	rBV4	1853	1750	0.12%	0.016%
7	2.930	566	572	575	rBV7	1044	1097	0.07%	0.010%
8	3.026	600	602	605	rVB4	1584	696	0.05%	0.006%
9	3.045	605	608	610	rBV2	1413	963	0.07%	0.009%
10	3.151	639	641	645	rVB4	1096	701	0.05%	0.006%
11	3.213	652	660	663	rBV7	1790	2028	0.14%	0.019%
12	3.370	707	709	717	rBV7	1327	1349	0.09%	0.012%
13	3.418	721	724	728	rVB4	1417	835	0.06%	0.008%
14	3.447	730	733	735	rBV3	916	688	0.05%	0.006%
15	3.512	750	753	756	rBV3	1294	988	0.07%	0.009%
16	3.589	775	777	780	rBV5	1505	1007	0.07%	0.009%
17	3.737	820	823	826	rVB3	1776	844	0.06%	0.008%
18	3.814	845	847	851	rBV4	1201	908	0.06%	0.008%
19	3.846	851	857	858	rBV4	1303	866	0.06%	0.008%
20	3.897	862	873	899	rBV	112199	306582	20.83%	2.824%
21	4.222	972	974	978	rVB5	1462	749	0.05%	0.007%
22	4.290	991	995	996	rBV4	968	696	0.05%	0.006%
23	4.373	1006	1021	1043	rBV	231948	563820	38.31%	5.193%
24	4.682	1115	1117	1119	rBV3	1103	633	0.04%	0.006%
25	4.749	1133	1138	1139	rBV3	990	707	0.05%	0.007%
26	4.791	1148	1151	1155	rVB7	1210	1042	0.07%	0.010%
27	4.811	1155	1157	1161	rBV4	1109	889	0.06%	0.008%
28	4.849	1164	1169	1174	rBV7	975	1196	0.08%	0.011%
29	4.952	1198	1201	1204	rBV3	1736	1100	0.07%	0.010%
30	5.071	1220	1238	1269	rBV2	574806	1471776	100.00%	13.557%
31	5.402	1339	1341	1346	rBV6	1481	1053	0.07%	0.010%
32	5.640	1402	1415	1438	rBV	445839	881476	59.89%	8.119%
33	5.926	1492	1504	1505	rBV10	9149	10627	0.72%	0.098%
34	6.093	1541	1556	1574	rVV	326921	658599	44.75%	6.066%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016621.D
 Acq On : 07 Jun 2020 04:55
 Operator : SY/MD
 Sample : L2875-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.277	1611	1613	1620	rVB8	1754	1023	0.07%	0.009%
36	6.367	1638	1641	1642	rBV4	1536	896	0.06%	0.008%
37	6.447	1662	1666	1668	rBV4	1500	1128	0.08%	0.010%
38	6.772	1765	1767	1772	rBV6	1088	905	0.06%	0.008%
39	6.814	1776	1780	1781	rBV4	1581	1239	0.08%	0.011%
40	6.855	1791	1793	1795	rBV2	1074	641	0.04%	0.006%
41	6.878	1795	1800	1804	rVV6	1404	1499	0.10%	0.014%
42	6.926	1810	1815	1818	rBV6	2754	2125	0.14%	0.020%
43	7.007	1829	1840	1859	rBV2	171387	311116	21.14%	2.866%
44	7.171	1887	1891	1892	rBV3	1674	1195	0.08%	0.011%
45	7.286	1923	1927	1930	rBV5	1568	1342	0.09%	0.012%
46	7.338	1931	1943	1961	rBV	673036	1157036	78.61%	10.658%
47	7.643	2027	2038	2054	rBV	123286	209339	14.22%	1.928%
48	7.833	2095	2097	2103	rBV7	1382	1356	0.09%	0.012%
49	7.968	2130	2139	2146	rBV7	3424	6465	0.44%	0.060%
50	8.000	2146	2149	2153	rVV5	1302	1081	0.07%	0.010%
51	8.106	2170	2182	2213	rBV	391967	708570	48.14%	6.527%
52	8.572	2324	2327	2329	rBV3	1272	768	0.05%	0.007%
53	8.656	2350	2353	2355	rVB4	1759	1010	0.07%	0.009%
54	8.695	2363	2365	2368	rVV3	1381	715	0.05%	0.007%
55	8.833	2404	2408	2409	rBV3	2413	1515	0.10%	0.014%
56	8.875	2410	2421	2442	rVV	657746	1065125	72.37%	9.811%
57	9.270	2542	2544	2546	rBV3	1312	696	0.05%	0.006%
58	9.357	2569	2571	2576	rBV3	1333	1334	0.09%	0.012%
59	9.563	2631	2635	2638	rBV5	1391	1089	0.07%	0.010%
60	9.810	2706	2712	2717	rVV8	1614	1804	0.12%	0.017%
61	9.836	2717	2720	2723	rBV3	1692	1200	0.08%	0.011%
62	10.122	2806	2809	2812	rBV5	1051	826	0.06%	0.008%
63	10.238	2833	2845	2858	rBV	410331	652802	44.35%	6.013%
64	10.572	2946	2949	2950	rBV2	1395	620	0.04%	0.006%
65	10.592	2953	2955	2957	rVB2	1789	696	0.05%	0.006%
66	10.752	3003	3005	3011	rBV7	1519	1321	0.09%	0.012%
67	10.813	3020	3024	3025	rBV2	1414	877	0.06%	0.008%
68	10.910	3052	3054	3055	rBV2	1615	709	0.05%	0.007%
69	10.932	3060	3061	3069	rVV7	1624	1469	0.10%	0.014%
70	11.006	3082	3084	3090	rVB7	2266	2136	0.15%	0.020%
71	11.039	3090	3094	3097	rBV4	970	736	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016621.D
 Acq On : 07 Jun 2020 04:55
 Operator : SY/MD
 Sample : L2875-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.061	3097	3101	3107	rBV8	1536	1965	0.13%	0.018%
73	11.090	3108	3110	3114	rVB4	1535	914	0.06%	0.008%
74	11.270	3153	3166	3181	rBV	633133	971681	66.02%	8.950%
75	11.646	3271	3283	3298	rBV	652926	1040286	70.68%	9.582%
76	12.087	3415	3420	3423	rBV6	1186	1144	0.08%	0.011%
77	12.109	3426	3427	3431	rBV3	1003	623	0.04%	0.006%
78	12.167	3443	3445	3447	rBV3	1027	612	0.04%	0.006%
79	12.206	3453	3457	3458	rBV4	1674	1047	0.07%	0.010%
80	12.238	3462	3467	3471	rBV8	1849	2247	0.15%	0.021%
81	12.299	3483	3486	3487	rBV	1454	863	0.06%	0.008%
82	12.347	3499	3501	3505	rBV4	1335	776	0.05%	0.007%
83	12.492	3543	3546	3548	rBV4	1732	1029	0.07%	0.009%
84	12.666	3598	3600	3602	rBV3	1452	755	0.05%	0.007%
85	12.820	3646	3648	3651	rBV3	1336	946	0.06%	0.009%
86	12.971	3689	3695	3699	rBV7	2009	2005	0.14%	0.018%
87	12.990	3699	3701	3705	rVB5	1078	637	0.04%	0.006%
88	13.151	3748	3751	3754	rBV3	1540	835	0.06%	0.008%
89	13.379	3819	3822	3824	rVB3	1320	696	0.05%	0.006%
90	13.444	3839	3842	3843	rBV3	1450	741	0.05%	0.007%
91	13.463	3846	3848	3853	rBV4	1098	910	0.06%	0.008%
92	13.624	3894	3898	3901	rBV4	1194	1055	0.07%	0.010%
93	13.736	3930	3933	3935	rBV3	1333	944	0.06%	0.009%
94	14.254	4091	4094	4097	rBV4	1318	1055	0.07%	0.010%
95	14.485	4162	4166	4169	rBV4	1611	1378	0.09%	0.013%
96	14.736	4243	4244	4248	rVB5	1213	756	0.05%	0.007%
97	15.022	4330	4333	4337	rVB4	1959	1530	0.10%	0.014%
98	15.463	4468	4470	4472	rBV3	1388	710	0.05%	0.007%
99	15.688	4537	4540	4541	rBV3	1762	962	0.07%	0.009%
100	15.720	4548	4550	4551	rBV2	1965	736	0.05%	0.007%


Sum of corrected areas: 10856400

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016621.D
Acq On : 07 Jun 2020 04:55
Operator : SY/MD
Sample : L2875-22
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

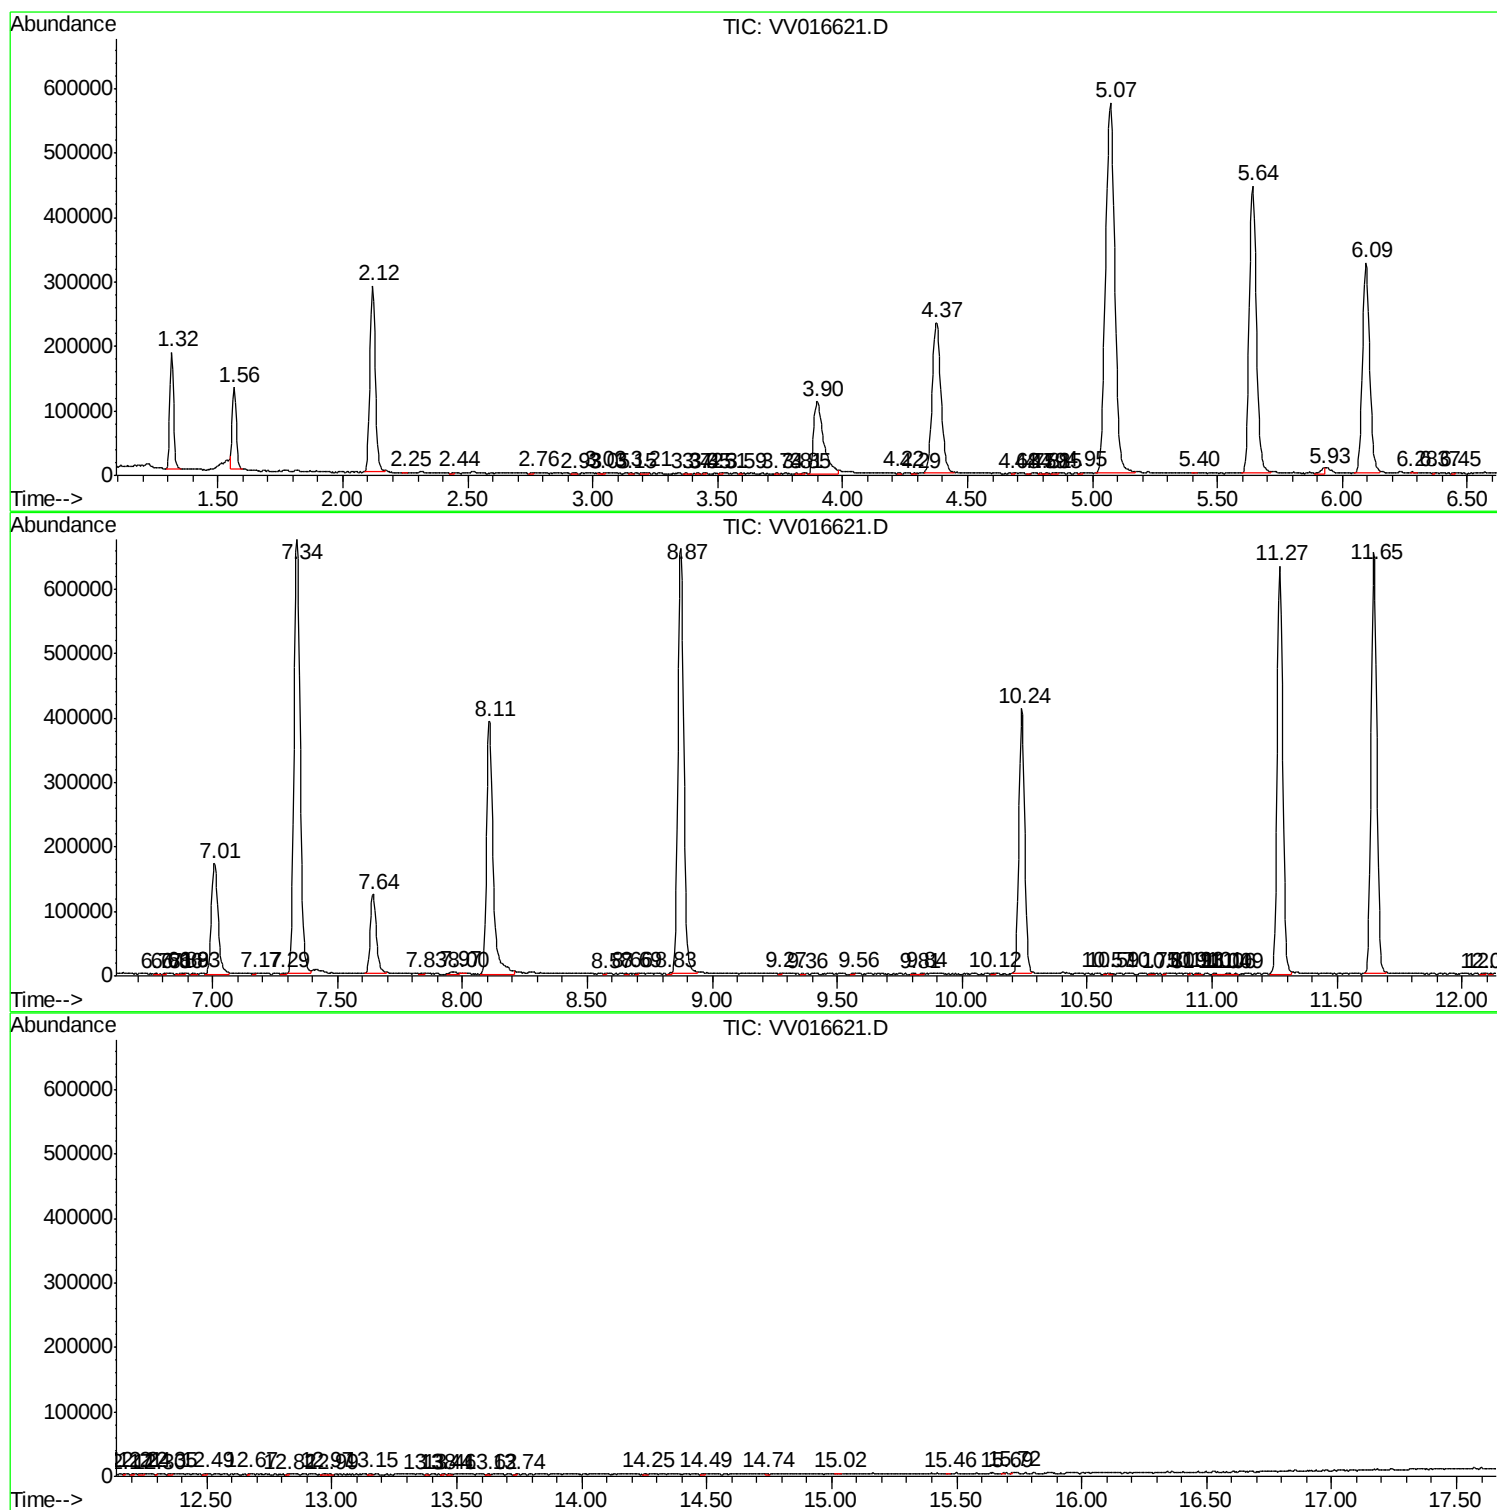

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016621.D
Acq On : 07 Jun 2020 04:55
Operator : SY/MD
Sample : L2875-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016621.D
Acq On : 07 Jun 2020 04:55
Operator : SY/MD
Sample : L2875-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc