

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016622.D
 Acq On : 07 Jun 2020 05:19
 Operator : SY/MD
 Sample : L2875-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	196553	189555	12.66%	1.728%
2	1.569	144	149	159	rVB	112873	122159	8.16%	1.114%
3	2.119	310	320	336	rBV	296601	439632	29.37%	4.008%
4	2.422	410	414	416	rBV5	1133	937	0.06%	0.009%
5	2.460	424	426	431	rVB4	1052	799	0.05%	0.007%
6	2.486	431	434	436	rBV3	1358	874	0.06%	0.008%
7	2.579	458	463	464	rBV4	1064	637	0.04%	0.006%
8	2.608	470	472	475	rBV3	1179	787	0.05%	0.007%
9	2.643	482	483	486	rBV3	1192	760	0.05%	0.007%
10	2.698	498	500	505	rBV4	1405	1038	0.07%	0.009%
11	2.756	515	518	519	rBV3	1293	792	0.05%	0.007%
12	2.939	572	575	578	rVB4	1214	780	0.05%	0.007%
13	3.000	592	594	597	rVB3	1378	746	0.05%	0.007%
14	3.116	627	630	632	rBV3	1285	843	0.06%	0.008%
15	3.277	676	680	687	rVB7	1296	1268	0.08%	0.012%
16	3.518	752	755	756	rBV3	1223	706	0.05%	0.006%
17	3.547	761	764	766	rBV4	1407	997	0.07%	0.009%
18	3.621	785	787	792	rVB5	1100	693	0.05%	0.006%
19	3.643	792	794	797	rBV4	1445	930	0.06%	0.008%
20	3.692	807	809	814	rVB4	1412	683	0.05%	0.006%
21	3.756	826	829	831	rBV3	1174	913	0.06%	0.008%
22	3.782	835	837	841	rVV3	1059	629	0.04%	0.006%
23	3.862	859	862	863	rBV3	1587	718	0.05%	0.007%
24	3.901	863	874	902	rVV	112338	307827	20.57%	2.806%
25	4.290	993	995	998	rVB3	1496	792	0.05%	0.007%
26	4.376	1007	1022	1044	rVB	238612	579683	38.73%	5.285%
27	4.605	1089	1093	1098	rVB6	1151	1090	0.07%	0.010%
28	4.865	1171	1174	1177	rBV4	1393	861	0.06%	0.008%
29	4.891	1180	1182	1186	rVV5	2269	1455	0.10%	0.013%
30	4.936	1189	1196	1198	rBV7	1299	1353	0.09%	0.012%
31	5.007	1216	1218	1220	rBV3	1377	798	0.05%	0.007%
32	5.071	1220	1238	1262	rVV2	587484	1496777	100.00%	13.645%
33	5.454	1355	1357	1363	rVB6	1097	928	0.06%	0.008%
34	5.492	1363	1369	1376	rBV9	1680	2847	0.19%	0.026%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016622.D
 Acq On : 07 Jun 2020 05:19
 Operator : SY/MD
 Sample : L2875-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.640	1400	1415	1435	rBV	452564	902104	60.27%	8.224%
36	6.093	1543	1556	1576	rBV	336357	677307	45.25%	6.175%
37	6.373	1641	1643	1646	rBV4	1016	769	0.05%	0.007%
38	6.521	1687	1689	1692	rBV4	1185	885	0.06%	0.008%
39	6.550	1696	1698	1701	rBV4	1135	732	0.05%	0.007%
40	6.640	1720	1726	1728	rBV7	2274	2366	0.16%	0.022%
41	6.769	1762	1766	1769	rBV5	1361	1095	0.07%	0.010%
42	7.007	1829	1840	1860	rBV	175900	312125	20.85%	2.845%
43	7.257	1916	1918	1924	rVB5	1978	1240	0.08%	0.011%
44	7.289	1924	1928	1930	rBV5	1425	1254	0.08%	0.011%
45	7.338	1931	1943	1961	rBV	686635	1172172	78.31%	10.686%
46	7.643	2028	2038	2058	rBV	125035	210268	14.05%	1.917%
47	7.888	2112	2114	2117	rVB3	1685	750	0.05%	0.007%
48	8.074	2169	2172	2173	rBV3	1308	625	0.04%	0.006%
49	8.106	2173	2182	2219	rVV	395862	714130	47.71%	6.510%
50	8.457	2288	2291	2294	rBV5	1773	1495	0.10%	0.014%
51	8.592	2329	2333	2334	rBV4	1281	787	0.05%	0.007%
52	8.640	2344	2348	2350	rBV6	1614	1147	0.08%	0.010%
53	8.826	2404	2406	2408	rBV3	1154	782	0.05%	0.007%
54	8.875	2409	2421	2443	rVV	663669	1070721	71.54%	9.761%
55	9.074	2481	2483	2486	rBV4	2035	996	0.07%	0.009%
56	9.113	2491	2495	2496	rBV4	1665	906	0.06%	0.008%
57	9.531	2623	2625	2628	rVB4	1447	660	0.04%	0.006%
58	9.572	2635	2638	2643	rBV7	1509	1443	0.10%	0.013%
59	9.624	2652	2654	2658	rBV4	915	714	0.05%	0.007%
60	9.682	2666	2672	2677	rVB8	1268	1261	0.08%	0.011%
61	9.942	2751	2753	2756	rBV3	1656	1017	0.07%	0.009%
62	10.051	2785	2787	2790	rVB3	1421	680	0.05%	0.006%
63	10.080	2794	2796	2798	rBV3	1030	669	0.04%	0.006%
64	10.177	2824	2826	2829	rBV3	1073	664	0.04%	0.006%
65	10.238	2833	2845	2862	rVV	420397	658398	43.99%	6.002%
66	10.633	2966	2968	2972	rVB3	1476	1046	0.07%	0.010%
67	10.752	3002	3005	3006	rBV2	1506	816	0.05%	0.007%
68	10.791	3015	3017	3021	rBV4	1725	1207	0.08%	0.011%
69	10.903	3050	3052	3055	rVB4	1199	607	0.04%	0.006%
70	10.920	3055	3057	3059	rBV3	1356	690	0.05%	0.006%
71	11.183	3135	3139	3141	rBV5	1517	1221	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016622.D
 Acq On : 07 Jun 2020 05:19
 Operator : SY/MD
 Sample : L2875-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3185	rBV	636773	979599	65.45%	8.930%
73	11.646	3270	3283	3299	rBV	667472	1053744	70.40%	9.606%
74	11.891	3355	3359	3363	rBV6	1588	1564	0.10%	0.014%
75	11.920	3363	3368	3370	rBV5	1175	1027	0.07%	0.009%
76	11.993	3389	3391	3393	rBV3	1274	609	0.04%	0.006%
77	12.087	3419	3420	3428	rVB7	1097	953	0.06%	0.009%
78	12.193	3448	3453	3459	rBV10	1345	1692	0.11%	0.015%
79	12.408	3516	3520	3522	rVB4	1326	1080	0.07%	0.010%
80	12.489	3542	3545	3547	rBV4	1745	1188	0.08%	0.011%
81	12.659	3593	3598	3601	rBV3	1495	1076	0.07%	0.010%
82	12.678	3601	3604	3607	rBV3	1221	1056	0.07%	0.010%
83	12.691	3607	3608	3614	rVB5	1360	750	0.05%	0.007%
84	12.813	3643	3646	3650	rBV4	1333	920	0.06%	0.008%
85	12.871	3663	3664	3667	rBV3	1113	655	0.04%	0.006%
86	12.910	3669	3676	3684	rVV3	1827	2722	0.18%	0.025%
87	13.010	3702	3707	3708	rBV3	1142	888	0.06%	0.008%
88	13.125	3741	3743	3746	rBV3	1189	814	0.05%	0.007%
89	13.161	3751	3754	3759	rBV6	1477	1023	0.07%	0.009%
90	13.283	3789	3792	3793	rBV3	1350	785	0.05%	0.007%
91	13.341	3807	3810	3813	rBV5	1450	984	0.07%	0.009%
92	13.524	3862	3867	3868	rBV4	1441	916	0.06%	0.008%
93	13.772	3940	3944	3947	rBV6	1840	1270	0.08%	0.012%
94	14.100	4042	4046	4048	rBV5	1133	927	0.06%	0.008%
95	14.231	4085	4087	4092	rBV4	1120	913	0.06%	0.008%
96	14.476	4160	4163	4165	rBV4	1735	1081	0.07%	0.010%
97	14.656	4217	4219	4221	rBV3	1188	752	0.05%	0.007%
98	14.810	4265	4267	4270	rBV3	1520	1031	0.07%	0.009%
99	15.180	4380	4382	4383	rBV2	1450	631	0.04%	0.006%
100	15.241	4398	4401	4402	rBV2	1289	732	0.05%	0.007%


Sum of corrected areas: 10969418

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016622.D
Acq On : 07 Jun 2020 05:19
Operator : SY/MD
Sample : L2875-23
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

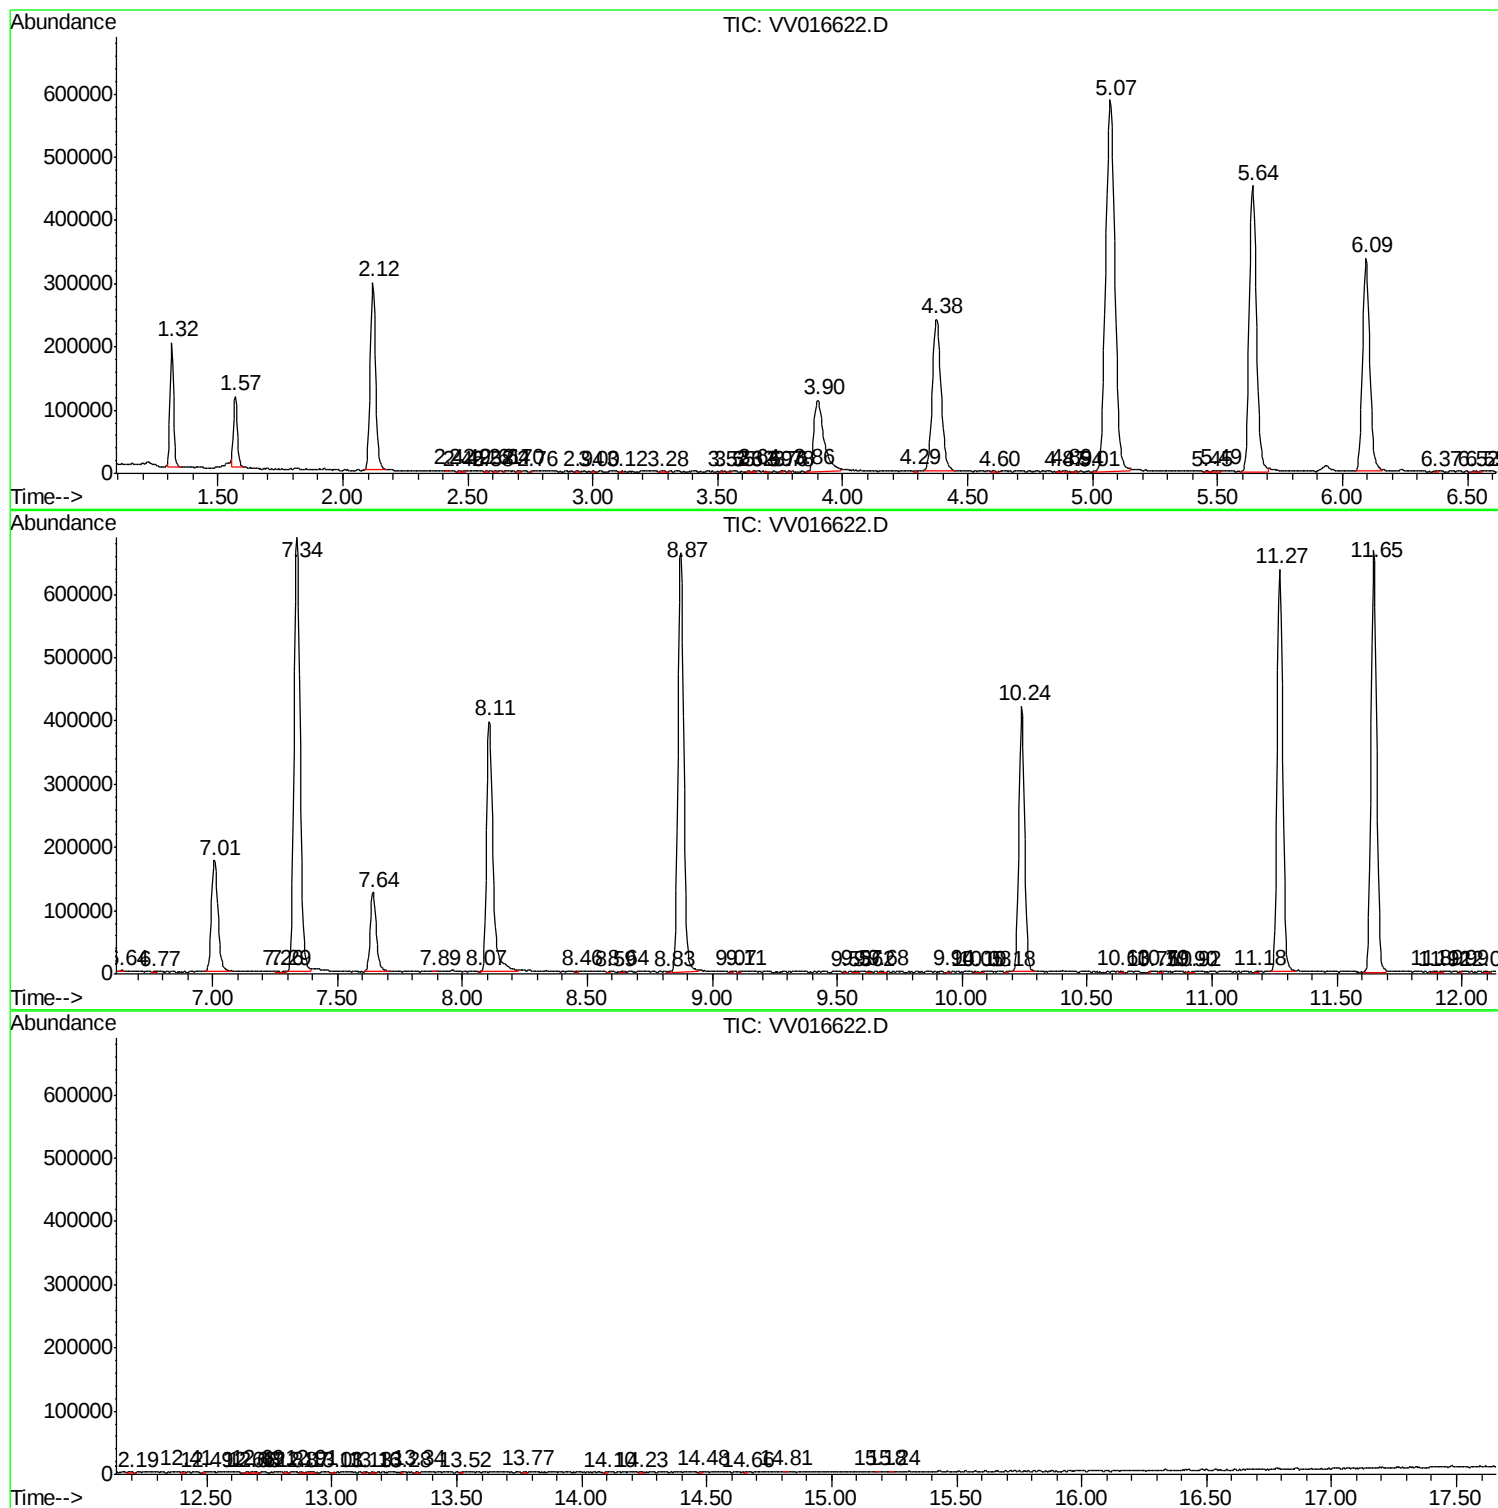

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016622.D
Acq On : 07 Jun 2020 05:19
Operator : SY/MD
Sample : L2875-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016622.D
Acq On : 07 Jun 2020 05:19
Operator : SY/MD
Sample : L2875-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc