

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016624.D
 Acq On : 07 Jun 2020 06:53
 Operator : SY/MD
 Sample : VV0606WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	169076	177648	12.75%	1.708%
2	1.560	141	146	158	rVB	115241	136442	9.79%	1.312%
3	2.119	310	320	336	rVB	262315	391259	28.08%	3.761%
4	2.212	347	349	352	rBV3	1657	1255	0.09%	0.012%
5	2.376	396	400	404	rBV6	1307	1258	0.09%	0.012%
6	2.566	457	459	462	rBV3	895	539	0.04%	0.005%
7	2.923	566	570	571	rBV3	1225	913	0.07%	0.009%
8	2.942	574	576	579	rVB3	1011	625	0.04%	0.006%
9	2.958	579	581	585	rVB5	1461	970	0.07%	0.009%
10	2.987	588	590	594	rBV4	1453	1069	0.08%	0.010%
11	3.090	618	622	626	rVB7	1151	925	0.07%	0.009%
12	3.293	681	685	688	rBV6	794	586	0.04%	0.006%
13	3.380	710	712	715	rVV3	1364	692	0.05%	0.007%
14	3.392	715	716	720	rVB4	1386	960	0.07%	0.009%
15	3.560	766	768	771	rVB4	1604	729	0.05%	0.007%
16	3.592	774	778	780	rBV4	918	574	0.04%	0.006%
17	3.608	780	783	785	rVB3	1102	621	0.04%	0.006%
18	3.843	854	856	858	rBV3	1048	547	0.04%	0.005%
19	3.897	861	873	902	rBV	110415	301853	21.66%	2.902%
20	4.193	961	965	968	rBV6	1417	1215	0.09%	0.012%
21	4.296	993	997	1000	rBV5	1609	1339	0.10%	0.013%
22	4.373	1005	1021	1047	rVV	225726	545975	39.18%	5.248%
23	4.588	1086	1088	1093	rBV5	929	560	0.04%	0.005%
24	4.701	1122	1123	1125	rBV2	1579	840	0.06%	0.008%
25	4.823	1160	1161	1165	rVB3	1163	610	0.04%	0.006%
26	4.855	1165	1171	1174	rBV6	1396	1612	0.12%	0.015%
27	4.926	1191	1193	1196	rVB3	1456	710	0.05%	0.007%
28	5.071	1219	1238	1267	rBV2	546155	1393514	100.00%	13.395%
29	5.460	1355	1359	1361	rBV5	1174	909	0.07%	0.009%
30	5.598	1397	1402	1403	rBV4	1511	1296	0.09%	0.012%
31	5.640	1403	1415	1442	rVV	418816	831910	59.70%	7.997%
32	5.929	1494	1505	1518	rBV10	10609	25918	1.86%	0.249%
33	6.093	1543	1556	1576	rBV	315274	629624	45.18%	6.052%
34	6.479	1673	1676	1677	rVV2	1304	831	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016624.D
 Acq On : 07 Jun 2020 06:53
 Operator : SY/MD
 Sample : VV0606WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.508	1681	1685	1688	rBV5	1579	1539	0.11%	0.015%
36	6.582	1706	1708	1714	rVB5	1261	1155	0.08%	0.011%
37	6.830	1783	1785	1788	rVB4	1431	698	0.05%	0.007%
38	6.881	1799	1801	1804	rBV3	1197	588	0.04%	0.006%
39	7.006	1828	1840	1855	rBV	162373	291705	20.93%	2.804%
40	7.338	1930	1943	1962	rBV	629719	1088164	78.09%	10.460%
41	7.643	2028	2038	2055	rVV2	114800	197910	14.20%	1.902%
42	7.810	2088	2090	2091	rBV2	1089	619	0.04%	0.006%
43	8.042	2158	2162	2164	rVB4	1343	915	0.07%	0.009%
44	8.106	2169	2182	2213	rBV	379609	701335	50.33%	6.741%
45	8.543	2315	2318	2321	rBV4	1399	1099	0.08%	0.011%
46	8.646	2347	2350	2352	rBV4	1350	898	0.06%	0.009%
47	8.874	2409	2421	2438	rBV	618284	999670	71.74%	9.609%
48	9.273	2538	2545	2548	rBV8	1554	1516	0.11%	0.015%
49	9.302	2552	2554	2557	rVB3	1028	666	0.05%	0.006%
50	9.383	2576	2579	2582	rVB4	1280	886	0.06%	0.009%
51	9.434	2592	2595	2596	rBV2	983	539	0.04%	0.005%
52	9.730	2684	2687	2690	rBV5	1116	696	0.05%	0.007%
53	9.775	2698	2701	2704	rBV5	1383	830	0.06%	0.008%
54	9.942	2749	2753	2754	rBV3	2386	1612	0.12%	0.015%
55	10.077	2790	2795	2799	rVB6	2024	1594	0.11%	0.015%
56	10.103	2799	2803	2804	rBV4	1148	727	0.05%	0.007%
57	10.128	2808	2811	2813	rBV2	1128	852	0.06%	0.008%
58	10.161	2819	2821	2824	rVB3	1452	756	0.05%	0.007%
59	10.238	2833	2845	2861	rVV	412077	644337	46.24%	6.194%
60	10.376	2885	2888	2894	rBV8	1603	1060	0.08%	0.010%
61	10.456	2908	2913	2915	rBV4	1139	1029	0.07%	0.010%
62	10.530	2931	2936	2937	rBV4	1612	1170	0.08%	0.011%
63	10.633	2965	2968	2970	rBV3	1645	1029	0.07%	0.010%
64	10.656	2973	2975	2979	rVB5	1499	1020	0.07%	0.010%
65	10.923	3054	3058	3059	rBV3	966	539	0.04%	0.005%
66	11.016	3084	3087	3089	rVV3	1312	741	0.05%	0.007%
67	11.054	3096	3099	3101	rBV4	1259	698	0.05%	0.007%
68	11.077	3103	3106	3111	rVB6	1628	1476	0.11%	0.014%
69	11.116	3112	3118	3121	rBV8	1002	1144	0.08%	0.011%
70	11.270	3155	3166	3188	rVB	611436	945434	67.85%	9.088%
71	11.646	3272	3283	3304	rBV	654501	1019736	73.18%	9.802%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016624.D
 Acq On : 07 Jun 2020 06:53
 Operator : SY/MD
 Sample : VV0606WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.768	3320	3321	3325	rVB4	1389	729	0.05%	0.007%
73	11.945	3374	3376	3377	rBV2	1213	610	0.04%	0.006%
74	11.977	3384	3386	3389	rBV3	1363	1030	0.07%	0.010%
75	12.009	3394	3396	3399	rVV4	1520	784	0.06%	0.008%
76	12.067	3410	3414	3416	rBV4	1283	871	0.06%	0.008%
77	12.151	3437	3440	3442	rBV3	1053	795	0.06%	0.008%
78	12.331	3494	3496	3499	rBV3	1138	738	0.05%	0.007%
79	12.366	3504	3507	3509	rBV3	1011	638	0.05%	0.006%
80	12.527	3555	3557	3559	rBV3	1228	559	0.04%	0.005%
81	12.868	3660	3663	3665	rBV4	1362	794	0.06%	0.008%
82	12.903	3672	3674	3678	rBV3	950	620	0.04%	0.006%
83	13.151	3748	3751	3758	rBV7	1314	1485	0.11%	0.014%
84	13.180	3758	3760	3763	rVB3	1070	608	0.04%	0.006%
85	13.228	3772	3775	3779	rBV5	1436	1312	0.09%	0.013%
86	13.276	3787	3790	3791	rBV2	1913	1142	0.08%	0.011%
87	13.392	3822	3826	3828	rBV4	1242	981	0.07%	0.009%
88	13.450	3837	3844	3849	rBV4	2034	2704	0.19%	0.026%
89	13.492	3855	3857	3862	rBV4	1015	831	0.06%	0.008%
90	13.533	3862	3870	3875	rBV9	3635	5557	0.40%	0.053%
91	13.633	3898	3901	3902	rBV3	992	656	0.05%	0.006%
92	13.755	3936	3939	3940	rBV3	1026	572	0.04%	0.005%
93	13.916	3987	3989	3992	rBV4	861	605	0.04%	0.006%
94	14.119	4050	4052	4053	rBV2	1451	608	0.04%	0.006%
95	14.151	4058	4062	4066	rVB6	1529	1094	0.08%	0.011%
96	14.408	4138	4142	4143	rBV4	1126	642	0.05%	0.006%
97	14.421	4143	4146	4153	rVV8	878	933	0.07%	0.009%
98	14.668	4221	4223	4225	rBV2	1385	561	0.04%	0.005%
99	15.099	4355	4357	4360	rVB2	1311	736	0.05%	0.007%
100	15.144	4367	4371	4374	rBV6	1788	1405	0.10%	0.014%


Sum of corrected areas: 10403310

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016624.D
Acq On : 07 Jun 2020 06:53
Operator : SY/MD
Sample : VV0606WBL03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

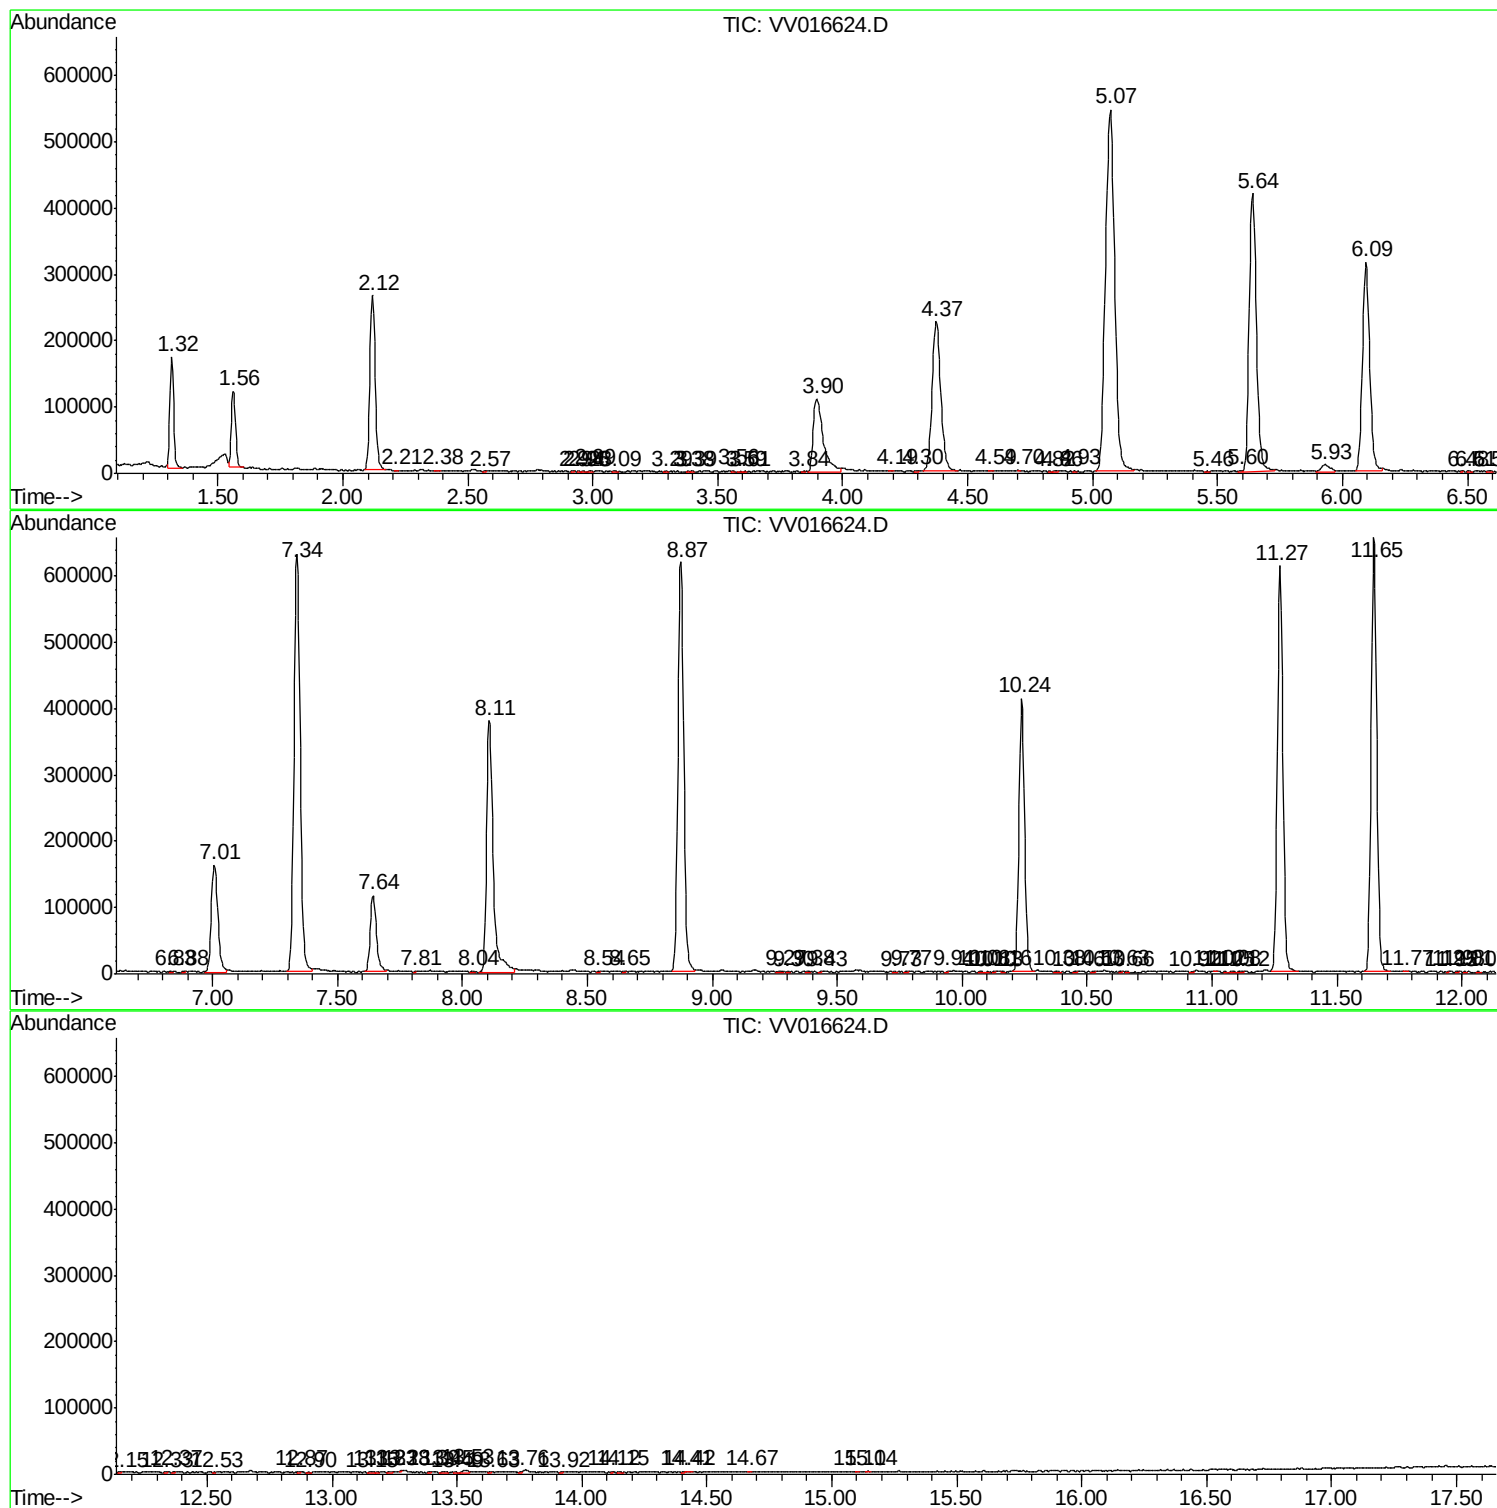

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016624.D
Acq On : 07 Jun 2020 06:53
Operator : SY/MD
Sample : VV0606WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016624.D
Acq On : 07 Jun 2020 06:53
Operator : SY/MD
Sample : VV0606WBL03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK72

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc