

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016625.D
 Acq On : 07 Jun 2020 07:17
 Operator : SY/MD
 Sample : L2872-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	180416	187116	13.05%	1.620%
2	1.566	141	148	158	rVB	127253	148105	10.33%	1.283%
3	2.119	310	320	338	rVB	279982	416816	29.07%	3.609%
4	2.621	471	476	477	rBV4	2588	2161	0.15%	0.019%
5	2.717	503	506	507	rBV2	947	576	0.04%	0.005%
6	2.843	540	545	547	rBV5	1485	1287	0.09%	0.011%
7	2.939	571	575	577	rVB4	1244	763	0.05%	0.007%
8	3.068	612	615	618	rBV5	1438	1046	0.07%	0.009%
9	3.212	651	660	662	rBV9	1497	2055	0.14%	0.018%
10	3.325	692	695	699	rVB5	1167	742	0.05%	0.006%
11	3.357	702	705	709	rVB5	1799	1237	0.09%	0.011%
12	3.431	725	728	730	rBV3	1156	688	0.05%	0.006%
13	3.499	747	749	751	rBV3	1172	696	0.05%	0.006%
14	3.534	756	760	761	rBV4	1743	998	0.07%	0.009%
15	3.605	779	782	786	rVV3	1481	1159	0.08%	0.010%
16	3.640	786	793	798	rVB7	2366	2912	0.20%	0.025%
17	3.666	798	801	803	rBV4	1436	892	0.06%	0.008%
18	3.749	822	827	830	rBV7	1434	1203	0.08%	0.010%
19	3.897	863	873	898	rBV	114466	325087	22.68%	2.815%
20	4.254	982	984	986	rBV2	1321	637	0.04%	0.006%
21	4.373	1008	1021	1043	rVB	227413	546212	38.10%	4.730%
22	4.515	1063	1065	1070	rBV5	1199	1109	0.08%	0.010%
23	4.592	1086	1089	1091	rBV4	1233	1035	0.07%	0.009%
24	4.846	1165	1168	1170	rBV4	960	732	0.05%	0.006%
25	4.904	1184	1186	1190	rVB6	1058	735	0.05%	0.006%
26	4.926	1190	1193	1195	rBV3	1045	698	0.05%	0.006%
27	4.945	1195	1199	1204	rVV7	932	1087	0.08%	0.009%
28	5.071	1218	1238	1263	rVV2	559277	1433658	100.00%	12.415%
29	5.402	1337	1341	1342	rBV4	2325	1595	0.11%	0.014%
30	5.640	1402	1415	1443	rBV	450149	887340	61.89%	7.684%
31	5.846	1476	1479	1480	rBV3	1185	723	0.05%	0.006%
32	5.997	1525	1526	1529	rBV4	1050	641	0.04%	0.006%
33	6.093	1541	1556	1577	rBV	325671	658903	45.96%	5.706%
34	6.328	1628	1629	1633	rBV4	1184	798	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016625.D
 Acq On : 07 Jun 2020 07:17
 Operator : SY/MD
 Sample : L2872-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.441	1661	1664	1667	rBV3	1134	666	0.05%	0.006%
36	6.498	1678	1682	1683	rBV3	1082	560	0.04%	0.005%
37	6.585	1705	1709	1711	rBV4	1271	863	0.06%	0.007%
38	6.637	1718	1725	1726	rBV5	2207	1970	0.14%	0.017%
39	6.762	1761	1764	1765	rBV3	1498	599	0.04%	0.005%
40	6.823	1780	1783	1787	rBV4	992	879	0.06%	0.008%
41	6.904	1804	1808	1810	rBV4	1354	946	0.07%	0.008%
42	6.955	1820	1824	1826	rBV4	1537	1221	0.09%	0.011%
43	7.007	1829	1840	1855	rBV	168765	300928	20.99%	2.606%
44	7.338	1930	1943	1961	rBV	657242	1126313	78.56%	9.753%
45	7.643	2024	2038	2058	rBV	119974	207580	14.48%	1.798%
46	7.913	2118	2122	2127	rBV7	1805	1665	0.12%	0.014%
47	7.997	2136	2148	2164	rBV	523004	870119	60.69%	7.535%
48	8.106	2172	2182	2213	rBV	381485	683577	47.68%	5.919%
49	8.389	2267	2270	2271	rBV3	1022	589	0.04%	0.005%
50	8.537	2314	2316	2322	rBV5	1670	1327	0.09%	0.011%
51	8.627	2342	2344	2347	rBV3	2086	861	0.06%	0.007%
52	8.656	2349	2353	2357	rVV7	1113	1138	0.08%	0.010%
53	8.875	2407	2421	2445	rBV	655206	1067658	74.47%	9.245%
54	9.109	2492	2494	2495	rBV2	1344	565	0.04%	0.005%
55	9.228	2528	2531	2532	rBV3	1060	574	0.04%	0.005%
56	9.354	2563	2570	2575	rBV6	1261	1544	0.11%	0.013%
57	9.392	2581	2582	2586	rVB3	954	590	0.04%	0.005%
58	9.460	2601	2603	2608	rBV5	1185	1068	0.07%	0.009%
59	9.537	2625	2627	2630	rBV4	961	571	0.04%	0.005%
60	9.662	2661	2666	2671	rBV8	1755	2393	0.17%	0.021%
61	9.701	2676	2678	2682	rVV5	1230	664	0.05%	0.006%
62	9.839	2718	2721	2724	rBV4	1203	864	0.06%	0.007%
63	9.862	2725	2728	2735	rVV9	1372	1302	0.09%	0.011%
64	10.132	2809	2812	2814	rBV3	1313	977	0.07%	0.008%
65	10.238	2834	2845	2865	rBV	409868	637596	44.47%	5.521%
66	10.405	2894	2897	2899	rBV2	1067	613	0.04%	0.005%
67	10.418	2899	2901	2904	rVV3	1067	598	0.04%	0.005%
68	10.437	2905	2907	2910	rVB4	1390	733	0.05%	0.006%
69	10.485	2915	2922	2925	rBV9	1566	1468	0.10%	0.013%
70	10.547	2939	2941	2943	rBV3	1421	645	0.04%	0.006%
71	10.662	2974	2977	2981	rBV6	1164	847	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016625.D
 Acq On : 07 Jun 2020 07:17
 Operator : SY/MD
 Sample : L2872-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.688	2982	2985	2988	rVB5	1260	943	0.07%	0.008%
73	10.829	3027	3029	3032	rBV3	1176	743	0.05%	0.006%
74	11.270	3155	3166	3184	rBV	621991	961180	67.04%	8.323%
75	11.473	3226	3229	3230	rBV3	1007	641	0.04%	0.006%
76	11.585	3261	3264	3267	rBV5	1195	759	0.05%	0.007%
77	11.646	3271	3283	3298	rBV	645033	1009707	70.43%	8.744%
78	11.858	3345	3349	3350	rBV2	1084	786	0.05%	0.007%
79	12.058	3407	3411	3414	rBV5	1124	847	0.06%	0.007%
80	12.254	3470	3472	3476	rVB4	1513	846	0.06%	0.007%
81	12.350	3497	3502	3503	rBV4	2089	1415	0.10%	0.012%
82	12.379	3508	3511	3512	rBV3	1462	604	0.04%	0.005%
83	12.447	3529	3532	3533	rBV3	1028	554	0.04%	0.005%
84	12.524	3553	3556	3559	rBV4	1286	861	0.06%	0.007%
85	12.649	3592	3595	3596	rBV2	1240	623	0.04%	0.005%
86	12.765	3629	3631	3635	rVB5	1138	583	0.04%	0.005%
87	13.135	3743	3746	3749	rBV4	1196	661	0.05%	0.006%
88	13.209	3764	3769	3770	rBV5	1309	871	0.06%	0.008%
89	13.373	3817	3820	3826	rBV4	1459	1684	0.12%	0.015%
90	13.418	3832	3834	3836	rBV3	1092	566	0.04%	0.005%
91	13.472	3850	3851	3853	rBV2	1076	547	0.04%	0.005%
92	13.624	3895	3898	3903	rBV5	1292	1286	0.09%	0.011%
93	13.704	3919	3923	3926	rBV4	1263	989	0.07%	0.009%
94	13.807	3953	3955	3958	rBV4	854	644	0.04%	0.006%
95	13.881	3976	3978	3984	rVB7	1635	1154	0.08%	0.010%
96	13.984	4007	4010	4013	rBV4	984	761	0.05%	0.007%
97	14.157	4062	4064	4068	rVB5	1490	955	0.07%	0.008%
98	14.177	4068	4070	4072	rBV3	1131	612	0.04%	0.005%
99	14.231	4084	4087	4089	rBV4	1033	550	0.04%	0.005%
100	14.482	4163	4165	4168	rBV3	1657	1126	0.08%	0.010%


Sum of corrected areas: 11548011

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016625.D
Acq On : 07 Jun 2020 07:17
Operator : SY/MD
Sample : L2872-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

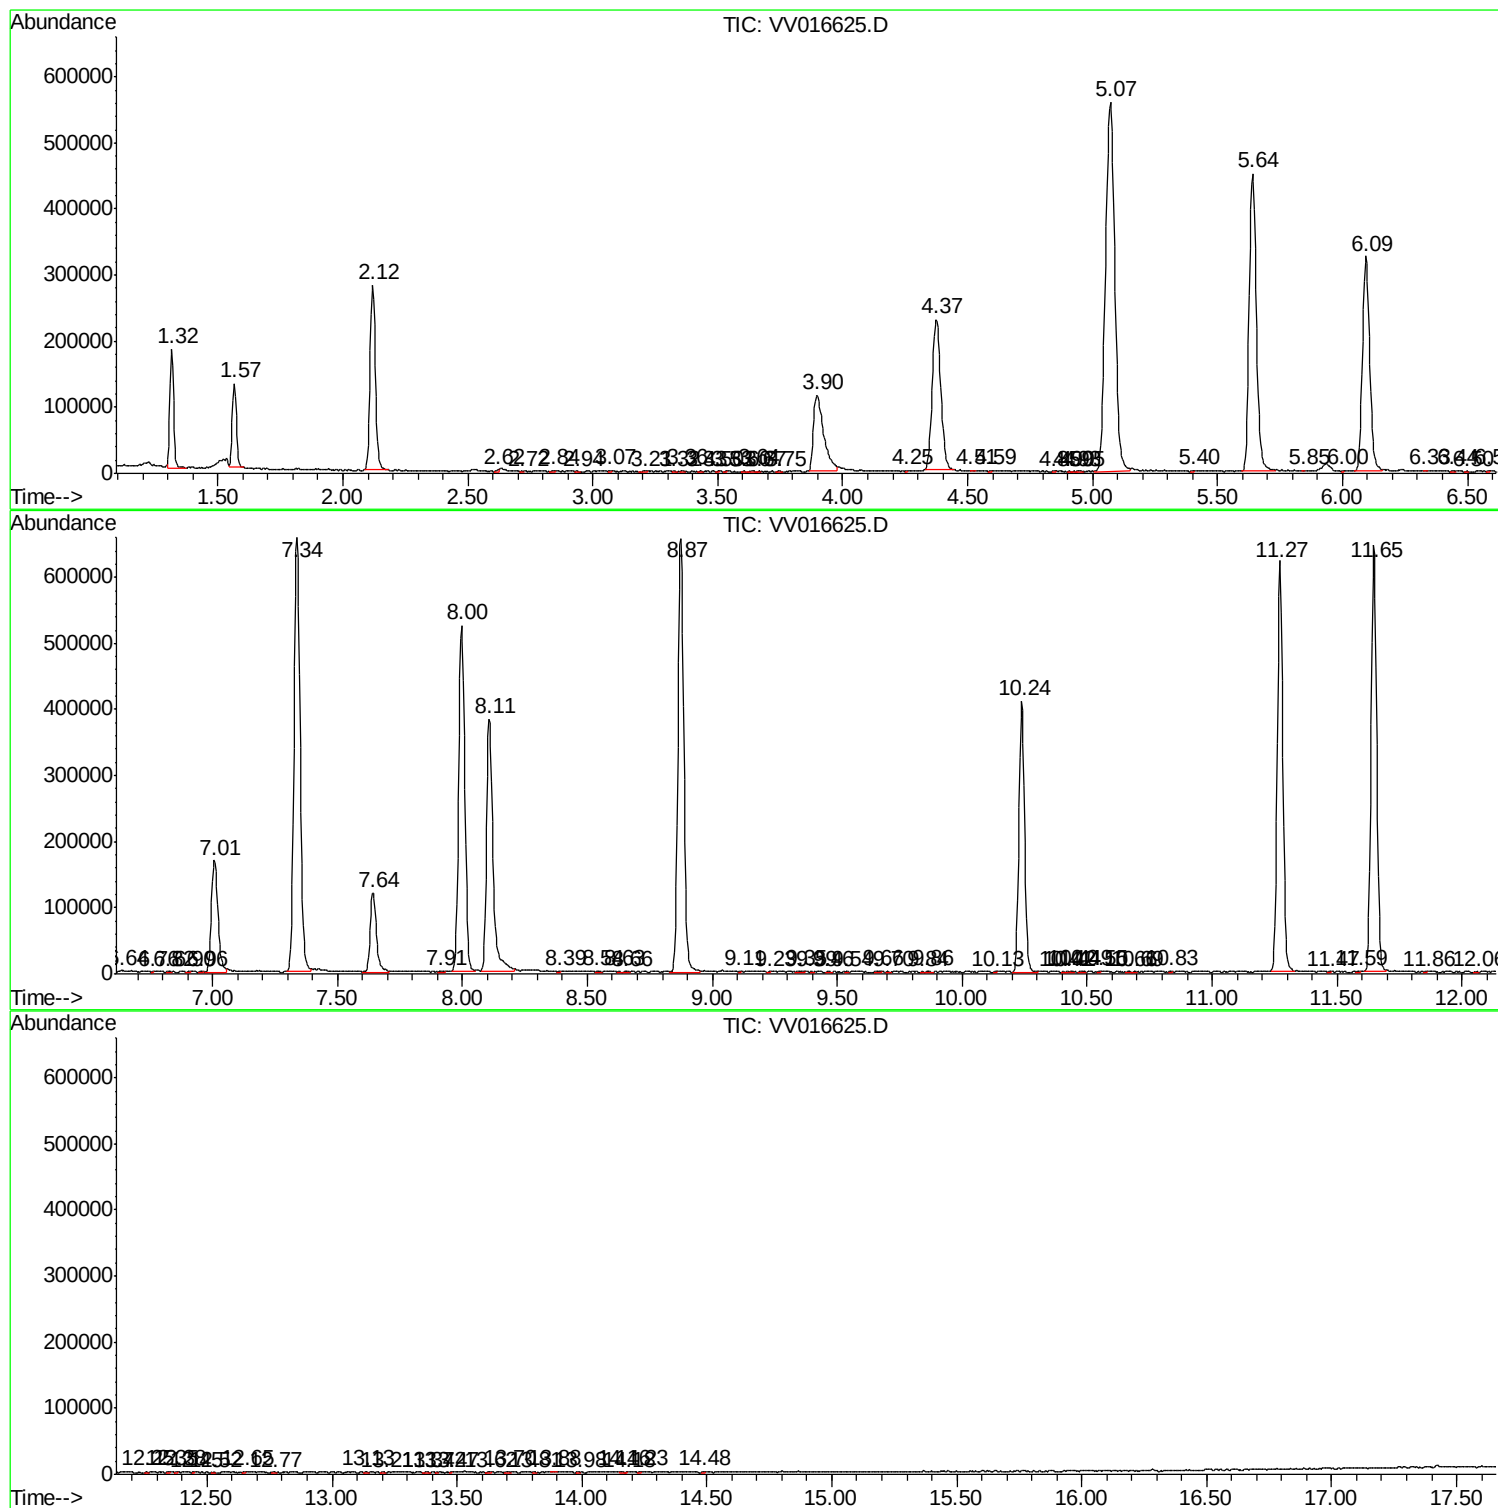

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016625.D
Acq On : 07 Jun 2020 07:17
Operator : SY/MD
Sample : L2872-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016625.D
Acq On : 07 Jun 2020 07:17
Operator : SY/MD
Sample : L2872-03DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFEN5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc