

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016627.D
 Acq On : 07 Jun 2020 08:09
 Operator : SY/MD
 Sample : L2872-14 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	174651	181505	12.74%	1.703%
2	1.563	142	147	160	rVB	115104	139665	9.80%	1.311%
3	2.119	310	320	334	rBV	275871	412392	28.94%	3.870%
4	2.441	416	420	423	rBV3	1461	1349	0.09%	0.013%
5	2.618	470	475	477	rBV5	1866	1412	0.10%	0.013%
6	2.884	554	558	562	rVB6	1688	1319	0.09%	0.012%
7	2.904	562	564	568	rBV4	1674	1039	0.07%	0.010%
8	2.971	581	585	590	rBV6	1238	1168	0.08%	0.011%
9	3.048	605	609	611	rBV5	1311	984	0.07%	0.009%
10	3.090	619	622	626	rBV3	799	814	0.06%	0.008%
11	3.187	650	652	654	rBV3	1237	810	0.06%	0.008%
12	3.254	670	673	677	rVV5	1465	1085	0.08%	0.010%
13	3.360	704	706	710	rBV4	1207	672	0.05%	0.006%
14	3.437	727	730	733	rVB5	1027	773	0.05%	0.007%
15	3.502	746	750	752	rBV4	1124	850	0.06%	0.008%
16	3.643	788	794	798	rBV6	1669	1534	0.11%	0.014%
17	3.900	861	874	904	rBV2	107625	307664	21.59%	2.887%
18	4.158	950	954	956	rBV3	919	794	0.06%	0.007%
19	4.296	994	997	1001	rBV6	1638	1442	0.10%	0.014%
20	4.373	1006	1021	1045	rVV	230190	559733	39.28%	5.253%
21	4.630	1098	1101	1104	rBV3	1103	826	0.06%	0.008%
22	4.775	1142	1146	1149	rBV4	1268	887	0.06%	0.008%
23	4.801	1149	1154	1156	rBV4	975	940	0.07%	0.009%
24	4.836	1163	1165	1169	rBV4	1149	756	0.05%	0.007%
25	4.884	1175	1180	1181	rBV4	1665	1039	0.07%	0.010%
26	4.917	1186	1190	1193	rBV4	1166	896	0.06%	0.008%
27	4.949	1198	1200	1203	rVV3	2167	1198	0.08%	0.011%
28	4.984	1209	1211	1216	rBV7	973	821	0.06%	0.008%
29	5.071	1221	1238	1264	rBV2	557071	1425048	100.00%	13.373%
30	5.408	1341	1343	1347	rBV4	1488	771	0.05%	0.007%
31	5.553	1383	1388	1391	rBV6	1583	1299	0.09%	0.012%
32	5.572	1391	1394	1397	rBV4	1346	910	0.06%	0.009%
33	5.640	1402	1415	1435	rBV	444791	874568	61.37%	8.207%
34	5.929	1494	1505	1517	rBV10	10513	23005	1.61%	0.216%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016627.D
 Acq On : 07 Jun 2020 08:09
 Operator : SY/MD
 Sample : L2872-14 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1542	1556	1579	rBV	318915	644928	45.26%	6.052%
36	6.425	1656	1659	1661	rBV4	1493	949	0.07%	0.009%
37	6.515	1685	1687	1692	rVB5	1410	966	0.07%	0.009%
38	6.537	1692	1694	1698	rBV4	924	747	0.05%	0.007%
39	6.633	1720	1724	1726	rBV5	1328	1289	0.09%	0.012%
40	7.006	1825	1840	1857	rBV	165076	301938	21.19%	2.834%
41	7.338	1931	1943	1961	rBV	653989	1123490	78.84%	10.543%
42	7.643	2028	2038	2054	rBV	116832	197029	13.83%	1.849%
43	7.746	2068	2070	2074	rBV5	1077	678	0.05%	0.006%
44	7.913	2119	2122	2123	rBV3	1085	673	0.05%	0.006%
45	7.952	2131	2134	2138	rBV6	1646	1239	0.09%	0.012%
46	7.974	2138	2141	2142	rBV3	1354	780	0.05%	0.007%
47	8.003	2142	2150	2159	rVV3	5665	10385	0.73%	0.097%
48	8.109	2172	2183	2215	rBV	371911	684240	48.02%	6.421%
49	8.585	2329	2331	2335	rVB5	1201	703	0.05%	0.007%
50	8.682	2358	2361	2363	rBV3	1566	726	0.05%	0.007%
51	8.701	2363	2367	2369	rBV3	1002	727	0.05%	0.007%
52	8.736	2376	2378	2382	rVB3	1308	825	0.06%	0.008%
53	8.807	2397	2400	2402	rBV4	1018	802	0.06%	0.008%
54	8.833	2404	2408	2409	rBV2	1342	745	0.05%	0.007%
55	8.875	2409	2421	2440	rBV	646626	1048354	73.57%	9.838%
56	9.045	2471	2474	2476	rBV4	1934	1302	0.09%	0.012%
57	9.093	2485	2489	2496	rVB8	1934	1784	0.13%	0.017%
58	9.315	2555	2558	2561	rBV5	1290	1093	0.08%	0.010%
59	9.453	2595	2601	2603	rVB5	1783	1600	0.11%	0.015%
60	9.469	2603	2606	2609	rBV4	938	783	0.05%	0.007%
61	9.502	2614	2616	2620	rVB5	1429	824	0.06%	0.008%
62	9.563	2630	2635	2637	rBV4	1382	950	0.07%	0.009%
63	9.846	2719	2723	2725	rVB5	1421	969	0.07%	0.009%
64	10.035	2780	2782	2785	rBV5	1308	846	0.06%	0.008%
65	10.238	2834	2845	2863	rVB	404465	630711	44.26%	5.919%
66	10.354	2879	2881	2885	rVB4	1353	807	0.06%	0.008%
67	10.392	2889	2893	2894	rBV2	1615	1034	0.07%	0.010%
68	10.444	2907	2909	2913	rBV4	1169	805	0.06%	0.008%
69	10.723	2993	2996	3000	rBV4	1371	1140	0.08%	0.011%
70	10.862	3035	3039	3041	rBV2	1373	1037	0.07%	0.010%
71	10.923	3057	3058	3064	rBV4	981	872	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016627.D
 Acq On : 07 Jun 2020 08:09
 Operator : SY/MD
 Sample : L2872-14 1000X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.952	3064	3067	3069	rBV3	1284	733	0.05%	0.007%
73	11.180	3132	3138	3140	rBV6	1275	1370	0.10%	0.013%
74	11.270	3153	3166	3181	rBV	643027	978850	68.69%	9.186%
75	11.556	3253	3255	3259	rBV5	1129	918	0.06%	0.009%
76	11.646	3272	3283	3300	rBV	658383	1027745	72.12%	9.645%
77	11.952	3375	3378	3381	rBV5	1128	960	0.07%	0.009%
78	11.964	3381	3382	3387	rVB5	1501	841	0.06%	0.008%
79	12.180	3447	3449	3454	rVB4	886	716	0.05%	0.007%
80	12.254	3469	3472	3474	rBV3	899	702	0.05%	0.007%
81	12.723	3615	3618	3621	rBV3	929	675	0.05%	0.006%
82	12.784	3634	3637	3640	rBV3	1386	1120	0.08%	0.011%
83	12.881	3664	3667	3671	rBV5	1185	818	0.06%	0.008%
84	12.968	3691	3694	3698	rVB6	1417	828	0.06%	0.008%
85	13.013	3704	3708	3711	rVB6	1366	1127	0.08%	0.011%
86	13.132	3740	3745	3747	rBV6	1395	1377	0.10%	0.013%
87	13.170	3756	3757	3763	rVB5	1496	909	0.06%	0.009%
88	13.296	3787	3796	3800	rBV10	1543	1977	0.14%	0.019%
89	13.389	3820	3825	3828	rBV6	2227	2039	0.14%	0.019%
90	13.669	3908	3912	3915	rBV6	1909	1688	0.12%	0.016%
91	13.865	3971	3973	3977	rVB4	1643	895	0.06%	0.008%
92	13.890	3977	3981	3984	rBV6	2079	1765	0.12%	0.017%
93	13.958	3999	4002	4003	rBV2	1210	834	0.06%	0.008%
94	13.987	4009	4011	4015	rVB4	1454	937	0.07%	0.009%
95	14.096	4042	4045	4049	rVB6	1301	843	0.06%	0.008%
96	14.180	4066	4071	4074	rBV6	1884	1334	0.09%	0.013%
97	14.244	4088	4091	4094	rVB5	1662	927	0.07%	0.009%
98	14.588	4193	4198	4200	rBV4	1099	844	0.06%	0.008%
99	14.614	4200	4206	4210	rBV7	1923	2631	0.18%	0.025%
100	15.408	4450	4453	4455	rBV3	1774	846	0.06%	0.008%


Sum of corrected areas: 10655987

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016627.D
Acq On : 07 Jun 2020 08:09
Operator : SY/MD
Sample : L2872-14 1000X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

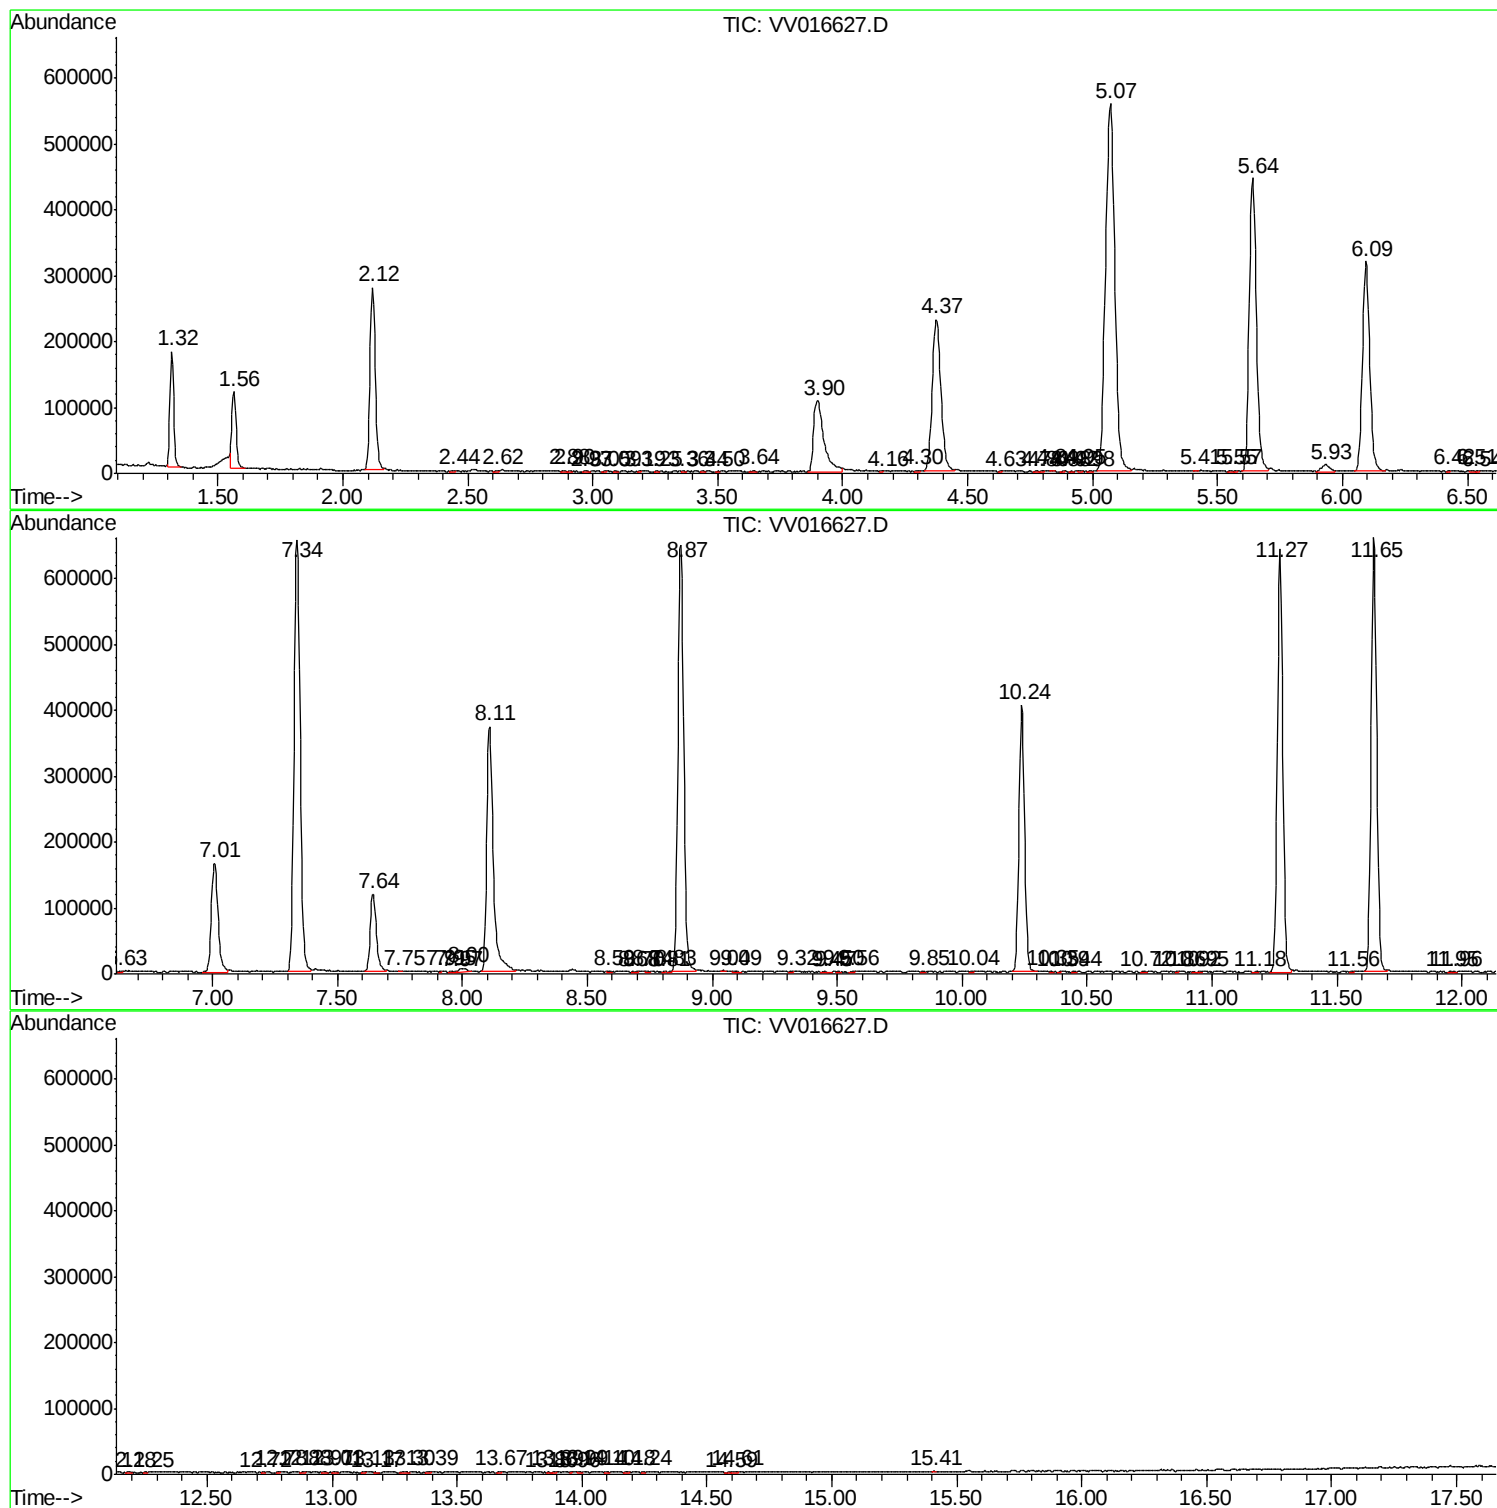

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016627.D
Acq On : 07 Jun 2020 08:09
Operator : SY/MD
Sample : L2872-14 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016627.D
Acq On : 07 Jun 2020 08:09
Operator : SY/MD
Sample : L2872-14 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEP6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc