

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016629.D
 Acq On : 07 Jun 2020 08:56
 Operator : SY/MD
 Sample : L2862-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D73DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	173419	177399	12.66%	1.708%
2	2.116	310	319	333	rBV	270928	398764	28.46%	3.839%
3	2.409	408	410	412	rBV3	1459	832	0.06%	0.008%
4	2.476	429	431	432	rBV2	848	404	0.03%	0.004%
5	2.865	547	552	555	rVB5	974	792	0.06%	0.008%
6	2.884	555	558	561	rVB3	1712	1011	0.07%	0.010%
7	2.897	561	562	563	rVB	377	73	0.01%	0.001%
8	2.907	563	565	566	rBV2	1179	452	0.03%	0.004%
9	2.917	566	568	569	rBV2	737	340	0.02%	0.003%
10	2.942	574	576	578	rBV3	722	404	0.03%	0.004%
11	2.955	578	580	584	rBV4	924	555	0.04%	0.005%
12	2.978	585	587	593	rVB5	1189	766	0.05%	0.007%
13	3.003	593	595	599	rVB4	900	644	0.05%	0.006%
14	3.023	599	601	602	rBV	374	186	0.01%	0.002%
15	3.029	602	603	604	rBV	539	130	0.01%	0.001%
16	3.048	604	609	610	rBV4	1794	1012	0.07%	0.010%
17	3.109	626	628	630	rBV2	1055	392	0.03%	0.004%
18	3.126	630	633	634	rBV3	1137	487	0.03%	0.005%
19	3.135	634	636	639	rVB3	1513	728	0.05%	0.007%
20	3.155	639	642	643	rBV3	1070	525	0.04%	0.005%
21	3.171	643	647	648	rBV4	852	562	0.04%	0.005%
22	3.203	655	657	659	rVB3	1110	536	0.04%	0.005%
23	3.219	659	662	663	rBV3	963	406	0.03%	0.004%
24	3.235	666	667	668	rVB	478	92	0.01%	0.001%
25	3.248	668	671	672	rBV3	819	467	0.03%	0.004%
26	3.267	676	677	678	rBB	327	63	0.00%	0.001%
27	3.283	678	682	683	rBV3	857	534	0.04%	0.005%
28	3.302	683	688	690	rBV4	1383	1031	0.07%	0.010%
29	3.363	703	707	709	rBV5	1376	1037	0.07%	0.010%
30	3.421	721	725	728	rBV3	1091	830	0.06%	0.008%
31	3.482	741	744	747	rBV4	1346	1032	0.07%	0.010%
32	3.611	782	784	788	rVB4	1482	1077	0.08%	0.010%
33	3.637	790	792	793	rBV2	419	171	0.01%	0.002%
34	3.653	795	797	799	rVV3	1182	450	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016629.D
 Acq On : 07 Jun 2020 08:56
 Operator : SY/MD
 Sample : L2862-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D73DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	3.691	807	809	810	rBV2	913	356	0.03%	0.003%
36	3.740	821	824	825	rBV3	1182	556	0.04%	0.005%
37	3.897	863	873	902	rBV	104596	293163	20.92%	2.822%
38	4.167	954	957	961	rBV3	1612	1318	0.09%	0.013%
39	4.277	989	991	992	rBV2	1257	513	0.04%	0.005%
40	4.373	1005	1021	1046	rBV	223282	549363	39.20%	5.288%
41	4.634	1100	1102	1104	rBV3	531	281	0.02%	0.003%
42	4.646	1104	1106	1107	rBV2	1019	376	0.03%	0.004%
43	4.833	1162	1164	1167	rVB3	848	456	0.03%	0.004%
44	4.884	1179	1180	1182	rBV2	748	262	0.02%	0.003%
45	4.913	1184	1189	1192	rBV6	1309	1254	0.09%	0.012%
46	5.071	1219	1238	1247	rBV2	549100	1401301	100.00%	13.489%
47	5.640	1402	1415	1434	rBV	431683	854778	61.00%	8.228%
48	5.929	1497	1505	1514	rBV9	7364	14564	1.04%	0.140%
49	6.093	1543	1556	1582	rBV	310146	628658	44.86%	6.052%
50	6.351	1633	1636	1638	rBV4	1081	602	0.04%	0.006%
51	6.527	1688	1691	1693	rBV4	715	490	0.03%	0.005%
52	6.621	1718	1720	1721	rBV2	1179	461	0.03%	0.004%
53	6.733	1751	1755	1757	rBV4	1360	1109	0.08%	0.011%
54	6.778	1767	1769	1771	rBV3	1409	911	0.07%	0.009%
55	6.961	1824	1826	1827	rBV2	628	210	0.01%	0.002%
56	7.006	1827	1840	1855	rBV	167098	297381	21.22%	2.863%
57	7.125	1875	1877	1878	rBV2	1010	462	0.03%	0.004%
58	7.267	1919	1921	1924	rBV4	1295	972	0.07%	0.009%
59	7.338	1931	1943	1960	rBV	638517	1091207	77.87%	10.504%
60	7.643	2021	2038	2055	rBV	114628	206579	14.74%	1.989%
61	7.765	2072	2076	2082	rBV6	1780	1868	0.13%	0.018%
62	7.990	2143	2146	2149	rBV4	2317	2068	0.15%	0.020%
63	8.109	2172	2183	2212	rBV	358514	673263	48.05%	6.481%
64	8.592	2331	2333	2335	rBV4	1006	634	0.05%	0.006%
65	8.617	2338	2341	2343	rBV3	1577	1191	0.08%	0.011%
66	8.875	2410	2421	2444	rBV	630019	1030531	73.54%	9.920%
67	9.042	2464	2473	2480	rBV3	9979	17298	1.23%	0.167%
68	9.283	2537	2548	2557	rBV9	14921	29419	2.10%	0.283%
69	9.405	2581	2586	2596	rVB6	11149	16176	1.15%	0.156%
70	9.682	2670	2672	2675	rBV3	1269	698	0.05%	0.007%
71	9.739	2680	2690	2704	rVV3	7715	16192	1.16%	0.156%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016629.D
 Acq On : 07 Jun 2020 08:56
 Operator : SY/MD
 Sample : L2862-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D73DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.103	2795	2803	2804	rBV8	4146	4948	0.35%	0.048%
73	10.238	2835	2845	2860	rVB	402753	633969	45.24%	6.103%
74	10.913	3053	3055	3057	rBV3	1322	699	0.05%	0.007%
75	11.270	3156	3166	3182	rBV	628468	965035	68.87%	9.290%
76	11.646	3272	3283	3297	rBV	668195	1037181	74.02%	9.984%
77	11.971	3382	3384	3386	rBV3	1082	478	0.03%	0.005%
78	12.964	3690	3693	3695	rBV4	2044	1558	0.11%	0.015%
79	13.019	3708	3710	3712	rBV3	834	414	0.03%	0.004%
80	13.138	3742	3747	3749	rBV3	1254	1100	0.08%	0.011%
81	13.154	3750	3752	3753	rBV2	1153	391	0.03%	0.004%
82	13.315	3799	3802	3805	rBV3	2056	1410	0.10%	0.014%
83	13.421	3833	3835	3836	rBV2	716	266	0.02%	0.003%
84	13.498	3856	3859	3861	rBV5	1619	1160	0.08%	0.011%
85	13.865	3968	3973	3975	rBV4	1465	1336	0.10%	0.013%
86	14.025	4020	4023	4027	rBV4	1889	1598	0.11%	0.015%
87	14.045	4027	4029	4030	rBV2	1599	744	0.05%	0.007%
88	14.521	4169	4177	4180	rBV8	1532	2149	0.15%	0.021%
89	15.160	4374	4376	4378	rBV3	1180	591	0.04%	0.006%
90	15.437	4460	4462	4465	rBV3	1374	582	0.04%	0.006%
91	15.717	4546	4549	4551	rBV4	2122	1541	0.11%	0.015%


Sum of corrected areas: 10388255

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016629.D
Acq On : 07 Jun 2020 08:56
Operator : SY/MD
Sample : L2862-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D73DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

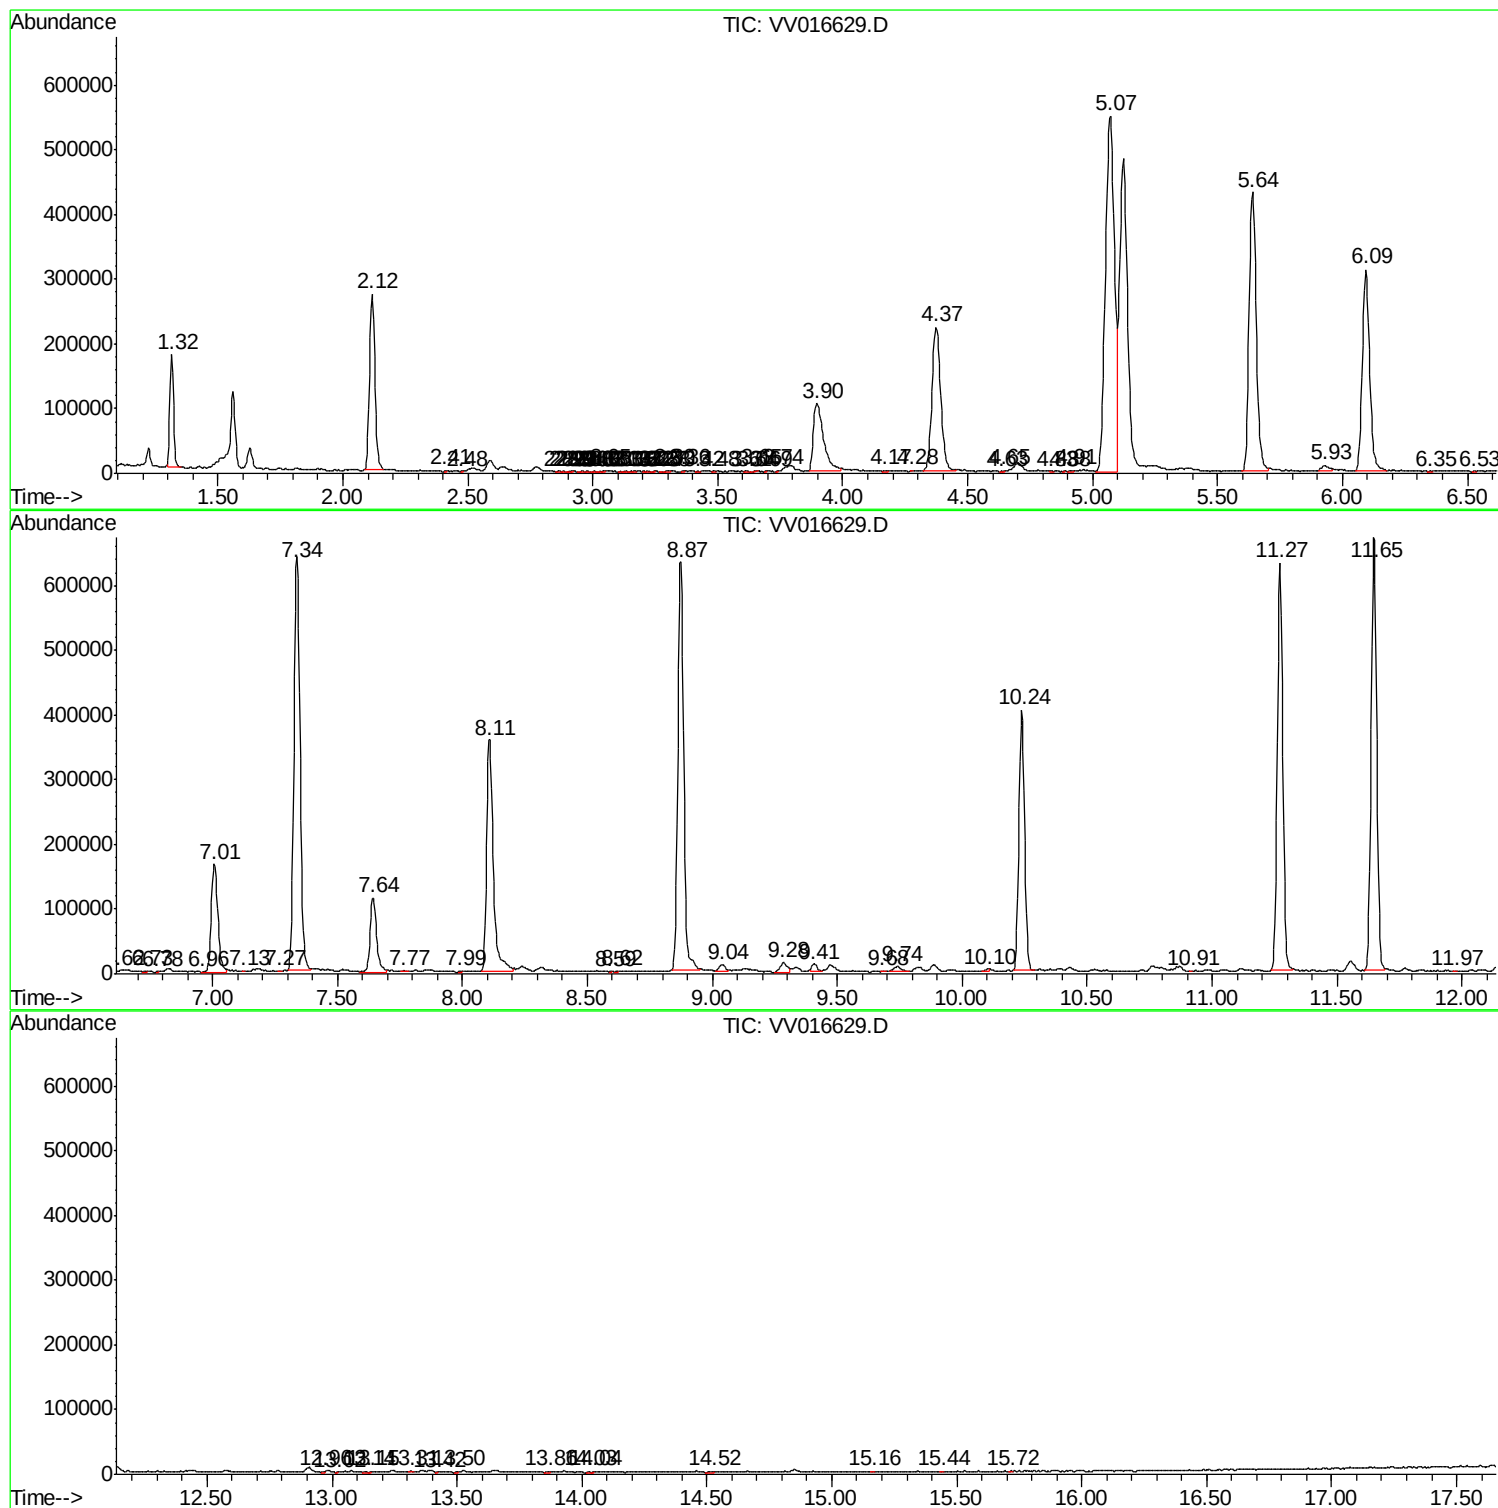

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016629.D
Acq On : 07 Jun 2020 08:56
Operator : SY/MD
Sample : L2862-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D73DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016629.D
Acq On : 07 Jun 2020 08:56
Operator : SY/MD
Sample : L2862-03DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9D73DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc