

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016631.D
 Acq On : 07 Jun 2020 09:44
 Operator : SY/MD
 Sample : L2862-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D88DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	190097	191561	13.40%	1.808%
2	1.563	142	147	158	rVB	111702	132168	9.25%	1.248%
3	2.116	310	319	338	rBV	270414	404676	28.31%	3.820%
4	2.901	559	563	564	rBV4	1291	587	0.04%	0.006%
5	2.955	578	580	582	rVB3	1155	547	0.04%	0.005%
6	2.971	582	585	590	rBV6	1238	1327	0.09%	0.013%
7	3.039	604	606	609	rBV4	1015	687	0.05%	0.006%
8	3.106	622	627	629	rBV4	1374	1236	0.09%	0.012%
9	3.151	638	641	644	rBV5	1034	637	0.04%	0.006%
10	3.212	655	660	661	rBV3	1276	932	0.07%	0.009%
11	3.270	675	678	679	rBV2	1098	737	0.05%	0.007%
12	3.370	705	709	710	rBV4	900	709	0.05%	0.007%
13	3.444	727	732	736	rBV7	1174	1416	0.10%	0.013%
14	3.592	775	778	782	rBV4	932	632	0.04%	0.006%
15	3.653	793	797	798	rBV4	1012	573	0.04%	0.005%
16	3.672	801	803	805	rVV4	1399	788	0.06%	0.007%
17	3.708	812	814	817	rVB4	842	514	0.04%	0.005%
18	3.897	859	873	901	rBV2	108316	310945	21.76%	2.935%
19	4.193	963	965	967	rBV3	1291	802	0.06%	0.008%
20	4.373	1006	1021	1046	rBV	227725	553730	38.74%	5.227%
21	4.798	1150	1153	1154	rBV3	1296	571	0.04%	0.005%
22	4.875	1175	1177	1181	rVB4	1923	1027	0.07%	0.010%
23	4.929	1191	1194	1196	rBV2	1203	763	0.05%	0.007%
24	4.965	1202	1205	1208	rBV5	936	686	0.05%	0.006%
25	5.071	1220	1238	1248	rBV2	560769	1429251	100.00%	13.492%
26	5.499	1367	1371	1373	rBV4	1924	1509	0.11%	0.014%
27	5.550	1385	1387	1391	rBV4	1649	894	0.06%	0.008%
28	5.579	1391	1396	1398	rBV4	975	961	0.07%	0.009%
29	5.640	1402	1415	1437	rBV	438429	868709	60.78%	8.200%
30	5.894	1492	1494	1495	rBV2	1458	665	0.05%	0.006%
31	6.093	1541	1556	1579	rBV	319035	651173	45.56%	6.147%
32	6.312	1621	1624	1625	rBV2	889	516	0.04%	0.005%
33	6.341	1630	1633	1639	rBV8	1068	1305	0.09%	0.012%
34	6.473	1672	1674	1676	rVB2	1482	515	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016631.D
 Acq On : 07 Jun 2020 09:44
 Operator : SY/MD
 Sample : L2862-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D88DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.502	1679	1683	1687	rBV6	1213	1151	0.08%	0.011%
36	6.566	1700	1703	1708	rVB6	1794	1421	0.10%	0.013%
37	6.595	1708	1712	1715	rBV5	975	1038	0.07%	0.010%
38	6.646	1722	1728	1729	rBV7	1915	2046	0.14%	0.019%
39	6.942	1818	1820	1822	rBV2	928	654	0.05%	0.006%
40	7.007	1826	1840	1860	rBV	164614	297701	20.83%	2.810%
41	7.164	1887	1889	1891	rBV3	1618	786	0.05%	0.007%
42	7.338	1931	1943	1960	rBV	656774	1107427	77.48%	10.454%
43	7.550	2005	2009	2012	rBV4	2043	1732	0.12%	0.016%
44	7.582	2015	2019	2020	rBV3	841	560	0.04%	0.005%
45	7.643	2028	2038	2051	rBV	115435	196437	13.74%	1.854%
46	7.733	2064	2066	2070	rVB4	1434	931	0.07%	0.009%
47	7.830	2092	2096	2100	rVB6	1018	868	0.06%	0.008%
48	7.920	2120	2124	2130	rBV6	1648	1498	0.10%	0.014%
49	7.945	2130	2132	2134	rBV3	1030	707	0.05%	0.007%
50	8.106	2172	2182	2215	rBV	364670	678937	47.50%	6.409%
51	8.505	2302	2306	2310	rVB5	1670	1682	0.12%	0.016%
52	8.682	2359	2361	2366	rBV3	830	531	0.04%	0.005%
53	8.707	2366	2369	2372	rVB5	1340	819	0.06%	0.008%
54	8.875	2409	2421	2447	rBV	642971	1051059	73.54%	9.922%
55	9.286	2542	2549	2557	rBV	3544	5845	0.41%	0.055%
56	9.399	2579	2584	2585	rBV4	2621	2070	0.14%	0.020%
57	9.469	2596	2606	2610	rBV9	4004	5920	0.41%	0.056%
58	9.640	2656	2659	2664	rVB8	1874	1333	0.09%	0.013%
59	9.733	2685	2688	2690	rBV4	2381	1499	0.10%	0.014%
60	10.071	2790	2793	2797	rBV5	1223	909	0.06%	0.009%
61	10.093	2798	2800	2802	rBV3	1313	723	0.05%	0.007%
62	10.141	2813	2815	2818	rBV5	1040	747	0.05%	0.007%
63	10.238	2832	2845	2860	rBV	397942	636669	44.55%	6.010%
64	10.350	2878	2880	2883	rBV4	1616	860	0.06%	0.008%
65	10.376	2884	2888	2892	rBV7	2728	2943	0.21%	0.028%
66	10.630	2965	2967	2971	rVB4	1874	1149	0.08%	0.011%
67	10.653	2971	2974	2977	rBV5	1450	1072	0.08%	0.010%
68	10.698	2984	2988	2989	rBV3	784	542	0.04%	0.005%
69	10.756	3003	3006	3009	rBV4	1516	1321	0.09%	0.012%
70	11.096	3110	3112	3114	rBV2	1624	996	0.07%	0.009%
71	11.270	3155	3166	3188	rVB	630510	968235	67.74%	9.140%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016631.D
 Acq On : 07 Jun 2020 09:44
 Operator : SY/MD
 Sample : L2862-05DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D88DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3297	rBV	654476	1023079	71.58%	9.658%
73	11.993	3388	3391	3393	rBV2	1727	1015	0.07%	0.010%
74	12.010	3393	3396	3399	rBV4	1642	1260	0.09%	0.012%
75	12.074	3413	3416	3420	rBV5	1726	1170	0.08%	0.011%
76	12.264	3473	3475	3477	rBV3	1110	577	0.04%	0.005%
77	12.592	3573	3577	3580	rBV3	1015	835	0.06%	0.008%
78	12.714	3611	3615	3619	rBV4	1399	1448	0.10%	0.014%
79	12.756	3625	3628	3631	rBV5	1458	1124	0.08%	0.011%
80	13.006	3703	3706	3709	rBV4	1613	1026	0.07%	0.010%
81	13.135	3744	3746	3747	rBV2	1089	561	0.04%	0.005%
82	13.151	3749	3751	3753	rVB3	1497	647	0.05%	0.006%
83	13.225	3772	3774	3778	rBV3	959	553	0.04%	0.005%
84	13.447	3837	3843	3844	rBV4	1265	1026	0.07%	0.010%
85	13.755	3935	3939	3940	rBV2	934	585	0.04%	0.006%
86	13.797	3948	3952	3954	rBV5	973	825	0.06%	0.008%
87	13.891	3979	3981	3985	rVB4	1469	844	0.06%	0.008%
88	14.006	4012	4017	4018	rBV4	1017	783	0.05%	0.007%
89	14.061	4032	4034	4036	rBV3	1142	750	0.05%	0.007%
90	14.135	4054	4057	4058	rBV2	1138	563	0.04%	0.005%
91	14.167	4065	4067	4068	rBV3	1244	650	0.05%	0.006%
92	14.209	4078	4080	4085	rBV4	1312	1010	0.07%	0.010%
93	14.231	4085	4087	4089	rVB3	1334	599	0.04%	0.006%
94	14.273	4097	4100	4103	rBV4	1491	1130	0.08%	0.011%
95	14.325	4114	4116	4121	rVB5	1850	1548	0.11%	0.015%
96	14.608	4200	4204	4206	rBV3	1216	915	0.06%	0.009%
97	14.800	4262	4264	4266	rBV3	1636	896	0.06%	0.008%
98	15.029	4333	4335	4339	rBV5	1109	1036	0.07%	0.010%
99	15.125	4362	4365	4368	rBV4	2303	1545	0.11%	0.015%
100	15.312	4420	4423	4425	rBV2	1158	823	0.06%	0.008%


Sum of corrected areas: 10593390

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016631.D
Acq On : 07 Jun 2020 09:44
Operator : SY/MD
Sample : L2862-05DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D88DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

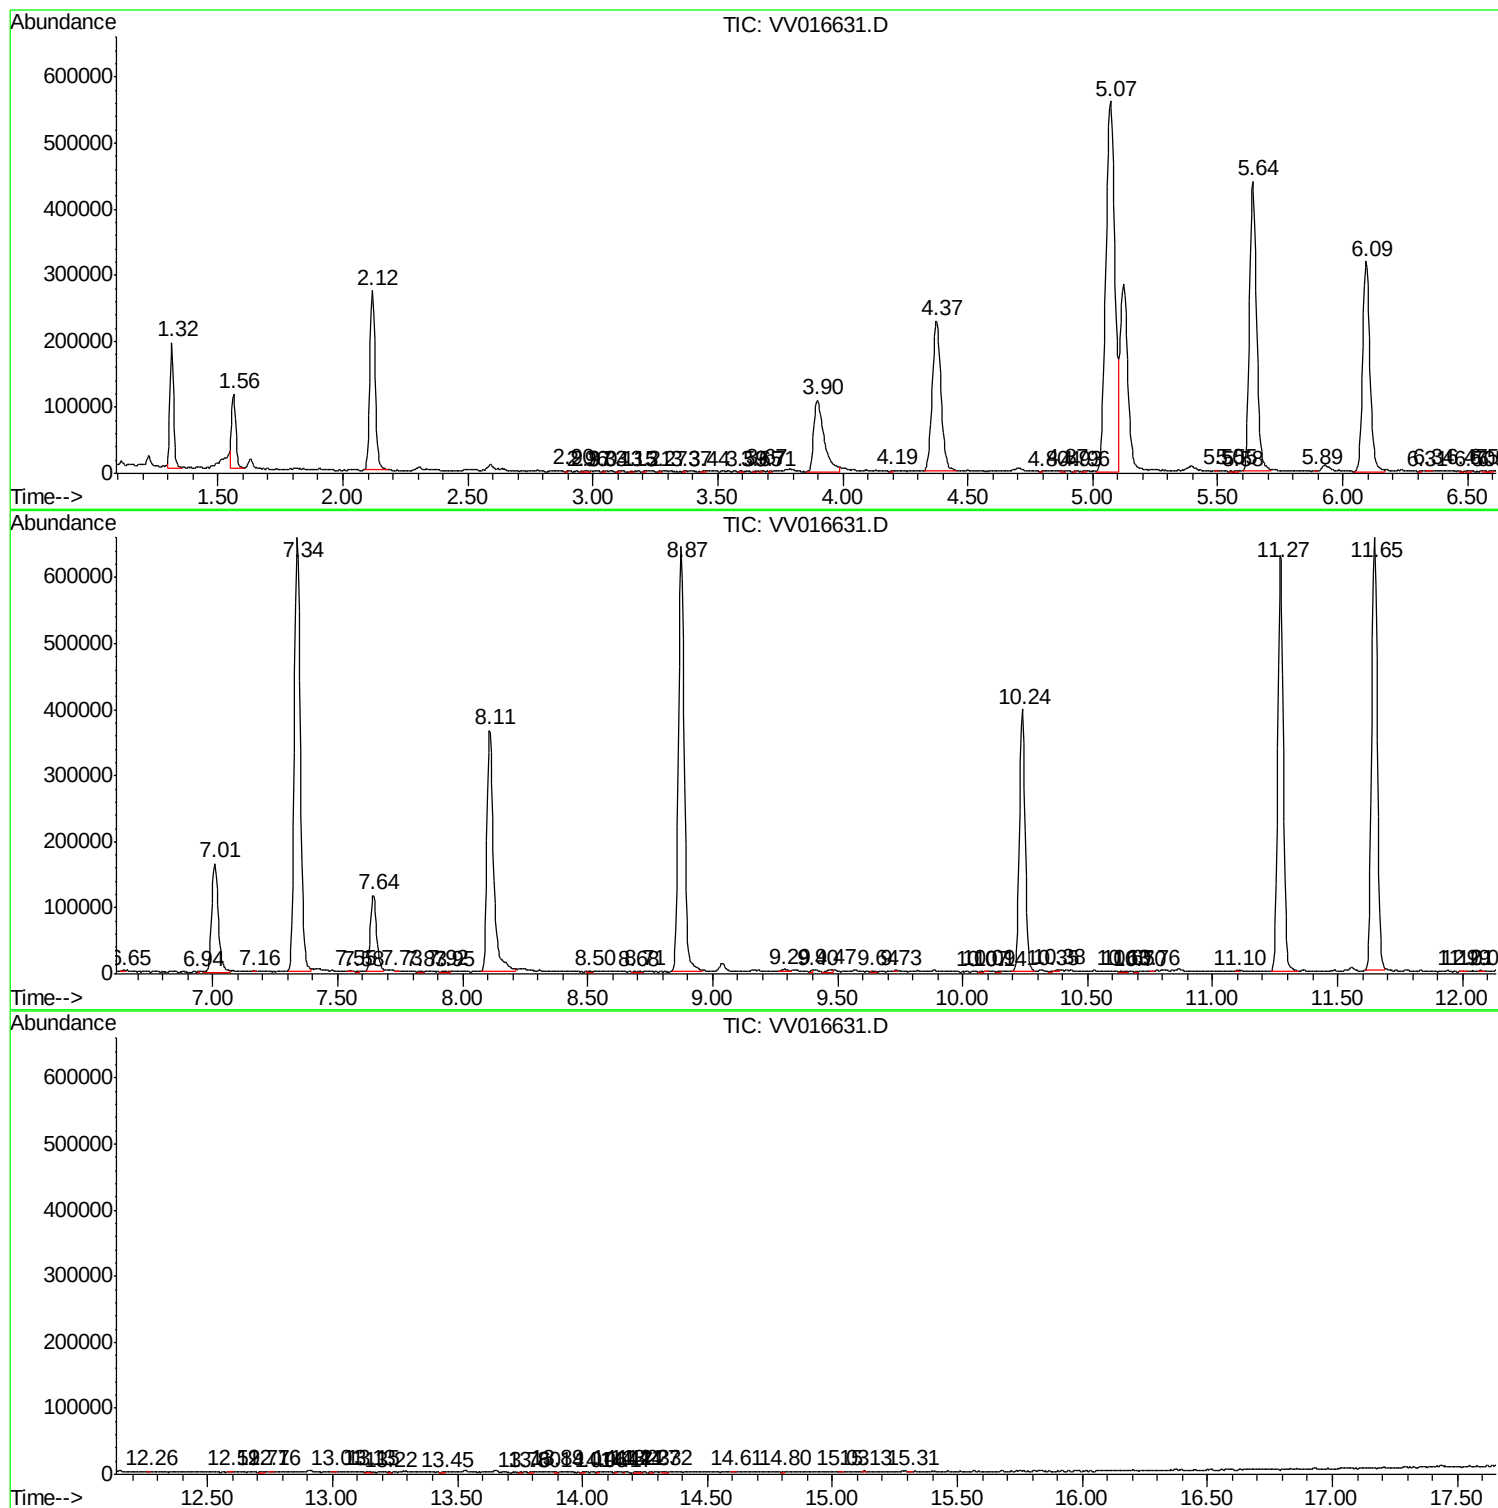

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016631.D
Acq On : 07 Jun 2020 09:44
Operator : SY/MD
Sample : L2862-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D88DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016631.D
Acq On : 07 Jun 2020 09:44
Operator : SY/MD
Sample : L2862-05DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9D88DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc