

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016632.D
 Acq On : 07 Jun 2020 10:08
 Operator : SY/MD
 Sample : L2862-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D89DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	187069	185250	13.51%	1.773%
2	1.563	141	147	157	rVB	118328	139356	10.16%	1.334%
3	2.119	310	320	336	rBV	270024	398124	29.04%	3.811%
4	2.737	510	512	516	rBV4	1123	910	0.07%	0.009%
5	2.765	518	521	523	rBV4	1767	1336	0.10%	0.013%
6	2.833	537	542	544	rBV5	992	1041	0.08%	0.010%
7	3.090	619	622	624	rBV4	1049	824	0.06%	0.008%
8	3.290	680	684	688	rBV6	948	901	0.07%	0.009%
9	3.518	753	755	759	rBV4	1061	633	0.05%	0.006%
10	3.595	775	779	782	rVB6	1471	1002	0.07%	0.010%
11	3.608	782	783	786	rBV3	719	476	0.03%	0.005%
12	3.659	796	799	801	rVV4	691	508	0.04%	0.005%
13	3.762	829	831	832	rBV	1276	565	0.04%	0.005%
14	3.897	862	873	900	rBV	112399	312960	22.83%	2.996%
15	4.283	991	993	996	rBV3	978	635	0.05%	0.006%
16	4.373	1003	1021	1043	rBV	229148	562121	41.00%	5.380%
17	4.598	1089	1091	1096	rVB5	1670	1190	0.09%	0.011%
18	4.624	1096	1099	1102	rBV4	1617	1517	0.11%	0.015%
19	4.833	1162	1164	1165	rBV2	1148	640	0.05%	0.006%
20	4.910	1185	1188	1190	rBV4	1213	780	0.06%	0.007%
21	5.071	1220	1238	1246	rBV2	549693	1371126	100.00%	13.124%
22	5.553	1386	1388	1391	rBV4	1289	842	0.06%	0.008%
23	5.579	1391	1396	1399	rBV7	1208	1088	0.08%	0.010%
24	5.640	1402	1415	1440	rBV	425437	849757	61.98%	8.134%
25	5.933	1494	1506	1516	rBV7	9050	20462	1.49%	0.196%
26	6.093	1543	1556	1577	rBV	321604	636929	46.45%	6.097%
27	6.457	1665	1669	1673	rBV7	1427	1447	0.11%	0.014%
28	6.547	1694	1697	1699	rBV3	1400	901	0.07%	0.009%
29	6.576	1704	1706	1709	rVV3	1384	783	0.06%	0.007%
30	6.592	1709	1711	1713	rVV3	1157	615	0.04%	0.006%
31	6.640	1721	1726	1729	rBV6	2427	2420	0.18%	0.023%
32	6.762	1762	1764	1766	rBV3	1266	657	0.05%	0.006%
33	6.820	1780	1782	1788	rVB7	1773	1570	0.11%	0.015%
34	6.846	1788	1790	1793	rBV3	852	559	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016632.D
 Acq On : 07 Jun 2020 10:08
 Operator : SY/MD
 Sample : L2862-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D89DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.894	1803	1805	1807	rBV3	908	495	0.04%	0.005%
36	6.942	1816	1820	1822	rBV4	1235	914	0.07%	0.009%
37	6.968	1825	1828	1829	rBV2	980	598	0.04%	0.006%
38	7.006	1829	1840	1859	rBV	162621	292769	21.35%	2.802%
39	7.338	1930	1943	1960	rBV	645425	1105778	80.65%	10.584%
40	7.643	2027	2038	2053	rBV	115888	196179	14.31%	1.878%
41	7.855	2102	2104	2109	rBV5	1149	766	0.06%	0.007%
42	7.916	2117	2123	2128	rBV7	1353	1833	0.13%	0.018%
43	7.945	2128	2132	2133	rBV4	1058	688	0.05%	0.007%
44	8.106	2172	2182	2198	rBV	374878	647780	47.24%	6.200%
45	8.373	2263	2265	2269	rBV4	1712	1366	0.10%	0.013%
46	8.412	2276	2277	2285	rBV9	1258	954	0.07%	0.009%
47	8.486	2296	2300	2304	rBV6	1725	1929	0.14%	0.018%
48	8.640	2345	2348	2349	rBV3	1174	681	0.05%	0.007%
49	8.701	2363	2367	2369	rBV4	1164	651	0.05%	0.006%
50	8.875	2409	2421	2449	rBV	638299	1032881	75.33%	9.886%
51	9.039	2463	2472	2481	rBV	19770	31774	2.32%	0.304%
52	9.286	2541	2549	2553	rBV10	3978	6344	0.46%	0.061%
53	9.521	2617	2622	2623	rBV3	1260	1071	0.08%	0.010%
54	9.569	2632	2637	2642	rBV6	2834	3241	0.24%	0.031%
55	9.920	2744	2746	2749	rBV2	1439	879	0.06%	0.008%
56	10.019	2773	2777	2782	rBV7	1769	1750	0.13%	0.017%
57	10.064	2787	2791	2792	rBV4	1324	1128	0.08%	0.011%
58	10.238	2834	2845	2860	rBV	400924	630211	45.96%	6.032%
59	10.608	2957	2960	2963	rBV4	1480	910	0.07%	0.009%
60	10.762	3005	3008	3011	rBV4	1949	1772	0.13%	0.017%
61	10.974	3072	3074	3077	rBV2	1602	978	0.07%	0.009%
62	11.270	3155	3166	3182	rBV	613973	934388	68.15%	8.944%
63	11.646	3272	3283	3299	rBV	635848	1011019	73.74%	9.677%
64	11.755	3315	3317	3318	rBV2	1413	551	0.04%	0.005%
65	11.971	3381	3384	3388	rBV5	1331	935	0.07%	0.009%
66	12.029	3400	3402	3403	rBV2	1119	581	0.04%	0.006%
67	12.096	3420	3423	3424	rBV3	1168	682	0.05%	0.007%
68	12.489	3541	3545	3546	rBV3	1273	774	0.06%	0.007%
69	12.630	3588	3589	3593	rBV4	1151	529	0.04%	0.005%
70	12.669	3599	3601	3604	rBV3	1006	596	0.04%	0.006%
71	12.720	3616	3617	3621	rBV4	1284	776	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016632.D
 Acq On : 07 Jun 2020 10:08
 Operator : SY/MD
 Sample : L2862-06DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D89DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.858	3656	3660	3663	rBV5	1233	997	0.07%	0.010%
73	12.900	3671	3673	3675	rBV3	1911	1166	0.09%	0.011%
74	12.948	3684	3688	3692	rBV6	2078	1794	0.13%	0.017%
75	13.009	3703	3707	3709	rBV5	1703	1206	0.09%	0.012%
76	13.164	3753	3755	3758	rVB3	1251	526	0.04%	0.005%
77	13.180	3758	3760	3763	rBV4	1154	609	0.04%	0.006%
78	13.235	3775	3777	3780	rVB4	1173	637	0.05%	0.006%
79	13.296	3793	3796	3798	rBV3	1334	735	0.05%	0.007%
80	13.341	3808	3810	3814	rBV5	989	653	0.05%	0.006%
81	13.447	3840	3843	3844	rBV3	981	487	0.04%	0.005%
82	13.466	3844	3849	3852	rVB4	1284	935	0.07%	0.009%
83	13.508	3858	3862	3863	rBV4	1798	1040	0.08%	0.010%
84	13.611	3892	3894	3898	rBV3	959	627	0.05%	0.006%
85	13.788	3947	3949	3953	rBV3	885	552	0.04%	0.005%
86	13.900	3982	3984	3989	rVB4	1352	884	0.06%	0.008%
87	13.993	4012	4013	4017	rVB4	1086	545	0.04%	0.005%
88	14.025	4017	4023	4034	rBV10	1729	3712	0.27%	0.036%
89	14.135	4054	4057	4062	rBV6	1417	943	0.07%	0.009%
90	14.251	4092	4093	4095	rBV2	1444	635	0.05%	0.006%
91	14.476	4160	4163	4164	rBV3	1538	882	0.06%	0.008%
92	14.559	4187	4189	4192	rBV3	1194	882	0.06%	0.008%
93	14.607	4200	4204	4206	rBV4	2035	1643	0.12%	0.016%
94	14.678	4223	4226	4229	rBV3	1952	1640	0.12%	0.016%
95	14.736	4242	4244	4247	rVB3	1234	597	0.04%	0.006%
96	14.829	4269	4273	4276	rBV6	1552	1577	0.12%	0.015%
97	15.173	4376	4380	4381	rBV3	2330	1343	0.10%	0.013%
98	15.218	4388	4394	4396	rBV7	1975	1841	0.13%	0.018%
99	15.308	4420	4422	4424	rBV2	1401	510	0.04%	0.005%
100	15.408	4451	4453	4456	rBV4	1205	747	0.05%	0.007%


Sum of corrected areas: 10447421

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016632.D
Acq On : 07 Jun 2020 10:08
Operator : SY/MD
Sample : L2862-06DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D89DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

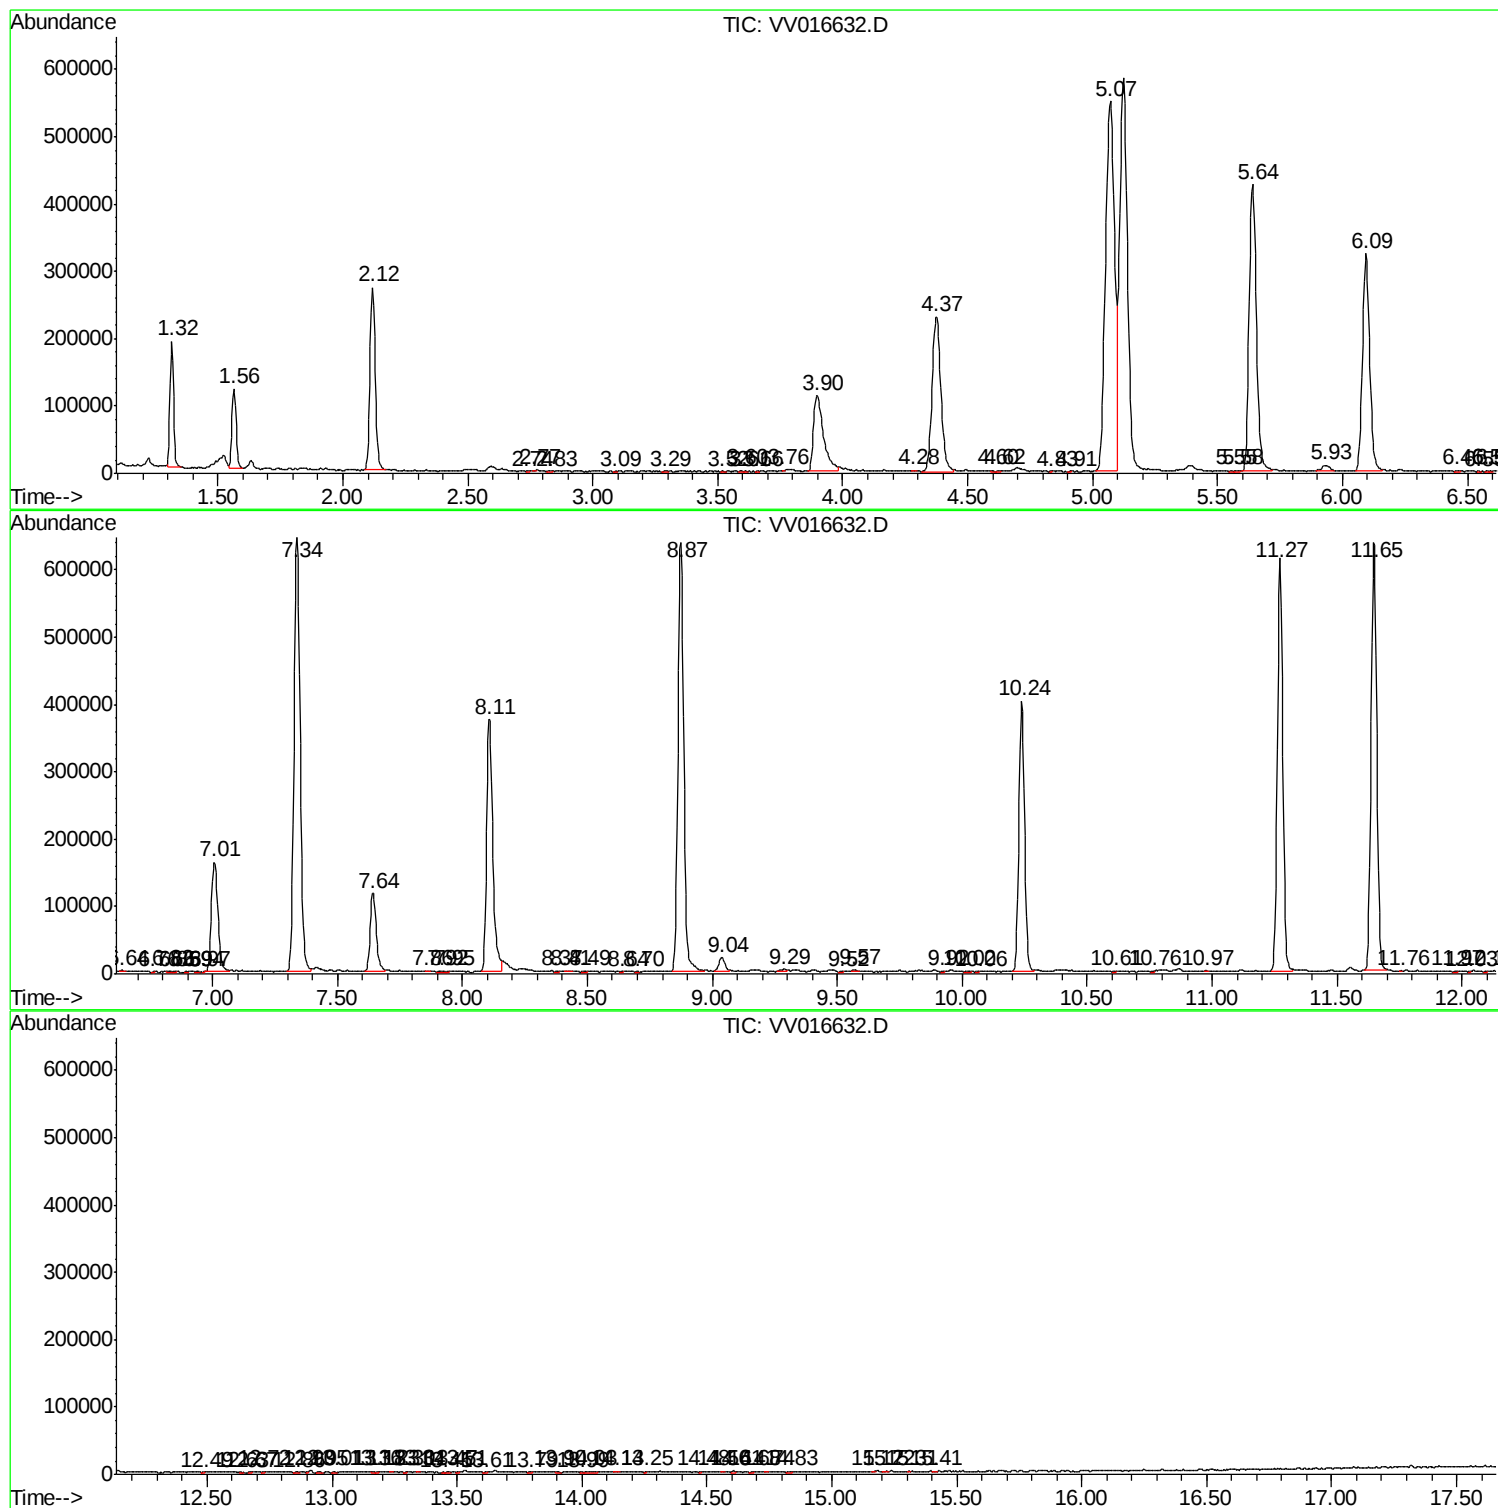

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016632.D
Acq On : 07 Jun 2020 10:08
Operator : SY/MD
Sample : L2862-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D89DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016632.D
Acq On : 07 Jun 2020 10:08
Operator : SY/MD
Sample : L2862-06DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9D89DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc