

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016636.D
 Acq On : 07 Jun 2020 11:42
 Operator : SY/MD
 Sample : L2862-10DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D94DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	189398	196513	13.98%	1.846%
2	1.563	143	147	160	rVB	113879	124654	8.87%	1.171%
3	2.119	310	320	335	rBV	270369	400232	28.47%	3.759%
4	2.306	375	378	379	rBV3	1377	848	0.06%	0.008%
5	2.753	511	517	520	rBV6	2021	2416	0.17%	0.023%
6	2.830	537	541	544	rVB5	1850	1271	0.09%	0.012%
7	2.891	557	560	564	rBV4	1371	1091	0.08%	0.010%
8	2.997	589	593	598	rBV8	1205	1139	0.08%	0.011%
9	3.055	606	611	614	rBV6	898	1063	0.08%	0.010%
10	3.084	618	620	625	rVB4	1617	978	0.07%	0.009%
11	3.222	660	663	665	rBV3	1787	1173	0.08%	0.011%
12	3.309	689	690	696	rVB4	1153	871	0.06%	0.008%
13	3.351	701	703	707	rVB5	1881	906	0.06%	0.009%
14	3.531	756	759	763	rVB5	990	792	0.06%	0.007%
15	3.611	782	784	788	rBV4	1246	1194	0.08%	0.011%
16	3.685	805	807	812	rVB4	1158	805	0.06%	0.008%
17	3.727	819	820	825	rVB4	1463	962	0.07%	0.009%
18	3.775	829	835	836	rBV4	3949	3644	0.26%	0.034%
19	3.901	863	874	905	rBV	108750	318572	22.66%	2.992%
20	4.373	1006	1021	1045	rBV	228070	549579	39.09%	5.162%
21	4.611	1092	1095	1097	rBV4	1835	1018	0.07%	0.010%
22	4.630	1100	1101	1105	rVB3	1853	900	0.06%	0.008%
23	4.692	1111	1120	1121	rBV7	5617	6056	0.43%	0.057%
24	4.788	1147	1150	1153	rVB5	1337	1013	0.07%	0.010%
25	4.807	1153	1156	1158	rBV3	1071	782	0.06%	0.007%
26	4.859	1169	1172	1174	rBV4	1473	886	0.06%	0.008%
27	4.904	1182	1186	1188	rBV2	1526	841	0.06%	0.008%
28	4.952	1196	1201	1203	rBV6	1306	1121	0.08%	0.011%
29	5.071	1221	1238	1246	rBV2	559459	1405803	100.00%	13.204%
30	5.572	1391	1394	1396	rBV4	1407	870	0.06%	0.008%
31	5.640	1402	1415	1435	rBV	436015	860863	61.24%	8.086%
32	5.926	1497	1504	1506	rBV7	8065	8776	0.62%	0.082%
33	6.093	1542	1556	1577	rBV	318604	643839	45.80%	6.047%
34	6.376	1642	1644	1652	rVB9	2499	2037	0.14%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016636.D
 Acq On : 07 Jun 2020 11:42
 Operator : SY/MD
 Sample : L2862-10DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D94DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.486	1674	1678	1682	rBV5	1468	1394	0.10%	0.013%
36	6.624	1719	1721	1723	rBV3	1654	801	0.06%	0.008%
37	6.720	1747	1751	1755	rBV8	1701	1200	0.09%	0.011%
38	6.775	1765	1768	1771	rBV4	1759	1018	0.07%	0.010%
39	6.826	1780	1784	1785	rBV2	1806	1398	0.10%	0.013%
40	6.897	1804	1806	1810	rVV5	1100	771	0.05%	0.007%
41	7.007	1829	1840	1858	rBV	163087	291623	20.74%	2.739%
42	7.177	1889	1893	1895	rBV5	2010	1692	0.12%	0.016%
43	7.338	1931	1943	1960	rVV	655765	1110259	78.98%	10.428%
44	7.640	2028	2037	2058	rBV	117376	195862	13.93%	1.840%
45	7.807	2087	2089	2090	rBV2	1670	801	0.06%	0.008%
46	7.971	2138	2140	2144	rBV4	1106	885	0.06%	0.008%
47	8.055	2162	2166	2170	rVB7	1275	943	0.07%	0.009%
48	8.109	2172	2183	2214	rBV	352935	673672	47.92%	6.328%
49	8.489	2296	2301	2304	rBV5	1849	1232	0.09%	0.012%
50	8.749	2378	2382	2385	rBV5	1379	1002	0.07%	0.009%
51	8.875	2409	2421	2450	rBV	633688	1037234	73.78%	9.742%
52	9.035	2462	2471	2485	rVB	58657	95187	6.77%	0.894%
53	9.328	2557	2562	2563	rBV3	3235	2953	0.21%	0.028%
54	9.402	2580	2585	2588	rBV5	3585	3465	0.25%	0.033%
55	9.569	2629	2637	2642	rBV4	5294	8424	0.60%	0.079%
56	9.736	2687	2689	2690	rBV2	1668	767	0.05%	0.007%
57	9.775	2699	2701	2705	rBV3	1025	790	0.06%	0.007%
58	9.817	2711	2714	2715	rBV3	1790	1099	0.08%	0.010%
59	9.952	2750	2756	2759	rBV7	2497	2537	0.18%	0.024%
60	9.987	2765	2767	2771	rBV5	961	799	0.06%	0.008%
61	10.103	2799	2803	2808	rVB7	1894	1950	0.14%	0.018%
62	10.238	2831	2845	2860	rBV	410863	638848	45.44%	6.000%
63	10.537	2936	2938	2942	rVB5	2384	1519	0.11%	0.014%
64	10.585	2947	2953	2957	rVB9	1960	2197	0.16%	0.021%
65	10.717	2991	2994	2996	rBV3	1918	1385	0.10%	0.013%
66	10.736	2996	3000	3001	rBV3	1201	814	0.06%	0.008%
67	11.270	3153	3166	3186	rBV	616696	954682	67.91%	8.967%
68	11.646	3270	3283	3301	rBV	656041	1026643	73.03%	9.643%
69	11.920	3366	3368	3372	rBV6	1337	1259	0.09%	0.012%
70	11.993	3389	3391	3393	rBV3	1441	834	0.06%	0.008%
71	12.206	3454	3457	3461	rBV4	1512	1358	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016636.D
 Acq On : 07 Jun 2020 11:42
 Operator : SY/MD
 Sample : L2862-10DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D94DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.260	3467	3474	3476	rBV8	1343	1574	0.11%	0.015%
73	12.363	3502	3506	3508	rBV3	1009	986	0.07%	0.009%
74	12.373	3508	3509	3512	rVV3	1639	1070	0.08%	0.010%
75	12.411	3519	3521	3524	rVB4	1288	809	0.06%	0.008%
76	12.543	3559	3562	3564	rBV4	1697	953	0.07%	0.009%
77	12.662	3596	3599	3601	rBV4	1647	831	0.06%	0.008%
78	12.701	3609	3611	3616	rVB5	1172	1019	0.07%	0.010%
79	12.784	3633	3637	3642	rBV6	1236	986	0.07%	0.009%
80	13.022	3707	3711	3712	rBV4	1682	1129	0.08%	0.011%
81	13.193	3760	3764	3765	rBV3	1289	1000	0.07%	0.009%
82	13.228	3771	3775	3778	rVB6	1024	811	0.06%	0.008%
83	13.264	3781	3786	3789	rBV6	1355	1383	0.10%	0.013%
84	13.440	3835	3841	3845	rBV8	1256	1382	0.10%	0.013%
85	13.466	3845	3849	3854	rBV8	2286	2004	0.14%	0.019%
86	13.489	3854	3856	3861	rVB4	1799	940	0.07%	0.009%
87	13.530	3863	3869	3871	rBV6	3071	3102	0.22%	0.029%
88	13.604	3887	3892	3894	rBV5	1411	1157	0.08%	0.011%
89	13.649	3902	3906	3907	rBV4	1660	1033	0.07%	0.010%
90	13.768	3940	3943	3945	rBV4	1223	786	0.06%	0.007%
91	13.810	3953	3956	3959	rVB4	1395	839	0.06%	0.008%
92	13.836	3962	3964	3970	rVB7	1089	870	0.06%	0.008%
93	13.993	4009	4013	4014	rBV3	1481	965	0.07%	0.009%
94	14.141	4057	4059	4064	rBV5	1042	770	0.05%	0.007%
95	14.180	4069	4071	4075	rVB4	1861	1108	0.08%	0.010%
96	14.289	4103	4105	4107	rBV2	1265	749	0.05%	0.007%
97	14.707	4232	4235	4240	rBV7	1282	1294	0.09%	0.012%
98	14.971	4313	4317	4321	rBV7	1399	1337	0.10%	0.013%
99	15.308	4418	4422	4425	rBV6	1771	1512	0.11%	0.014%
100	15.360	4435	4438	4443	rBV6	1438	1481	0.11%	0.014%


Sum of corrected areas: 10646685

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016636.D
Acq On : 07 Jun 2020 11:42
Operator : SY/MD
Sample : L2862-10DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D94DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

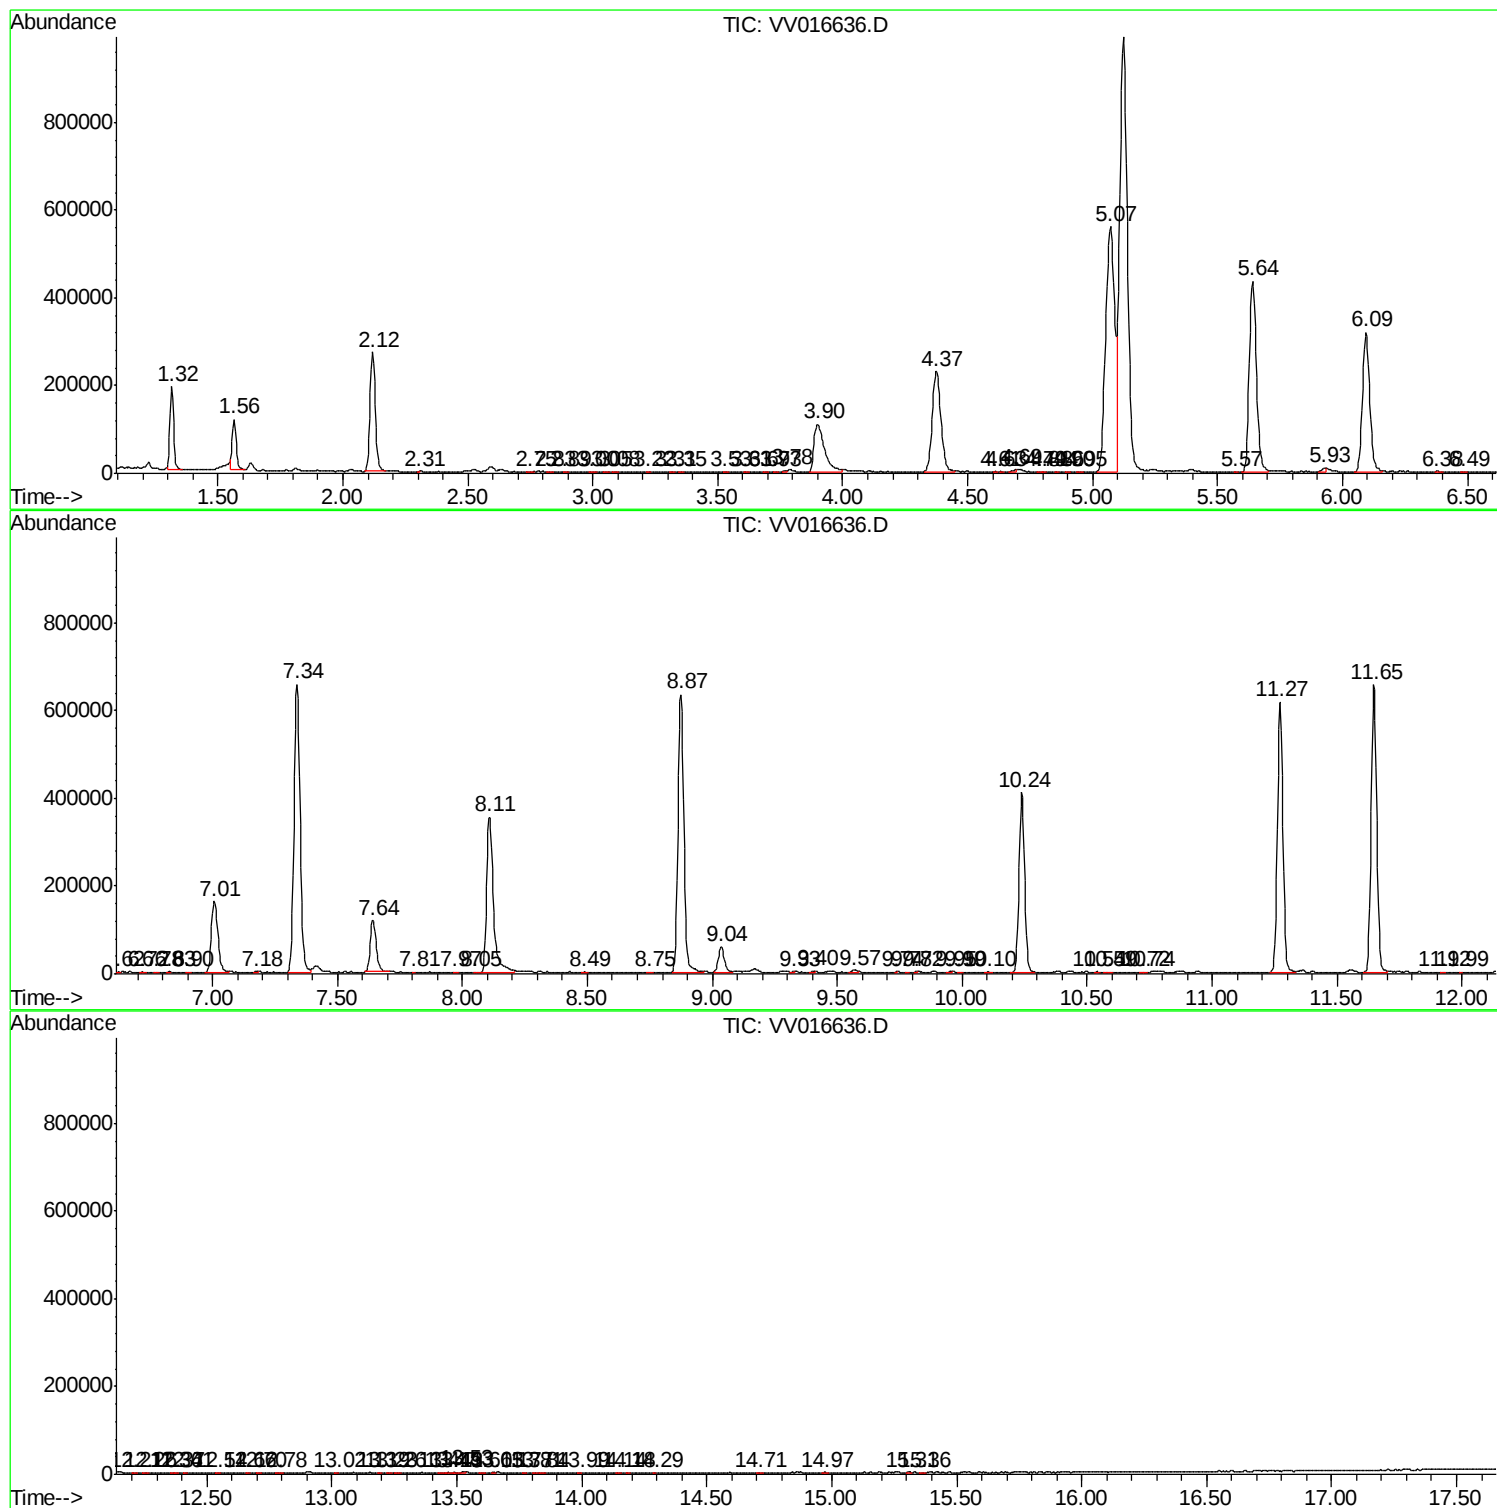

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016636.D
Acq On : 07 Jun 2020 11:42
Operator : SY/MD
Sample : L2862-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D94DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016636.D
Acq On : 07 Jun 2020 11:42
Operator : SY/MD
Sample : L2862-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 63 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D94DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc