

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016638.D
 Acq On : 07 Jun 2020 12:30
 Operator : SY/MD
 Sample : L2862-12DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D99DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	62	70	80	rVB	209508	226123	17.39%	2.082%
2	1.566	141	148	158	rVB	120109	144722	11.13%	1.333%
3	2.119	311	320	336	rVB	262698	389871	29.98%	3.590%
4	2.592	456	467	480	rBV2	18010	37837	2.91%	0.348%
5	2.856	547	549	554	rBV5	1316	1079	0.08%	0.010%
6	2.894	559	561	562	rBV2	1627	578	0.04%	0.005%
7	3.042	605	607	608	rBV2	1156	329	0.03%	0.003%
8	3.106	623	627	628	rBV4	950	634	0.05%	0.006%
9	3.132	633	635	636	rBV2	787	272	0.02%	0.003%
10	3.177	647	649	654	rVB5	2148	1761	0.14%	0.016%
11	3.373	708	710	711	rBV2	889	431	0.03%	0.004%
12	3.557	764	767	770	rBV3	1112	685	0.05%	0.006%
13	3.573	770	772	774	rBV3	1103	639	0.05%	0.006%
14	3.669	798	802	804	rBV4	1945	1507	0.12%	0.014%
15	3.897	863	873	898	rBV2	111150	296759	22.82%	2.732%
16	4.184	959	962	966	rBV5	1116	1124	0.09%	0.010%
17	4.248	980	982	983	rBV2	1039	375	0.03%	0.003%
18	4.373	1008	1021	1045	rVB	224920	541180	41.61%	4.983%
19	4.888	1179	1181	1185	rBV5	1434	961	0.07%	0.009%
20	4.917	1189	1190	1195	rVB3	1139	517	0.04%	0.005%
21	4.949	1198	1200	1203	rBV5	786	519	0.04%	0.005%
22	5.071	1219	1238	1244	rBV2	553053	1300528	100.00%	11.975%
23	5.640	1403	1415	1435	rBV	415243	811707	62.41%	7.474%
24	6.093	1543	1556	1578	rBV	312809	630724	48.50%	5.808%
25	6.454	1666	1668	1669	rBV2	1572	677	0.05%	0.006%
26	6.524	1688	1690	1694	rVB4	2030	1136	0.09%	0.010%
27	6.544	1694	1696	1698	rBV4	1316	806	0.06%	0.007%
28	6.859	1793	1794	1797	rVB3	1546	646	0.05%	0.006%
29	7.007	1829	1840	1860	rBV	163470	289525	22.26%	2.666%
30	7.338	1931	1943	1956	rBV	638785	1085436	83.46%	9.994%
31	7.409	1958	1965	1983	rVB	170159	297598	22.88%	2.740%
32	7.640	2029	2037	2053	rBV	113101	185054	14.23%	1.704%
33	7.945	2129	2132	2135	rBV5	1132	994	0.08%	0.009%
34	8.106	2172	2182	2214	rBV	374701	681843	52.43%	6.278%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016638.D
 Acq On : 07 Jun 2020 12:30
 Operator : SY/MD
 Sample : L2862-12DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D99DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	8.412	2274	2277	2280	rBV3	1790	1363	0.10%	0.013%
36	8.666	2349	2356	2359	rBV8	1387	1986	0.15%	0.018%
37	8.714	2366	2371	2374	rBV6	1690	1528	0.12%	0.014%
38	8.875	2410	2421	2432	rBV	603692	976567	75.09%	8.992%
39	9.032	2461	2470	2484	rBV	180363	291637	22.42%	2.685%
40	9.408	2579	2587	2599	rBV6	13060	22818	1.75%	0.210%
41	10.106	2793	2804	2816	rBV6	8941	17793	1.37%	0.164%
42	10.238	2834	2845	2858	rBV	409713	639880	49.20%	5.892%
43	11.228	3151	3153	3155	rBV3	2111	1067	0.08%	0.010%
44	11.270	3155	3166	3185	rVB	612624	933071	71.75%	8.592%
45	11.646	3273	3283	3301	rVB	633219	1012973	77.89%	9.327%
46	12.781	3632	3636	3639	rBV5	1954	1505	0.12%	0.014%
47	13.534	3862	3870	3880	rBV3	8412	13768	1.06%	0.127%
48	13.720	3925	3928	3929	rBV4	1308	705	0.05%	0.006%
49	13.765	3940	3942	3944	rBV3	1609	858	0.07%	0.008%
50	13.807	3953	3955	3956	rBV2	935	349	0.03%	0.003%
51	13.907	3983	3986	3987	rBV3	1157	700	0.05%	0.006%
52	13.958	4000	4002	4003	rBV2	1531	666	0.05%	0.006%
53	14.035	4021	4026	4028	rBV5	2176	1936	0.15%	0.018%
54	14.080	4037	4040	4043	rVB4	1415	1004	0.08%	0.009%
55	14.257	4093	4095	4096	rBV2	800	291	0.02%	0.003%
56	14.382	4132	4134	4138	rBV5	913	452	0.03%	0.004%
57	14.450	4153	4155	4159	rBV4	1638	1199	0.09%	0.011%
58	14.624	4207	4209	4211	rBV3	948	416	0.03%	0.004%
59	14.733	4241	4243	4245	rBV3	1237	611	0.05%	0.006%
60	14.839	4274	4276	4278	rBV3	1657	662	0.05%	0.006%


Sum of corrected areas: 10860382

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016638.D
Acq On : 07 Jun 2020 12:30
Operator : SY/MD
Sample : L2862-12DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D99DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

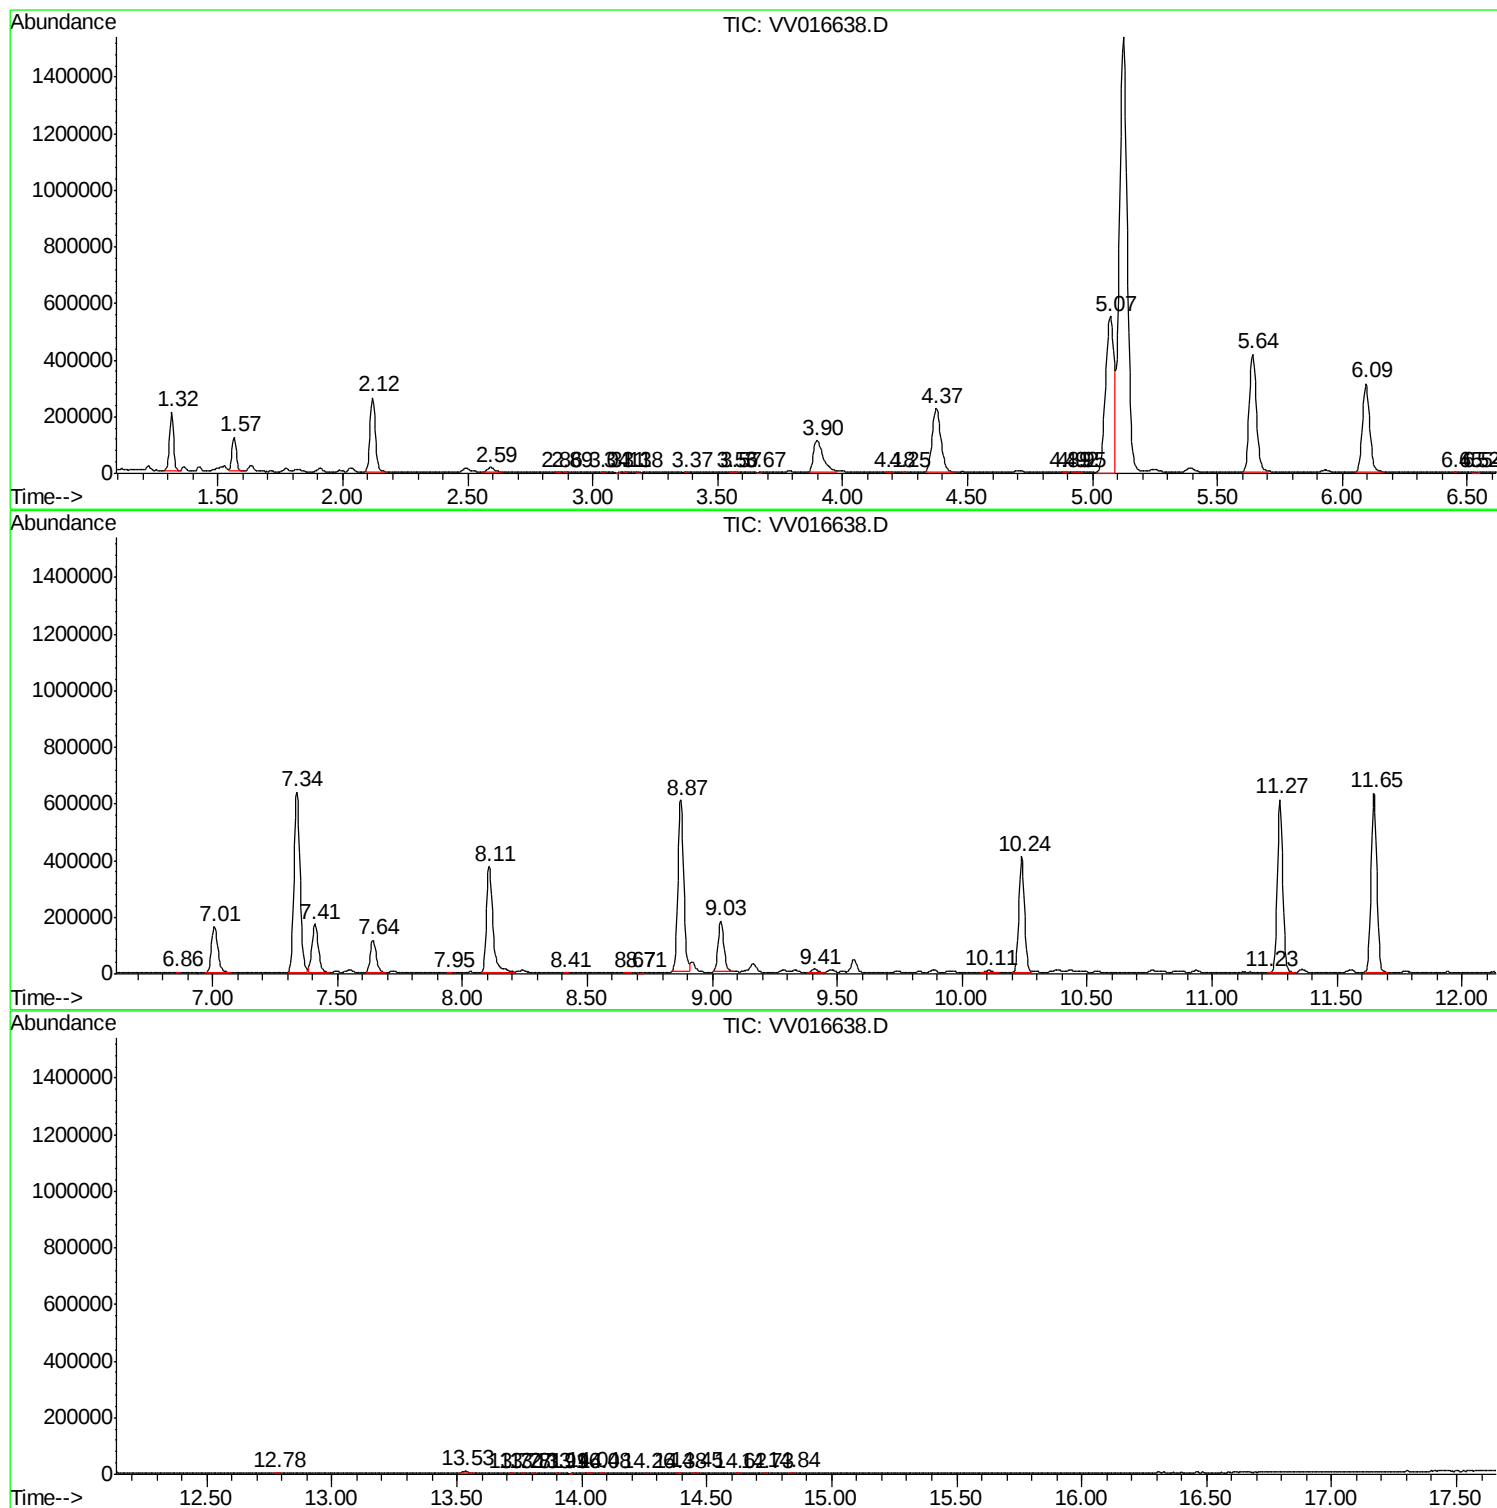

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016638.D
Acq On : 07 Jun 2020 12:30
Operator : SY/MD
Sample : L2862-12DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D99DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016638.D
Acq On : 07 Jun 2020 12:30
Operator : SY/MD
Sample : L2862-12DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D99DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc