

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016641.D
 Acq On : 07 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2861-08DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	179744	186106	6.94%	1.219%
2	1.563	142	147	157	rVB	122102	142060	5.30%	0.931%
3	2.119	310	320	341	rVB	279907	415983	15.52%	2.726%
4	2.267	365	366	369	rBV3	1267	674	0.03%	0.004%
5	2.749	512	516	519	rBV6	1336	1127	0.04%	0.007%
6	2.891	557	560	564	rBV4	1038	1026	0.04%	0.007%
7	2.923	567	570	573	rBV5	1425	1087	0.04%	0.007%
8	2.945	573	577	578	rBV4	1224	1001	0.04%	0.007%
9	3.158	640	643	645	rBV2	1598	911	0.03%	0.006%
10	3.171	645	647	652	rVV5	1007	785	0.03%	0.005%
11	3.373	705	710	713	rVV7	1689	1537	0.06%	0.010%
12	3.389	713	715	719	rVB5	1659	1156	0.04%	0.008%
13	3.704	811	813	817	rVB5	1008	615	0.02%	0.004%
14	3.743	822	825	827	rBV4	1211	835	0.03%	0.005%
15	3.894	862	872	902	rBV	108579	296365	11.05%	1.942%
16	4.248	978	982	986	rVB6	1497	1369	0.05%	0.009%
17	4.309	996	1001	1004	rBV7	1140	1349	0.05%	0.009%
18	4.373	1004	1021	1043	rBV	234967	572622	21.36%	3.752%
19	4.563	1075	1080	1081	rBV3	1394	993	0.04%	0.007%
20	4.611	1092	1095	1096	rVV3	1813	1004	0.04%	0.007%
21	4.643	1100	1105	1108	rVB7	1468	1244	0.05%	0.008%
22	4.891	1180	1182	1187	rBV4	1463	1054	0.04%	0.007%
23	4.923	1187	1192	1193	rBV4	1120	828	0.03%	0.005%
24	4.958	1197	1203	1208	rBV8	1596	1963	0.07%	0.013%
25	5.071	1220	1238	1246	rBV3	569480	1442411	53.80%	9.451%
26	5.582	1394	1397	1401	rBV4	1327	1117	0.04%	0.007%
27	5.640	1402	1415	1438	rBV	450406	890650	33.22%	5.836%
28	5.781	1457	1459	1463	rVB5	1849	1134	0.04%	0.007%
29	5.865	1484	1485	1490	rVB4	1409	766	0.03%	0.005%
30	6.093	1541	1556	1585	rBV	328009	663987	24.77%	4.351%
31	6.402	1650	1652	1655	rBV2	1701	763	0.03%	0.005%
32	6.479	1673	1676	1679	rVV3	1734	1070	0.04%	0.007%
33	6.550	1694	1698	1700	rBV3	1359	923	0.03%	0.006%
34	6.778	1767	1769	1770	rBV2	1350	608	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016641.D
 Acq On : 07 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2861-08DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.814	1778	1780	1782	rBV2	2179	1384	0.05%	0.009%
36	6.852	1790	1792	1795	rBV4	1080	654	0.02%	0.004%
37	7.006	1829	1840	1858	rBV	170437	299240	11.16%	1.961%
38	7.151	1883	1885	1888	rBV4	1752	1159	0.04%	0.008%
39	7.293	1925	1929	1931	rBV5	1131	985	0.04%	0.006%
40	7.338	1931	1943	1954	rVV	672646	1147095	42.78%	7.516%
41	7.408	1955	1965	1987	rVB	1598159	2681083	100.00%	17.567%
42	7.643	2027	2038	2053	rBV	119892	198719	7.41%	1.302%
43	7.990	2142	2146	2147	rBV3	2050	1051	0.04%	0.007%
44	8.106	2172	2182	2215	rVV	381857	690323	25.75%	4.523%
45	8.476	2295	2297	2303	rVV6	1389	1391	0.05%	0.009%
46	8.614	2336	2340	2342	rBV5	894	597	0.02%	0.004%
47	8.649	2349	2351	2354	rBV3	864	687	0.03%	0.005%
48	8.807	2398	2400	2406	rVB6	1709	1320	0.05%	0.009%
49	8.875	2406	2421	2443	rBV	665252	1094425	40.82%	7.171%
50	9.032	2459	2470	2485	rBV	528070	824025	30.73%	5.399%
51	9.157	2502	2509	2536	rVB	212384	361194	13.47%	2.367%
52	9.254	2536	2539	2541	rBV4	1763	1058	0.04%	0.007%
53	9.405	2577	2586	2595	rBV6	8676	15111	0.56%	0.099%
54	9.566	2627	2636	2652	rVB	198153	309310	11.54%	2.027%
55	9.714	2680	2682	2683	rBV2	1416	701	0.03%	0.005%
56	9.801	2702	2709	2711	rBV7	4903	5529	0.21%	0.036%
57	9.881	2728	2734	2735	rBV6	4514	4055	0.15%	0.027%
58	9.958	2750	2758	2765	rVB3	10888	15368	0.57%	0.101%
59	10.071	2789	2793	2794	rBV3	1255	985	0.04%	0.006%
60	10.106	2794	2804	2814	rVV3	6884	13348	0.50%	0.087%
61	10.238	2834	2845	2858	rBV	425527	656258	24.48%	4.300%
62	10.762	2999	3008	3016	rBV2	18982	34245	1.28%	0.224%
63	10.845	3030	3034	3036	rBV5	2862	2667	0.10%	0.017%
64	10.939	3054	3063	3072	rBV	26321	40383	1.51%	0.265%
65	11.051	3096	3098	3100	rBV3	1386	847	0.03%	0.006%
66	11.270	3155	3166	3182	rBV	665004	1027159	38.31%	6.730%
67	11.360	3187	3194	3206	rVB	22579	35055	1.31%	0.230%
68	11.553	3246	3254	3266	rVB3	13487	21372	0.80%	0.140%
69	11.646	3272	3283	3302	rBV	678450	1065851	39.75%	6.984%
70	11.942	3372	3375	3379	rBV5	1880	1481	0.06%	0.010%
71	11.990	3387	3390	3394	rVB5	1373	1079	0.04%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016641.D
 Acq On : 07 Jun 2020 13:41
 Operator : SY/MD
 Sample : L2861-08DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.235	3462	3466	3469	rBV6	697	634	0.02%	0.004%
73	12.299	3482	3486	3488	rBV3	1862	1388	0.05%	0.009%
74	12.334	3493	3497	3498	rBV3	2147	1324	0.05%	0.009%
75	12.453	3530	3534	3538	rBV7	1694	1823	0.07%	0.012%
76	12.717	3613	3616	3618	rBV4	1149	675	0.03%	0.004%
77	12.826	3648	3650	3654	rVB5	1250	864	0.03%	0.006%
78	12.865	3658	3662	3664	rVB5	950	631	0.02%	0.004%
79	12.881	3664	3667	3669	rBV4	1142	777	0.03%	0.005%
80	13.054	3718	3721	3723	rBV3	1386	1029	0.04%	0.007%
81	13.116	3738	3740	3743	rBV4	1560	704	0.03%	0.005%
82	13.331	3803	3807	3809	rBV4	1076	873	0.03%	0.006%
83	13.527	3856	3868	3882	rBV2	22309	39595	1.48%	0.259%
84	13.598	3885	3890	3893	rBV7	1563	1349	0.05%	0.009%
85	13.620	3893	3897	3900	rBV3	1227	1328	0.05%	0.009%
86	13.781	3944	3947	3949	rBV4	1084	815	0.03%	0.005%
87	13.800	3951	3953	3956	rVV3	1196	773	0.03%	0.005%
88	13.816	3956	3958	3963	rVB4	1514	1081	0.04%	0.007%
89	13.903	3981	3985	3987	rBV5	1890	1365	0.05%	0.009%
90	13.939	3993	3996	3999	rBV3	1392	914	0.03%	0.006%
91	14.006	4015	4017	4021	rBV3	1335	775	0.03%	0.005%
92	14.189	4069	4074	4079	rBV9	1795	2372	0.09%	0.016%
93	14.334	4116	4119	4121	rBV4	1363	768	0.03%	0.005%
94	14.363	4126	4128	4130	rBV3	998	602	0.02%	0.004%
95	14.392	4134	4137	4139	rBV3	1442	844	0.03%	0.006%
96	14.511	4172	4174	4177	rBV4	1104	717	0.03%	0.005%
97	14.527	4177	4179	4182	rVV3	1139	591	0.02%	0.004%
98	14.652	4214	4218	4219	rBV2	1178	693	0.03%	0.005%
99	14.794	4260	4262	4266	rBV4	1457	1130	0.04%	0.007%
100	15.115	4360	4362	4366	rBV4	1704	1197	0.04%	0.008%


Sum of corrected areas: 15261948

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016641.D
Acq On : 07 Jun 2020 13:41
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

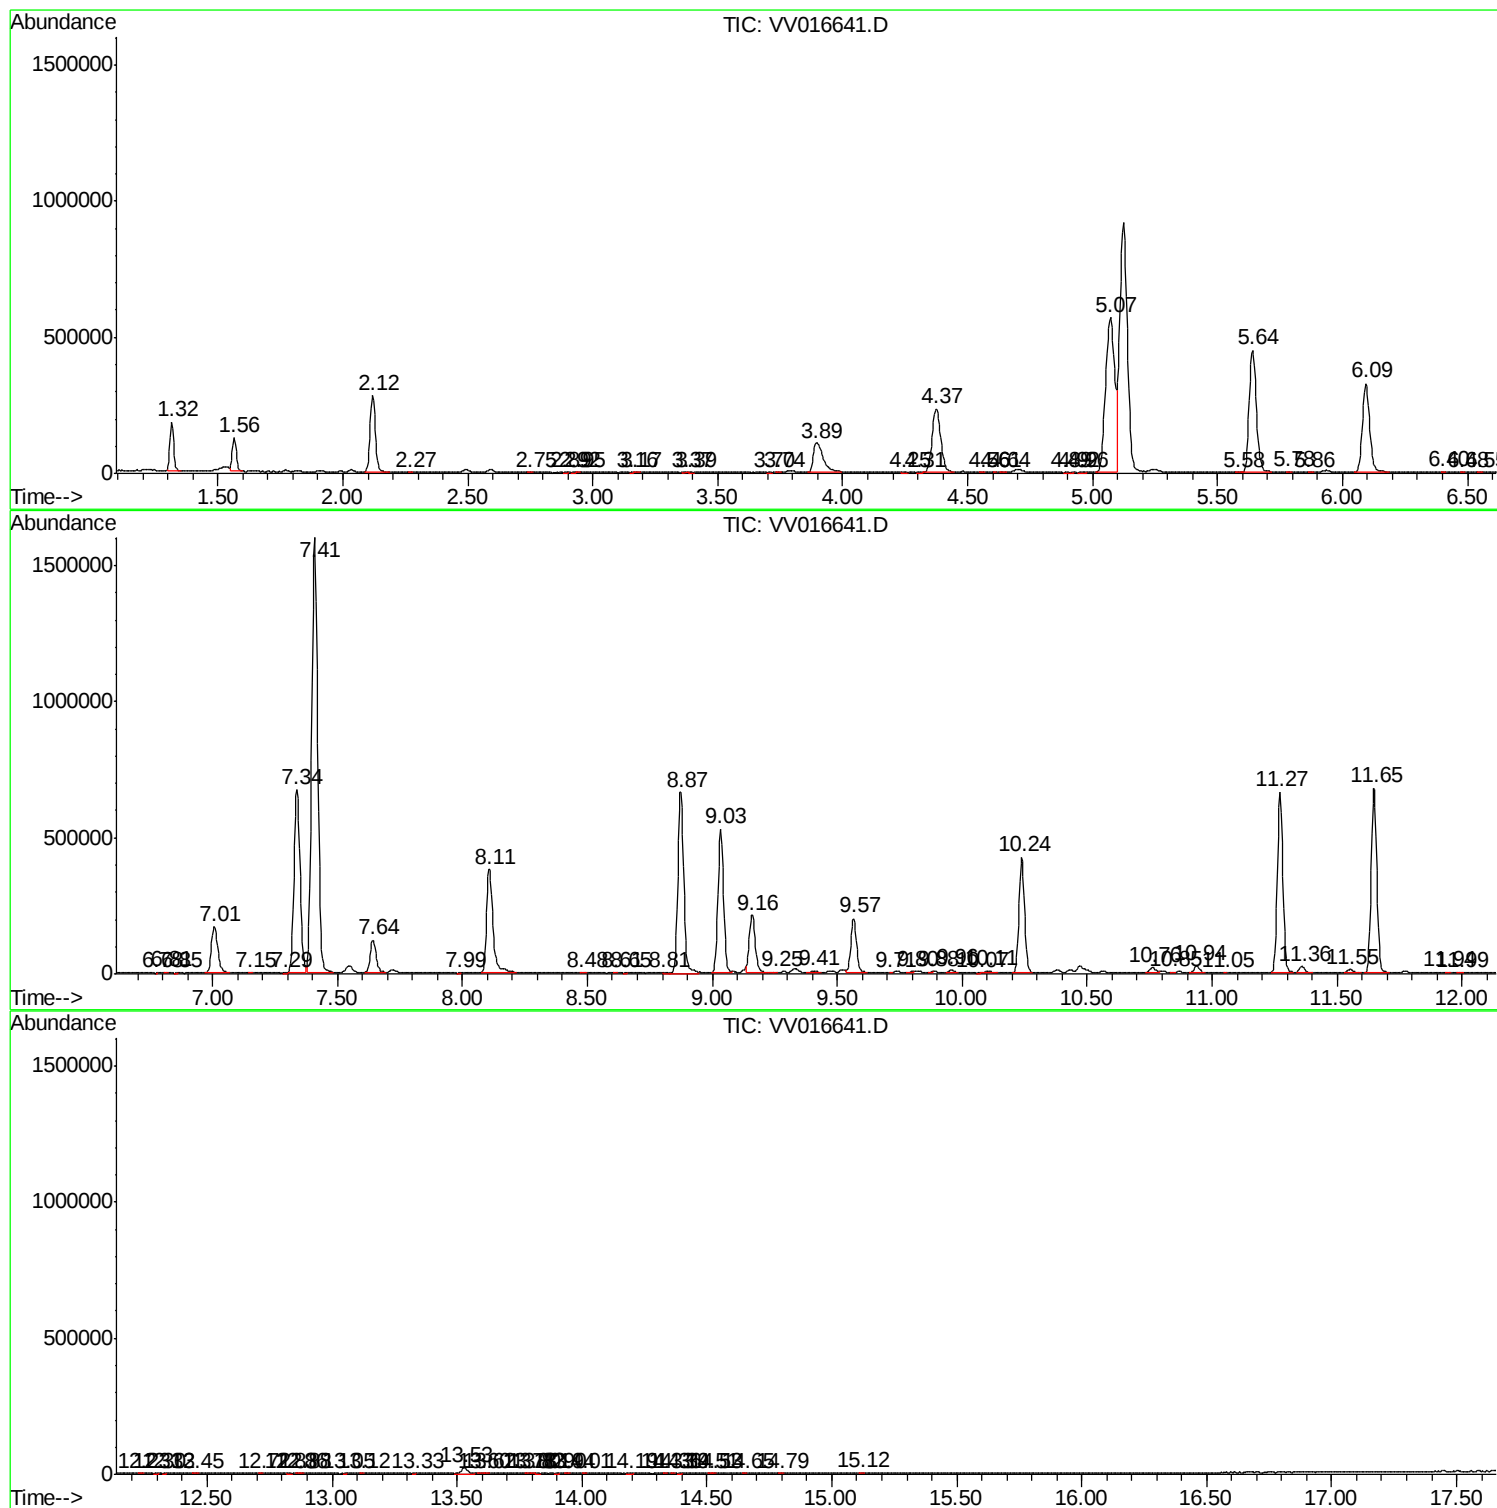

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016641.D
Acq On : 07 Jun 2020 13:41
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016641.D
Acq On : 07 Jun 2020 13:41
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc