

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016643.D
 Acq On : 07 Jun 2020 14:28
 Operator : SY/MD
 Sample : L2861-15DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	61	70	79	rVV2	226528	267962	20.57%	2.366%
2	1.364	81	85	95	rVB	43225	41707	3.20%	0.368%
3	1.425	99	104	113	rVB	37626	39333	3.02%	0.347%
4	1.566	142	148	161	rVB	116069	143283	11.00%	1.265%
5	2.036	288	294	306	rVB	27688	37953	2.91%	0.335%
6	2.119	311	320	336	rVB	265497	394126	30.25%	3.481%
7	2.393	403	405	408	rBV4	1067	637	0.05%	0.006%
8	2.492	428	436	449	rVB2	24388	41402	3.18%	0.366%
9	2.888	554	559	563	rVV8	1456	1264	0.10%	0.011%
10	3.155	636	642	643	rBV4	1339	1195	0.09%	0.011%
11	3.219	659	662	664	rBV3	1834	1148	0.09%	0.010%
12	3.232	664	666	670	rVV5	1629	1387	0.11%	0.012%
13	3.560	764	768	772	rVB6	1285	1429	0.11%	0.013%
14	3.592	772	778	780	rBV6	1757	1703	0.13%	0.015%
15	3.634	789	791	795	rVB4	957	462	0.04%	0.004%
16	3.682	802	806	807	rBV4	1277	833	0.06%	0.007%
17	3.753	820	828	830	rBV8	1599	1725	0.13%	0.015%
18	3.791	830	840	848	rVV8	5612	12441	0.95%	0.110%
19	3.846	853	857	862	rBV7	1464	1747	0.13%	0.015%
20	3.897	863	873	905	rVV	106707	284464	21.84%	2.512%
21	4.274	989	990	994	rVB4	1242	581	0.04%	0.005%
22	4.302	994	999	1001	rBV3	1568	1402	0.11%	0.012%
23	4.315	1001	1003	1005	rVV3	1152	714	0.05%	0.006%
24	4.373	1006	1021	1044	rVV	224196	546841	41.97%	4.829%
25	4.579	1083	1085	1087	rBV4	1356	638	0.05%	0.006%
26	4.704	1110	1124	1139	rBV9	9352	23799	1.83%	0.210%
27	4.846	1164	1168	1174	rVB9	1302	1217	0.09%	0.011%
28	4.875	1174	1177	1178	rBV3	1390	759	0.06%	0.007%
29	4.904	1184	1186	1191	rVB4	1061	789	0.06%	0.007%
30	4.997	1213	1215	1218	rBV3	1396	678	0.05%	0.006%
31	5.071	1221	1238	1244	rBV2	553140	1302786	100.00%	11.505%
32	5.489	1364	1368	1371	rVB6	1779	1185	0.09%	0.010%
33	5.640	1399	1415	1436	rBV	436081	862112	66.17%	7.614%
34	5.852	1479	1481	1485	rVB4	2070	1049	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016643.D
 Acq On : 07 Jun 2020 14:28
 Operator : SY/MD
 Sample : L2861-15DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.875	1485	1488	1490	rBV4	909	578	0.04%	0.005%
36	6.093	1544	1556	1576	rBV	311083	621697	47.72%	5.490%
37	6.380	1643	1645	1648	rBV4	1314	790	0.06%	0.007%
38	6.425	1654	1659	1661	rBV5	2025	1591	0.12%	0.014%
39	6.531	1689	1692	1694	rVB5	1067	551	0.04%	0.005%
40	6.544	1694	1696	1698	rBV3	1466	874	0.07%	0.008%
41	6.736	1755	1756	1759	rBV3	1041	602	0.05%	0.005%
42	6.794	1773	1774	1778	rVB2	915	458	0.04%	0.004%
43	6.894	1803	1805	1808	rBV4	996	641	0.05%	0.006%
44	6.913	1808	1811	1812	rBV2	1030	649	0.05%	0.006%
45	7.007	1827	1840	1858	rBV	162364	292271	22.43%	2.581%
46	7.177	1883	1893	1895	rBV9	3714	5868	0.45%	0.052%
47	7.338	1931	1943	1957	rBV	649088	1105386	84.85%	9.762%
48	7.643	2028	2038	2054	rBV	114259	187728	14.41%	1.658%
49	7.936	2125	2129	2131	rBV4	919	625	0.05%	0.006%
50	7.965	2134	2138	2139	rBV4	1500	824	0.06%	0.007%
51	7.994	2146	2147	2149	rBV2	926	469	0.04%	0.004%
52	8.106	2170	2182	2214	rBV	369679	671201	51.52%	5.928%
53	8.434	2281	2284	2285	rBV2	1450	700	0.05%	0.006%
54	8.531	2312	2314	2319	rVB4	1574	783	0.06%	0.007%
55	8.553	2319	2321	2322	rBV2	1245	586	0.04%	0.005%
56	8.650	2349	2351	2353	rBV3	1100	616	0.05%	0.005%
57	8.707	2365	2369	2371	rBV3	979	614	0.05%	0.005%
58	8.752	2380	2383	2387	rVB4	1254	949	0.07%	0.008%
59	8.785	2392	2393	2396	rBV3	1196	582	0.04%	0.005%
60	8.875	2409	2421	2431	rBV	640738	1027003	78.83%	9.070%
61	9.035	2461	2471	2483	rBV	164149	253902	19.49%	2.242%
62	9.161	2503	2510	2530	rVB2	98608	170354	13.08%	1.504%
63	9.283	2542	2548	2557	rBV6	13562	22977	1.76%	0.203%
64	9.408	2581	2587	2597	rVB5	15610	22903	1.76%	0.202%
65	9.566	2628	2636	2646	rVB	74747	114750	8.81%	1.013%
66	10.071	2790	2793	2795	rBV3	1252	690	0.05%	0.006%
67	10.106	2796	2804	2817	rVB6	11818	21080	1.62%	0.186%
68	10.238	2832	2845	2859	rBV	399807	628919	48.27%	5.554%
69	10.601	2956	2958	2961	rBV4	1857	1066	0.08%	0.009%
70	10.643	2969	2971	2975	rBV4	998	771	0.06%	0.007%
71	10.939	3055	3063	3072	rBV2	17888	26738	2.05%	0.236%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016643.D
 Acq On : 07 Jun 2020 14:28
 Operator : SY/MD
 Sample : L2861-15DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3183	rBV	626007	969121	74.39%	8.559%
73	11.360	3187	3194	3208	rVB2	21096	35634	2.74%	0.315%
74	11.553	3248	3254	3264	rVB3	12205	19621	1.51%	0.173%
75	11.646	3272	3283	3306	rVB	655033	1018900	78.21%	8.998%
76	12.688	3604	3607	3608	rBV3	1187	655	0.05%	0.006%
77	12.804	3640	3643	3646	rBV5	1139	854	0.07%	0.008%
78	12.823	3646	3649	3652	rVV4	1230	982	0.08%	0.009%
79	12.907	3665	3675	3682	rBV4	6602	10732	0.82%	0.095%
80	13.009	3706	3707	3710	rBV4	898	645	0.05%	0.006%
81	13.141	3742	3748	3751	rBV7	1974	2017	0.15%	0.018%
82	13.218	3770	3772	3774	rBV3	1001	607	0.05%	0.005%
83	13.530	3860	3869	3882	rVB	18484	30647	2.35%	0.271%
84	13.653	3898	3907	3914	rBV8	5476	9577	0.74%	0.085%
85	13.955	3999	4001	4005	rBV3	1053	876	0.07%	0.008%
86	13.993	4010	4013	4015	rBV3	759	500	0.04%	0.004%
87	14.042	4026	4028	4031	rVB4	1121	596	0.05%	0.005%
88	14.135	4052	4057	4060	rBV7	1136	1050	0.08%	0.009%
89	14.206	4077	4079	4082	rVB3	1068	523	0.04%	0.005%
90	14.379	4129	4133	4135	rBV6	765	658	0.05%	0.006%
91	14.411	4139	4143	4147	rBV6	1293	1469	0.11%	0.013%
92	14.440	4149	4152	4154	rBV5	1460	790	0.06%	0.007%
93	14.511	4171	4174	4176	rBV4	830	569	0.04%	0.005%
94	14.566	4188	4191	4192	rBV3	1608	788	0.06%	0.007%
95	14.653	4216	4218	4221	rBV4	1365	801	0.06%	0.007%
96	14.720	4236	4239	4242	rBV5	1309	1229	0.09%	0.011%
97	15.135	4366	4368	4372	rBV3	1406	831	0.06%	0.007%
98	15.267	4406	4409	4411	rBV3	1910	1061	0.08%	0.009%
99	15.443	4463	4464	4467	rVB3	1558	609	0.05%	0.005%
100	15.550	4493	4497	4499	rBV4	2018	1492	0.11%	0.013%


Sum of corrected areas: 11323371

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016643.D
Acq On : 07 Jun 2020 14:28
Operator : SY/MD
Sample : L2861-15DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

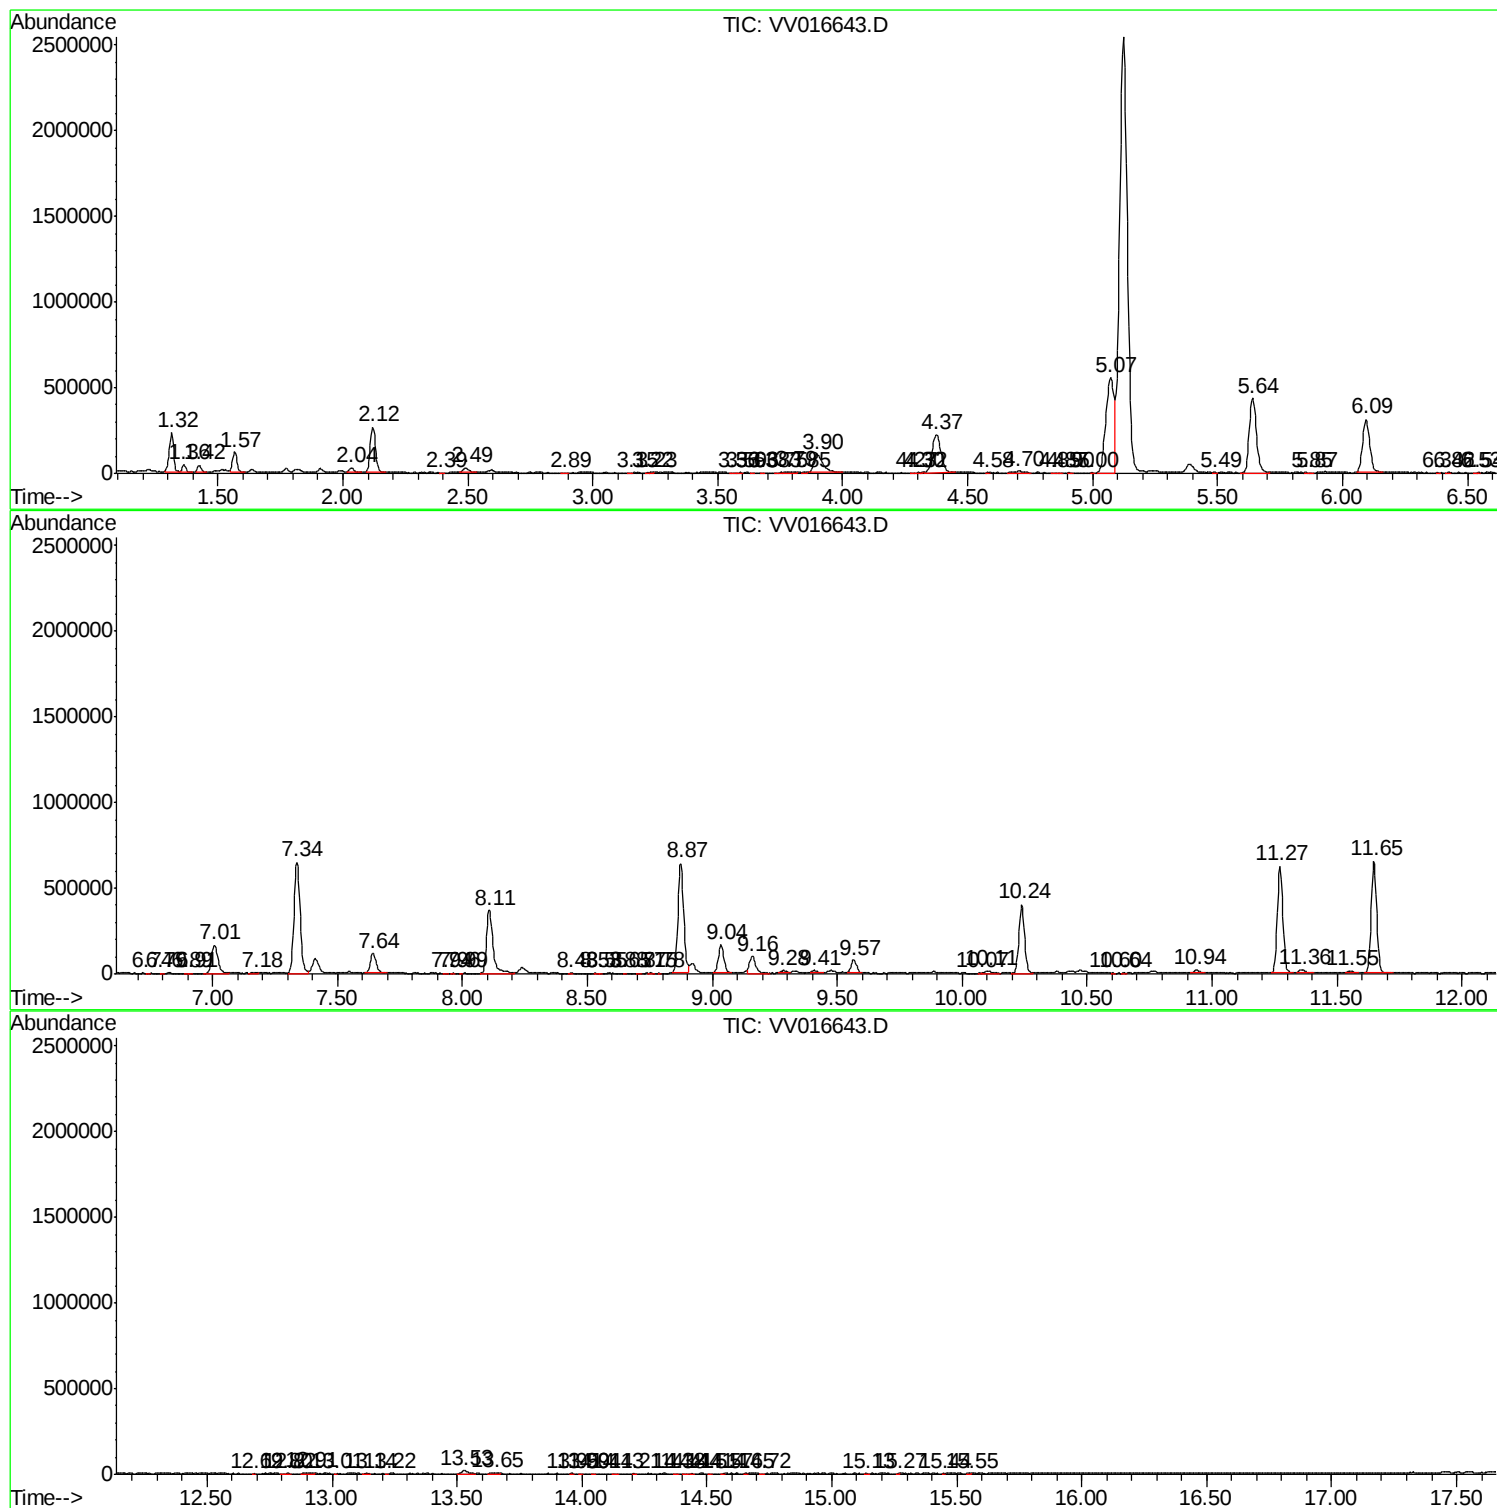

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016643.D
Acq On : 07 Jun 2020 14:28
Operator : SY/MD
Sample : L2861-15DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060620\
Data File : VV016643.D
Acq On : 07 Jun 2020 14:28
Operator : SY/MD
Sample : L2861-15DL 50X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9E48DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc