

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016644.D
 Acq On : 07 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2861-19DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	171000	178664	13.39%	1.615%
2	1.566	143	148	163	rVB	111727	125883	9.43%	1.138%
3	2.119	310	320	336	rVB	274343	409500	30.68%	3.701%
4	2.360	392	395	397	rBV4	1314	648	0.05%	0.006%
5	2.399	404	407	408	rBV3	772	477	0.04%	0.004%
6	2.843	542	545	547	rVB4	1042	534	0.04%	0.005%
7	2.855	547	549	554	rBV5	850	726	0.05%	0.007%
8	2.891	557	560	567	rVB6	1507	1677	0.13%	0.015%
9	2.923	567	570	571	rBV3	970	384	0.03%	0.003%
10	2.965	581	583	584	rBV3	1420	534	0.04%	0.005%
11	3.019	598	600	603	rBV4	1132	830	0.06%	0.008%
12	3.036	603	605	607	rVV2	812	452	0.03%	0.004%
13	3.113	626	629	631	rBV3	1301	785	0.06%	0.007%
14	3.209	653	659	663	rBV10	1387	1136	0.09%	0.010%
15	3.235	663	667	669	rBV3	1698	1141	0.09%	0.010%
16	3.290	681	684	686	rBV4	1272	600	0.04%	0.005%
17	3.357	703	705	706	rBV2	988	362	0.03%	0.003%
18	3.415	721	723	725	rBV3	686	383	0.03%	0.003%
19	3.505	750	751	757	rVB5	938	451	0.03%	0.004%
20	3.592	775	778	782	rBV4	934	812	0.06%	0.007%
21	3.611	782	784	786	rBV3	995	455	0.03%	0.004%
22	3.679	803	805	809	rBV4	724	454	0.03%	0.004%
23	3.698	809	811	814	rVB4	1042	544	0.04%	0.005%
24	3.717	814	817	820	rBV4	1139	803	0.06%	0.007%
25	3.826	848	851	853	rBV2	756	572	0.04%	0.005%
26	3.839	853	855	857	rVV3	1451	702	0.05%	0.006%
27	3.900	863	874	907	rBV2	109735	308825	23.14%	2.791%
28	4.248	978	982	985	rBV6	1280	1171	0.09%	0.011%
29	4.273	988	990	991	rBV2	1052	366	0.03%	0.003%
30	4.373	1006	1021	1042	rBV	229356	563718	42.24%	5.095%
31	4.894	1181	1183	1184	rBV2	1277	508	0.04%	0.005%
32	4.926	1190	1193	1195	rVB3	737	414	0.03%	0.004%
33	4.949	1195	1200	1202	rBV5	1794	1262	0.09%	0.011%
34	5.071	1221	1238	1244	rBV3	568591	1334591	100.00%	12.062%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016644.D
 Acq On : 07 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2861-19DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1433	rBV	435039	856348	64.17%	7.740%
36	5.929	1493	1505	1515	rBV8	10313	23255	1.74%	0.210%
37	6.093	1543	1556	1578	rBV2	325824	653527	48.97%	5.906%
38	6.338	1626	1632	1635	rBV7	1835	2129	0.16%	0.019%
39	6.466	1667	1672	1673	rBV5	1377	974	0.07%	0.009%
40	6.547	1694	1697	1698	rBV3	869	378	0.03%	0.003%
41	6.723	1749	1752	1753	rBV3	1366	631	0.05%	0.006%
42	6.865	1794	1796	1798	rVB3	1231	616	0.05%	0.006%
43	6.881	1798	1801	1804	rBV4	1130	773	0.06%	0.007%
44	6.907	1806	1809	1810	rBV2	857	509	0.04%	0.005%
45	7.006	1829	1840	1859	rBV	167773	299634	22.45%	2.708%
46	7.170	1888	1891	1894	rBV5	2151	1330	0.10%	0.012%
47	7.338	1931	1943	1957	rBV	660187	1137120	85.20%	10.277%
48	7.412	1958	1966	1986	rVB	162177	284524	21.32%	2.571%
49	7.643	2028	2038	2054	rBV	118183	197419	14.79%	1.784%
50	7.781	2080	2081	2082	rBV	1322	386	0.03%	0.003%
51	7.810	2088	2090	2093	rBV3	1322	879	0.07%	0.008%
52	7.929	2125	2127	2130	rVB3	1142	596	0.04%	0.005%
53	7.981	2141	2143	2145	rBV3	865	418	0.03%	0.004%
54	8.032	2153	2159	2170	rBV3	5115	8504	0.64%	0.077%
55	8.106	2172	2182	2216	rBV	386197	700899	52.52%	6.335%
56	8.440	2281	2286	2289	rBV6	1878	1770	0.13%	0.016%
57	8.457	2289	2291	2293	rBV4	805	498	0.04%	0.005%
58	8.521	2309	2311	2313	rVB3	1504	582	0.04%	0.005%
59	8.537	2313	2316	2319	rVB3	1011	476	0.04%	0.004%
60	8.553	2319	2321	2322	rBV2	1207	455	0.03%	0.004%
61	8.595	2333	2334	2338	rVB4	1554	800	0.06%	0.007%
62	8.617	2338	2341	2342	rBV3	1415	758	0.06%	0.007%
63	8.643	2347	2349	2351	rBV3	1036	590	0.04%	0.005%
64	8.714	2369	2371	2375	rVV4	1435	975	0.07%	0.009%
65	8.775	2387	2390	2393	rBV5	1879	1455	0.11%	0.013%
66	8.874	2411	2421	2432	rBV	629545	997320	74.73%	9.014%
67	9.035	2462	2471	2487	rBV	91791	154841	11.60%	1.399%
68	9.283	2539	2548	2556	rBV	8225	16425	1.23%	0.148%
69	9.405	2577	2586	2598	rBV3	23963	41056	3.08%	0.371%
70	9.566	2628	2636	2647	rBV2	43467	66887	5.01%	0.605%
71	10.238	2834	2845	2857	rBV	419759	656574	49.20%	5.934%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016644.D
 Acq On : 07 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2861-19DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.646	2971	2972	2974	rBV2	1418	589	0.04%	0.005%
73	11.270	3156	3166	3184	rVB	625432	961078	72.01%	8.686%
74	11.646	3273	3283	3297	rVB	666725	1028761	77.08%	9.298%
75	12.071	3413	3415	3416	rBV2	1082	403	0.03%	0.004%
76	12.640	3590	3592	3594	rBV4	1135	488	0.04%	0.004%
77	12.733	3618	3621	3625	rBV6	2009	1738	0.13%	0.016%
78	12.781	3634	3636	3638	rBV3	1778	680	0.05%	0.006%
79	12.958	3689	3691	3694	rVB3	1496	766	0.06%	0.007%
80	12.980	3694	3698	3699	rBV3	2261	1421	0.11%	0.013%
81	13.058	3717	3722	3723	rBV4	1871	1636	0.12%	0.015%
82	13.315	3800	3802	3804	rBV3	1595	817	0.06%	0.007%
83	13.569	3879	3881	3885	rVB3	1540	971	0.07%	0.009%
84	13.871	3971	3975	3977	rBV3	815	560	0.04%	0.005%
85	13.974	4005	4007	4008	rBV2	1140	579	0.04%	0.005%
86	14.038	4025	4027	4029	rBV2	796	403	0.03%	0.004%
87	14.135	4054	4057	4059	rBV3	1239	626	0.05%	0.006%
88	14.170	4066	4068	4072	rVB4	1377	983	0.07%	0.009%
89	14.193	4072	4075	4076	rBV2	1222	665	0.05%	0.006%
90	14.331	4115	4118	4123	rVB5	1362	1022	0.08%	0.009%
91	14.382	4130	4134	4137	rVB5	1146	945	0.07%	0.009%
92	14.440	4148	4152	4154	rBV4	1791	1617	0.12%	0.015%
93	14.505	4169	4172	4173	rBV3	987	402	0.03%	0.004%
94	14.595	4198	4200	4205	rVB5	1374	1158	0.09%	0.010%
95	14.617	4205	4207	4209	rBV2	889	397	0.03%	0.004%
96	14.646	4214	4216	4220	rVB5	2237	987	0.07%	0.009%
97	14.710	4234	4236	4239	rBV2	921	568	0.04%	0.005%
98	14.749	4244	4248	4249	rBV2	1008	606	0.05%	0.005%
99	14.881	4287	4289	4291	rVB3	998	354	0.03%	0.003%
100	15.328	4426	4428	4429	rBV2	1413	649	0.05%	0.006%


Sum of corrected areas: 11064544

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016644.D
Acq On : 07 Jun 2020 14:52
Operator : SY/MD
Sample : L2861-19DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

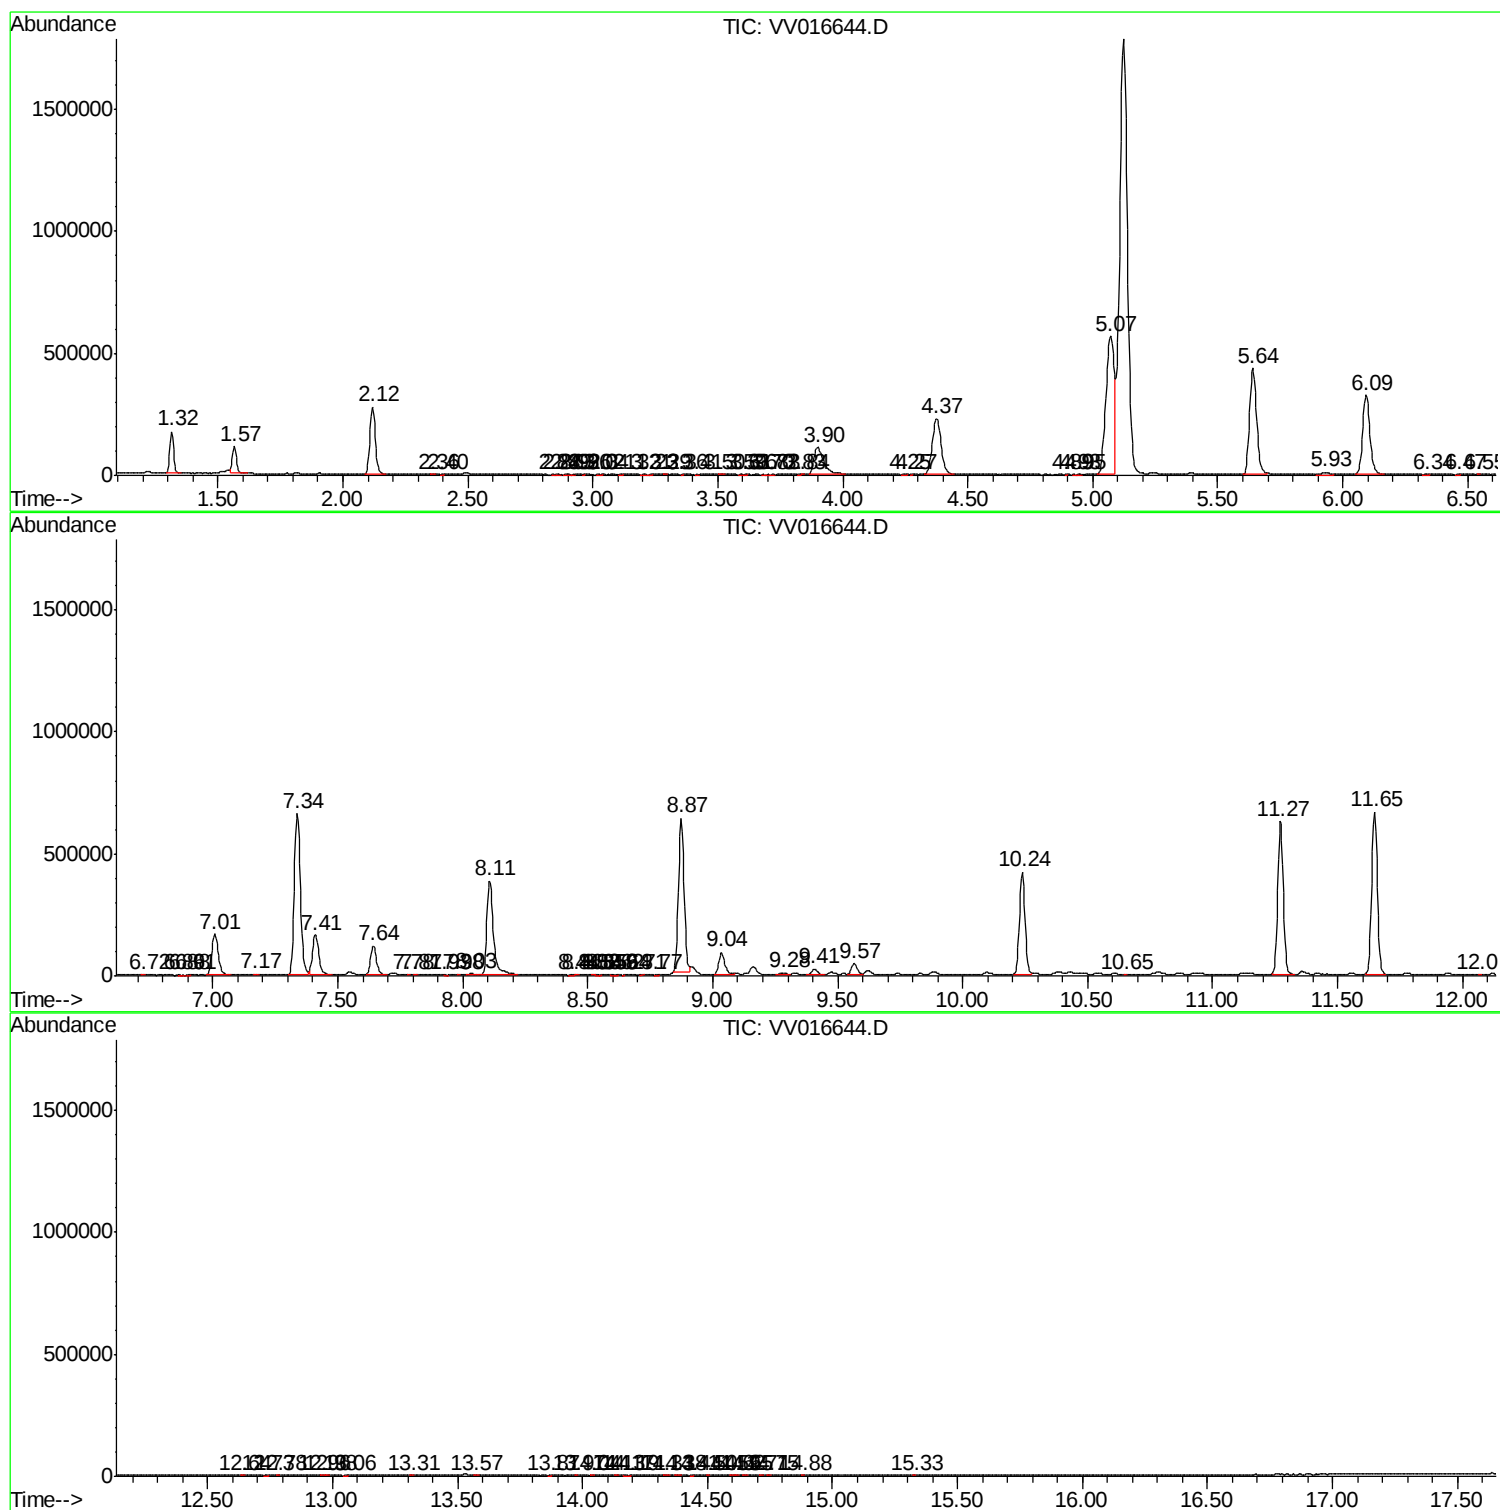

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016644.D
Acq On : 07 Jun 2020 14:52
Operator : SY/MD
Sample : L2861-19DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016644.D
Acq On : 07 Jun 2020 14:52
Operator : SY/MD
Sample : L2861-19DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc