


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060620\
 Data File : VV016577.D
 Acq On : 06 Jun 2020 09:19
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis
 Last Update : Mon Jun 08 05:42:16 2020

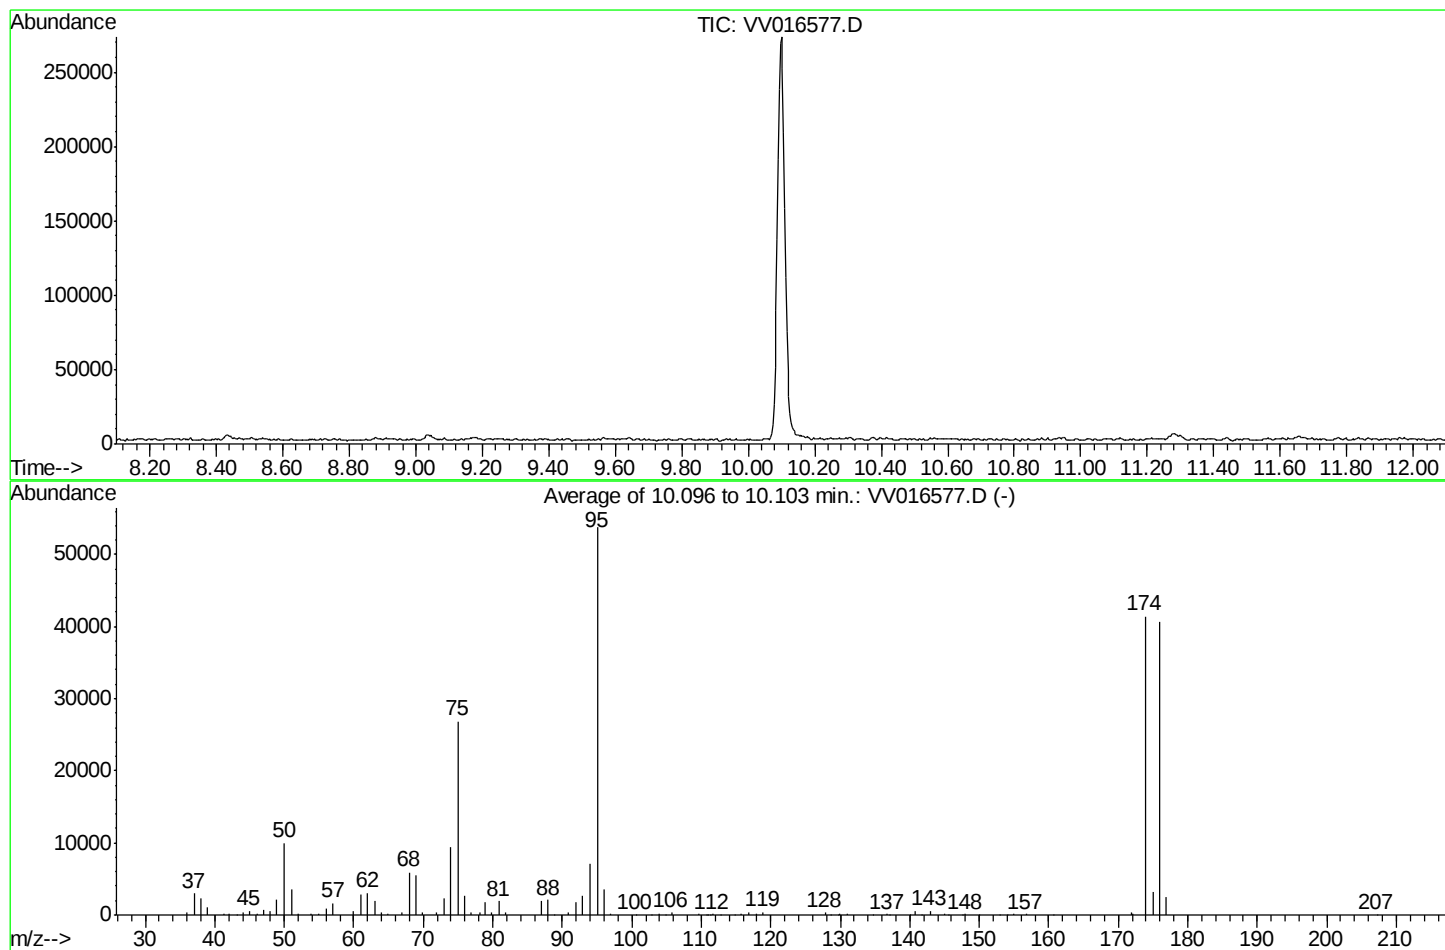

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	9991	PASS
75	95	30	80	50.0	26885	PASS
95	95	100	100	100.0	53752	PASS
96	95	5	9	6.6	3568	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.9	41354	PASS
175	174	5	9	7.8	3213	PASS
176	174	95	101	98.4	40680	PASS
177	176	5	9	6.3	2560	PASS

m/z	Abundance
35.00	135.0
35.90	574.0
37.00	3315.0
38.00	2416.0
39.00	1167.0
39.90	382.0
40.80	147.0
41.40	102.0
41.90	112.0
43.00	129.0
44.00	753.0
45.00	615.0
46.00	106.0
46.90	848.0
47.90	547.0
49.00	2446.0
50.00	10704.0
51.00	3714.0
52.00	162.0
52.90	120.0
53.90	127.0
55.00	204.0
56.00	1002.0
57.00	1541.0
57.90	111.0
60.00	524.0
61.00	3144.0
62.00	3343.0
63.00	1867.0
64.10	303.0
65.00	235.0
66.90	266.0
68.00	6237.0
68.90	5794.0
69.90	441.0
72.00	360.0
73.00	2579.0
74.00	9710.0
75.00	27456.0
76.00	2716.0
77.10	280.0
78.10	268.0
78.90	1760.0
79.80	589.0
80.90	2056.0
81.80	363.0
87.00	2043.0
88.00	2138.0
90.90	292.0
91.90	1682.0
93.00	2726.0
94.00	7005.0
95.00	54184.0
96.00	3810.0
96.90	191.0
100.60	115.0
102.80	114.0
103.90	304.0
104.90	131.0
105.70	314.0
109.70	112.0
110.80	114.0
111.70	118.0
114.80	103.0
115.80	236.0
116.80	381.0
117.90	169.0
118.90	425.0
127.80	367.0
128.60	102.0
129.80	177.0
131.10	149.0
134.60	110.0
136.70	174.0
140.80	571.0
141.70	106.0
142.90	599.0
145.00	133.0
148.00	146.0
149.90	115.0
153.00	110.0
154.10	124.0
156.70	109.0
160.70	130.0
171.80	425.0
173.90	41768.0
175.00	3235.0
175.90	39904.0
176.90	2710.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.10	107.0
35.90	620.0
37.00	3256.0
38.00	2284.0
39.00	1228.0
39.90	384.0
41.30	115.0
42.10	125.0
43.10	144.0
44.00	947.0
45.00	588.0
46.10	126.0
47.00	776.0
47.90	526.0
49.00	2325.0
50.00	10480.0
51.00	3665.0
52.00	162.0
52.90	108.0
53.90	127.0
55.00	220.0
56.00	989.0
57.00	1672.0
57.90	110.0
60.00	569.0
61.00	3015.0
62.00	3274.0
63.00	1910.0
64.00	296.0
64.90	268.0
66.90	300.0
68.00	6111.0
69.00	5638.0
69.90	439.0
71.90	463.0
73.00	2463.0
74.00	9737.0
75.00	27752.0
76.00	2787.0
76.90	320.0
78.10	299.0
78.90	1748.0
79.80	550.0
80.90	1964.0
81.80	362.0
87.00	2000.0
88.00	2136.0
90.80	301.0
92.00	1758.0
93.00	2701.0
94.00	7484.0
95.00	55512.0
96.00	3686.0
97.00	172.0
103.90	274.0
105.70	329.0
109.70	124.0
111.00	100.0
111.60	136.0
115.80	235.0
116.80	357.0
117.90	176.0
118.90	445.0
127.80	315.0
130.00	215.0
131.00	153.0
136.80	153.0
140.90	547.0
142.90	571.0
145.00	163.0
148.00	176.0
149.90	129.0
154.10	105.0
155.00	125.0
156.70	119.0
160.70	118.0
171.80	377.0
173.90	42872.0
175.00	3367.0
175.90	42160.0
176.90	2670.0
207.20	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	594.0
37.00	2669.0
38.00	2145.0
39.00	1085.0
39.90	439.0
41.30	119.0
42.10	170.0
43.20	159.0
44.00	1020.0
45.00	529.0
46.20	138.0
47.00	634.0
47.90	429.0
49.00	2011.0
50.00	9470.0
51.00	3241.0
51.90	158.0
52.80	107.0
53.90	109.0
55.00	188.0
56.00	917.0
57.00	1676.0
57.90	104.0
60.00	573.0
61.00	2588.0
62.00	2795.0
63.00	1925.0
64.00	235.0
64.90	244.0
66.90	274.0
68.00	5275.0
69.00	5182.0
69.90	441.0
71.90	480.0
73.00	2057.0
74.00	8658.0
75.00	25448.0
76.00	2448.0
76.90	379.0
78.10	258.0
78.90	1639.0
79.80	435.0
80.90	1691.0
81.80	337.0
87.00	1841.0
88.00	1921.0
88.80	117.0
90.80	270.0
92.00	1675.0
92.90	2358.0
94.00	6980.0
95.00	51560.0
96.00	3209.0
97.00	160.0
103.90	197.0
105.80	274.0
109.70	116.0
111.30	120.0
111.70	125.0
112.80	109.0
115.80	241.0
116.80	349.0
117.80	190.0
118.90	395.0
127.80	239.0
129.90	226.0
130.90	170.0
137.00	132.0
140.00	107.0
140.90	510.0
142.90	591.0
145.10	152.0
145.60	105.0
147.60	132.0
148.00	152.0
155.00	178.0
156.70	122.0
171.80	301.0
172.00	292.0
173.90	39424.0
175.00	3037.0
175.90	39976.0
176.90	2302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.10	143.0
35.80	159.0
37.00	131.0
37.40	157.0
38.80	104.0
39.90	488.0
40.90	108.0
42.00	106.0
43.10	108.0
44.00	589.0
48.90	120.0
50.00	113.0
50.20	114.0
52.70	119.0
53.10	116.0
55.30	104.0
58.00	119.0
58.50	114.0
60.50	119.0
61.90	109.0
66.20	102.0
72.90	110.0
79.80	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82