

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025993.D
 Acq On : 06 Jun 2022 10:33
 Operator : SY/MD
 Sample : VV0606WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M

Title : VOC Analysis

Signal : TIC: VV025993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	102	rVB	226930	238689	15.94%	2.216%
2	1.571	158	165	178	rVB	212513	234329	15.65%	2.176%
3	2.111	323	333	347	rVB	420600	602489	40.23%	5.594%
4	2.449	436	438	441	rBV3	350	231	0.02%	0.002%
5	2.481	446	448	451	rBV2	301	218	0.01%	0.002%
6	2.510	451	457	458	rBV4	1845	1784	0.12%	0.017%
7	2.558	470	472	474	rBV	241	128	0.01%	0.001%
8	2.574	474	477	482	rVB3	405	412	0.03%	0.004%
9	2.748	525	531	532	rBV2	426	368	0.02%	0.003%
10	2.828	554	556	560	rVB2	303	226	0.02%	0.002%
11	2.850	560	563	566	rBV2	231	127	0.01%	0.001%
12	2.867	566	568	571	rBV2	209	156	0.01%	0.001%
13	3.021	613	616	620	rVB2	342	323	0.02%	0.003%
14	3.047	620	624	626	rBV2	264	189	0.01%	0.002%
15	3.178	661	665	667	rVB3	227	154	0.01%	0.001%
16	3.191	667	669	672	rVB3	304	168	0.01%	0.002%
17	3.217	672	677	678	rBV	255	181	0.01%	0.002%
18	3.301	697	703	704	rBV	279	256	0.02%	0.002%
19	3.355	717	720	723	rVB	343	205	0.01%	0.002%
20	3.378	723	727	731	rBV2	137	126	0.01%	0.001%
21	3.558	775	783	787	rBV3	342	442	0.03%	0.004%
22	3.600	791	796	797	rBV2	413	254	0.02%	0.002%
23	3.693	821	825	830	rBV2	332	413	0.03%	0.004%
24	3.728	835	836	842	rVB	386	158	0.01%	0.001%
25	3.805	856	860	864	rBV	160	155	0.01%	0.001%
26	3.850	869	874	880	rVB2	298	369	0.02%	0.003%
27	3.899	880	889	917	rBV	58792	209880	14.01%	1.949%
28	4.349	1014	1029	1056	rBV	252773	618360	41.29%	5.742%
29	4.661	1123	1126	1128	rVB2	523	275	0.02%	0.003%
30	4.677	1128	1131	1133	rBV2	348	228	0.02%	0.002%
31	4.754	1152	1155	1158	rBV2	234	217	0.01%	0.002%
32	4.815	1167	1174	1175	rBV2	405	416	0.03%	0.004%
33	4.860	1183	1188	1190	rBV2	352	234	0.02%	0.002%
34	4.876	1190	1193	1197	rBV3	238	218	0.01%	0.002%
35	4.969	1218	1222	1223	rBV2	318	201	0.01%	0.002%
36	5.046	1229	1246	1281	rBV2	584146	1497613	100.00%	13.906%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025993.D
 Acq On : 06 Jun 2022 10:33
 Operator : SY/MD
 Sample : VV0606WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.365	1343	1345	1347	rBV2	280	158	0.01%	0.001%
38	5.500	1383	1387	1392	rBV3	450	421	0.03%	0.004%
39	5.535	1396	1398	1403	rVB2	396	213	0.01%	0.002%
40	5.567	1403	1408	1409	rBV3	452	336	0.02%	0.003%
41	5.616	1412	1423	1453	rBV	356985	734245	49.03%	6.818%
42	5.905	1503	1513	1530	rBV3	21836	46473	3.10%	0.432%
43	6.011	1542	1546	1548	rBV3	537	402	0.03%	0.004%
44	6.069	1551	1564	1595	rBV	341608	704242	47.02%	6.539%
45	6.333	1644	1646	1650	rVB	436	232	0.02%	0.002%
46	6.407	1667	1669	1674	rBV2	341	244	0.02%	0.002%
47	6.458	1684	1685	1687	rBV2	249	129	0.01%	0.001%
48	6.468	1687	1688	1690	rVV	475	145	0.01%	0.001%
49	6.497	1694	1697	1698	rBV	341	177	0.01%	0.002%
50	6.590	1723	1726	1727	rBV	228	141	0.01%	0.001%
51	6.616	1731	1734	1736	rBV2	291	212	0.01%	0.002%
52	6.651	1744	1745	1749	rVB	255	169	0.01%	0.002%
53	6.680	1749	1754	1758	rBV3	472	403	0.03%	0.004%
54	6.789	1786	1788	1790	rVV	329	186	0.01%	0.002%
55	6.815	1794	1796	1799	rVV2	316	179	0.01%	0.002%
56	6.844	1801	1805	1808	rVV2	241	229	0.02%	0.002%
57	6.876	1812	1815	1821	rVV	347	331	0.02%	0.003%
58	6.908	1821	1825	1828	rVV2	470	347	0.02%	0.003%
59	6.924	1828	1830	1833	rVB2	332	218	0.01%	0.002%
60	6.985	1838	1849	1885	rBV	159561	304464	20.33%	2.827%
61	7.265	1934	1936	1939	rBV3	375	289	0.02%	0.003%
62	7.316	1939	1952	1977	rBV	670902	1173222	78.34%	10.894%
63	7.622	2036	2047	2068	rBV	110362	202525	13.52%	1.881%
64	7.870	2122	2124	2127	rVV4	276	167	0.01%	0.002%
65	7.985	2156	2160	2162	rBV3	651	518	0.03%	0.005%
66	8.091	2183	2193	2233	rBV	297006	672214	44.89%	6.242%
67	8.416	2290	2294	2301	rBV5	1016	884	0.06%	0.008%
68	8.567	2339	2341	2343	rBV	284	150	0.01%	0.001%
69	8.683	2373	2377	2379	rBV	363	292	0.02%	0.003%
70	8.706	2381	2384	2388	rVB2	460	376	0.03%	0.003%
71	8.799	2411	2413	2415	rBV2	256	133	0.01%	0.001%
72	8.850	2418	2429	2449	rBV	574719	935399	62.46%	8.685%
73	9.146	2519	2521	2524	rBV2	355	247	0.02%	0.002%
74	9.233	2544	2548	2552	rBV3	449	451	0.03%	0.004%
75	9.271	2556	2560	2562	rBV	215	182	0.01%	0.002%
76	9.329	2576	2578	2582	rVB	367	206	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025993.D
 Acq On : 06 Jun 2022 10:33
 Operator : SY/MD
 Sample : VV0606WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.361	2585	2588	2594	rVB	420	392	0.03%	0.004%
78	9.567	2649	2652	2653	rBV	379	190	0.01%	0.002%
79	9.651	2676	2678	2681	rVB2	457	171	0.01%	0.002%
80	9.680	2685	2687	2690	rVB	412	215	0.01%	0.002%
81	9.705	2690	2695	2696	rBV2	247	185	0.01%	0.002%
82	9.866	2743	2745	2748	rVB2	318	177	0.01%	0.002%
83	9.931	2762	2765	2766	rBV2	727	433	0.03%	0.004%
84	10.053	2799	2803	2807	rBV2	289	338	0.02%	0.003%
85	10.120	2821	2824	2827	rBV	265	198	0.01%	0.002%
86	10.213	2841	2853	2880	rBV	447022	704373	47.03%	6.540%
87	10.413	2913	2915	2922	rVB2	610	417	0.03%	0.004%
88	10.467	2929	2932	2933	rBV2	311	143	0.01%	0.001%
89	10.693	2999	3002	3007	rVB2	522	342	0.02%	0.003%
90	10.812	3038	3039	3041	rBV	281	144	0.01%	0.001%
91	10.857	3050	3053	3056	rBV2	248	205	0.01%	0.002%
92	10.927	3067	3075	3081	rBV3	724	1096	0.07%	0.010%
93	10.982	3089	3092	3094	rBV2	181	134	0.01%	0.001%
94	11.156	3143	3146	3150	rBV2	564	540	0.04%	0.005%
95	11.246	3163	3174	3199	rBV	526586	836367	55.85%	7.766%
96	11.622	3274	3291	3311	rBV	657433	1027113	68.58%	9.537%
97	12.046	3420	3423	3424	rBV2	376	209	0.01%	0.002%
98	12.082	3430	3434	3436	rBV	421	334	0.02%	0.003%
99	12.246	3480	3485	3486	rBV3	756	671	0.04%	0.006%
100	13.265	3798	3802	3814	rVB6	2244	3549	0.24%	0.033%


Sum of corrected areas: 10769679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025993.D
Acq On : 06 Jun 2022 10:33
Operator : SY/MD
Sample : VV0606WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

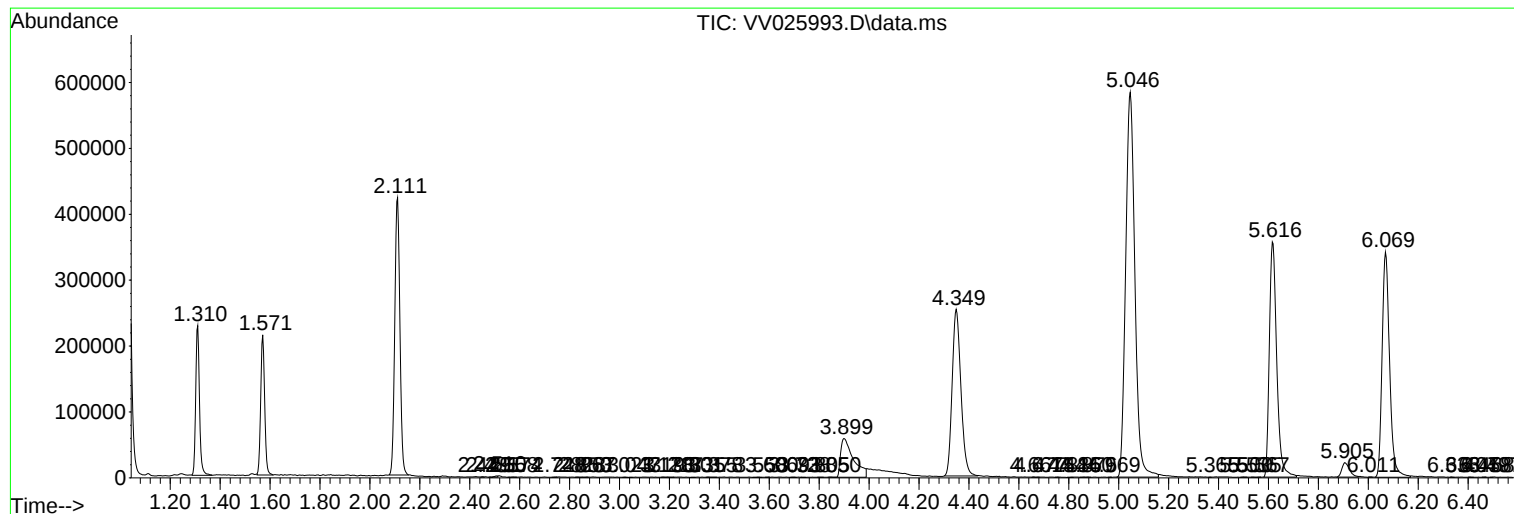

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025993.D
Acq On : 06 Jun 2022 10:33
Operator : SY/MD
Sample : VV0606WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025993.D
Acq On : 06 Jun 2022 10:33
Operator : SY/MD
Sample : VV0606WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------