

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025994.D
 Acq On : 06 Jun 2022 11:45
 Operator : SY/MD
 Sample : VV0606MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	98	rVB	216817	222611	15.45%	2.156%
2	1.571	158	165	179	rVB	193290	218039	15.13%	2.111%
3	2.108	323	332	357	rVB	392067	568220	39.44%	5.502%
4	2.622	488	492	495	rBV2	306	246	0.02%	0.002%
5	2.757	530	534	535	rBV	345	222	0.02%	0.002%
6	2.851	560	563	565	rBV3	233	126	0.01%	0.001%
7	2.918	581	584	588	rBV2	259	252	0.02%	0.002%
8	3.040	620	622	625	rBV2	285	145	0.01%	0.001%
9	3.227	677	680	684	rVB2	619	432	0.03%	0.004%
10	3.252	684	688	690	rBV2	309	229	0.02%	0.002%
11	3.362	720	722	724	rVB2	220	90	0.01%	0.001%
12	3.375	724	726	729	rBV2	302	182	0.01%	0.002%
13	3.404	734	735	739	rVB	251	146	0.01%	0.001%
14	3.510	763	768	773	rBV	287	311	0.02%	0.003%
15	3.571	781	787	790	rBV3	308	312	0.02%	0.003%
16	3.625	799	804	807	rBV2	348	308	0.02%	0.003%
17	3.722	831	834	836	rBV2	388	241	0.02%	0.002%
18	3.738	836	839	842	rVB	512	323	0.02%	0.003%
19	3.761	842	846	850	rBV2	369	368	0.03%	0.004%
20	3.809	859	861	863	rVB	281	98	0.01%	0.001%
21	3.834	867	869	873	rBV3	181	126	0.01%	0.001%
22	3.892	877	887	918	rBV	58676	206666	14.34%	2.001%
23	4.346	1014	1028	1056	rVB	241525	593367	41.19%	5.746%
24	4.596	1102	1106	1108	rBV3	806	551	0.04%	0.005%
25	4.667	1126	1128	1135	rVB3	430	267	0.02%	0.003%
26	4.722	1142	1145	1149	rBV3	566	329	0.02%	0.003%
27	4.744	1149	1152	1156	rBV2	388	326	0.02%	0.003%
28	4.786	1161	1165	1167	rBV2	209	180	0.01%	0.002%
29	4.822	1173	1176	1178	rBV2	399	268	0.02%	0.003%
30	4.860	1185	1188	1189	rBV2	309	147	0.01%	0.001%
31	4.870	1189	1191	1193	rVB	291	111	0.01%	0.001%
32	4.934	1207	1211	1212	rBV2	185	131	0.01%	0.001%
33	5.043	1228	1245	1291	rBV2	550906	1440728	100.00%	13.951%
34	5.432	1363	1366	1370	rBV3	547	464	0.03%	0.004%
35	5.516	1390	1392	1395	rVB2	490	234	0.02%	0.002%
36	5.532	1395	1397	1399	rVB	216	87	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025994.D
 Acq On : 06 Jun 2022 11:45
 Operator : SY/MD
 Sample : VV0606MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.558	1400	1405	1407	rBV3	271	264	0.02%	0.003%
38	5.613	1410	1422	1464	rBV	342268	700300	48.61%	6.781%
39	5.905	1502	1513	1530	rBV2	20063	43904	3.05%	0.425%
40	6.066	1550	1563	1588	rBV	327829	672337	46.67%	6.510%
41	6.307	1635	1638	1639	rBV2	488	253	0.02%	0.002%
42	6.368	1654	1657	1661	rBV4	290	227	0.02%	0.002%
43	6.410	1668	1670	1673	rVB2	213	116	0.01%	0.001%
44	6.426	1673	1675	1678	rBV	449	237	0.02%	0.002%
45	6.452	1681	1683	1684	rBV	337	135	0.01%	0.001%
46	6.465	1684	1687	1689	rVB2	432	233	0.02%	0.002%
47	6.481	1689	1692	1696	rBV3	452	328	0.02%	0.003%
48	6.529	1704	1707	1709	rBV	281	165	0.01%	0.002%
49	6.539	1709	1710	1713	rVB2	308	138	0.01%	0.001%
50	6.645	1740	1743	1744	rBV	473	254	0.02%	0.002%
51	6.680	1747	1754	1757	rVV2	382	279	0.02%	0.003%
52	6.703	1757	1761	1764	rBV2	237	161	0.01%	0.002%
53	6.744	1771	1774	1776	rBV	267	190	0.01%	0.002%
54	6.821	1796	1798	1802	rVB	302	135	0.01%	0.001%
55	6.876	1810	1815	1816	rBV	281	177	0.01%	0.002%
56	6.921	1827	1829	1831	rBV	239	91	0.01%	0.001%
57	6.982	1837	1848	1882	rBV	155376	299725	20.80%	2.902%
58	7.313	1939	1951	1978	rBV	634653	1108231	76.92%	10.731%
59	7.619	2036	2046	2068	rBV2	111430	199798	13.87%	1.935%
60	7.850	2116	2118	2121	rVB3	417	201	0.01%	0.002%
61	7.883	2126	2128	2130	rBV2	366	162	0.01%	0.002%
62	7.911	2134	2137	2139	rBV2	378	201	0.01%	0.002%
63	7.931	2139	2143	2146	rBV3	442	389	0.03%	0.004%
64	7.966	2152	2154	2156	rVB2	246	86	0.01%	0.001%
65	7.982	2156	2159	2160	rBV	251	116	0.01%	0.001%
66	8.021	2168	2171	2173	rBV2	247	204	0.01%	0.002%
67	8.088	2182	2192	2225	rBV	280123	638108	44.29%	6.179%
68	8.519	2323	2326	2328	rBV2	421	246	0.02%	0.002%
69	8.686	2376	2378	2381	rVB2	389	201	0.01%	0.002%
70	8.709	2382	2385	2388	rBV3	438	288	0.02%	0.003%
71	8.764	2400	2402	2404	rVB	291	106	0.01%	0.001%
72	8.780	2404	2407	2410	rBV2	286	252	0.02%	0.002%
73	8.799	2410	2413	2417	rVB2	409	245	0.02%	0.002%
74	8.850	2417	2429	2454	rBV	542647	892405	61.94%	8.641%
75	9.018	2478	2481	2489	rVB3	2234	2571	0.18%	0.025%
76	9.088	2501	2503	2504	rBV	334	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025994.D
 Acq On : 06 Jun 2022 11:45
 Operator : SY/MD
 Sample : VV0606MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.317	2572	2574	2577	rBV	466	221	0.02%	0.002%
78	9.387	2594	2596	2601	rVB2	414	263	0.02%	0.003%
79	9.410	2601	2603	2607	rVB2	229	89	0.01%	0.001%
80	9.461	2617	2619	2622	rVB	365	154	0.01%	0.001%
81	9.548	2638	2646	2656	rBV5	3060	4890	0.34%	0.047%
82	9.657	2679	2680	2683	rBV	266	126	0.01%	0.001%
83	9.712	2695	2697	2699	rBV2	409	170	0.01%	0.002%
84	9.757	2708	2711	2715	rVB	517	337	0.02%	0.003%
85	9.792	2719	2722	2724	rBV2	293	152	0.01%	0.001%
86	9.850	2737	2740	2743	rBV	328	245	0.02%	0.002%
87	9.921	2760	2762	2764	rBV	242	103	0.01%	0.001%
88	9.934	2764	2766	2770	rBV	260	182	0.01%	0.002%
89	10.085	2809	2813	2817	rBV2	551	506	0.04%	0.005%
90	10.214	2840	2853	2873	rBV	435085	682104	47.34%	6.605%
91	10.352	2894	2896	2899	rVB2	444	210	0.01%	0.002%
92	10.426	2911	2919	2927	rBV2	2735	3754	0.26%	0.036%
93	10.718	3006	3010	3013	rBV2	379	330	0.02%	0.003%
94	10.776	3026	3028	3030	rBV	355	224	0.02%	0.002%
95	10.844	3047	3049	3052	rBV2	248	160	0.01%	0.002%
96	10.915	3067	3071	3077	rBV2	656	564	0.04%	0.005%
97	10.989	3090	3094	3095	rBV2	359	260	0.02%	0.003%
98	11.246	3163	3174	3197	rBV	533090	813975	56.50%	7.882%
99	11.622	3279	3291	3313	rBV	638516	997092	69.21%	9.655%
100	13.403	3842	3845	3848	rBV2	434	343	0.02%	0.003%




Sum of corrected areas: 10326980

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025994.D
Acq On : 06 Jun 2022 11:45
Operator : SY/MD
Sample : VV0606MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

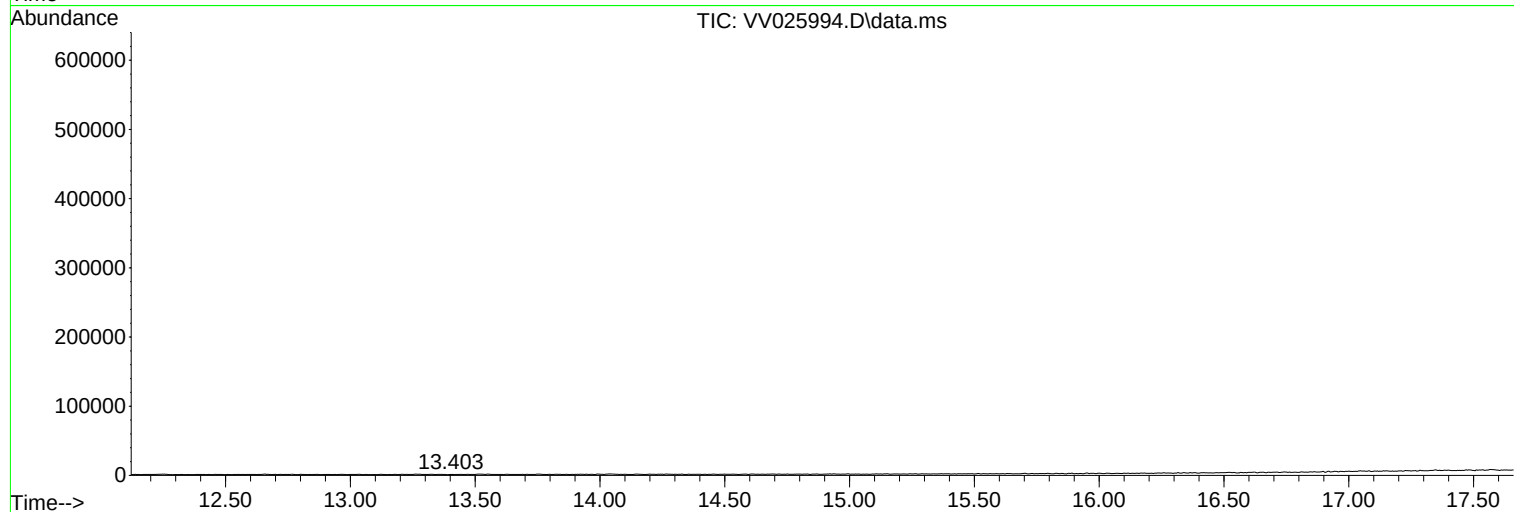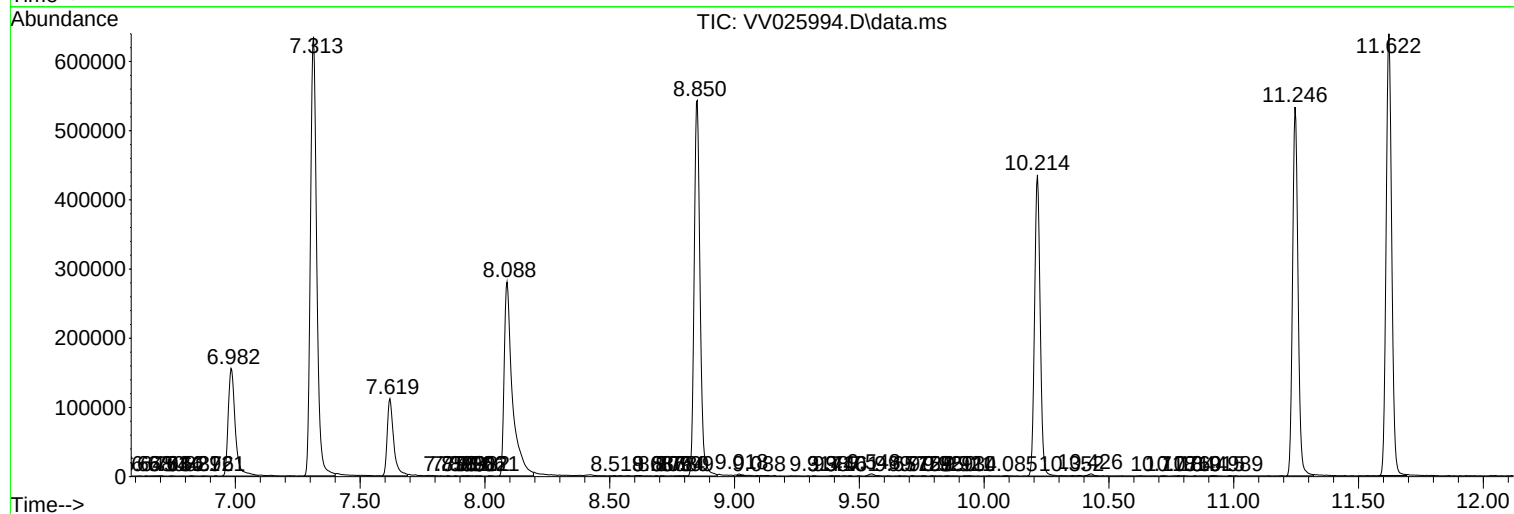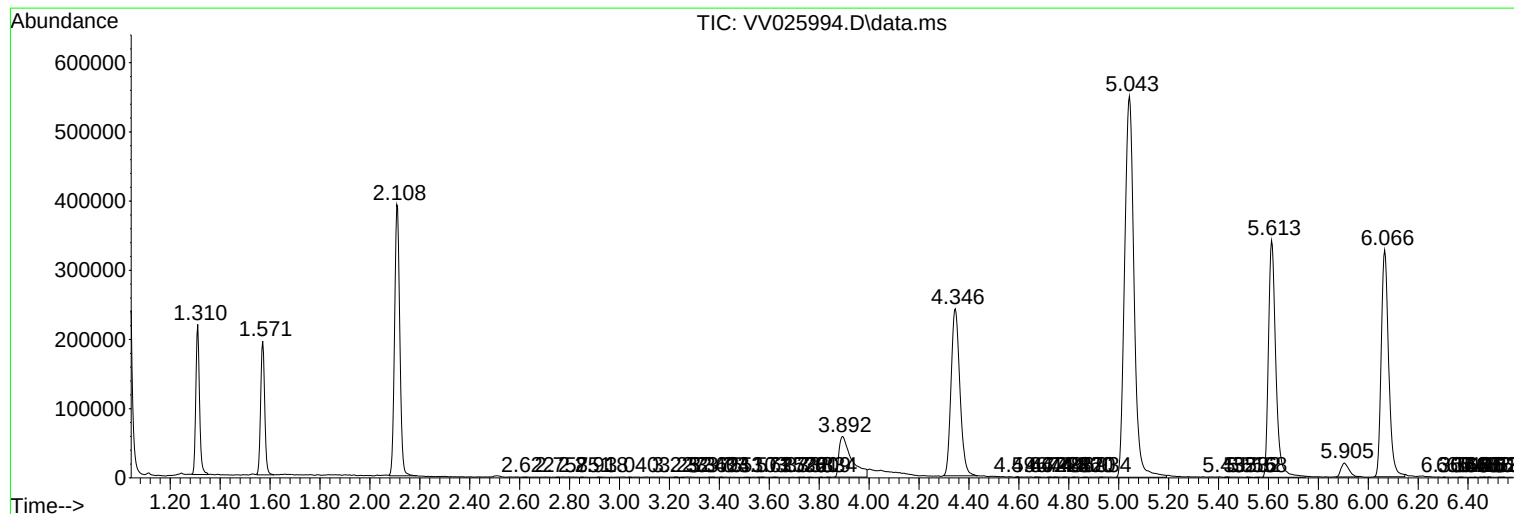

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025994.D
Acq On : 06 Jun 2022 11:45
Operator : SY/MD
Sample : VV0606MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025994.D
Acq On : 06 Jun 2022 11:45
Operator : SY/MD
Sample : VV0606MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc