

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025999.D
 Acq On : 06 Jun 2022 14:02
 Operator : SY/MD
 Sample : N3171-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M

Title : VOC Analysis

Signal : TIC: VV025999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rBV	244808	253023	15.59%	2.116%
2	1.571	157	165	179	rVB	219817	247994	15.28%	2.074%
3	2.108	323	332	354	rVB	456554	652071	40.18%	5.452%
4	2.365	408	412	415	rBV3	784	709	0.04%	0.006%
5	2.960	595	597	599	rBV2	370	215	0.01%	0.002%
6	3.008	609	612	617	rVB3	447	381	0.02%	0.003%
7	3.147	652	655	658	rBV	403	333	0.02%	0.003%
8	3.172	661	663	667	rBV2	478	375	0.02%	0.003%
9	3.224	677	679	681	rBV2	284	132	0.01%	0.001%
10	3.372	722	725	728	rVB2	356	224	0.01%	0.002%
11	3.391	728	731	732	rBV	197	120	0.01%	0.001%
12	3.446	746	748	750	rBV	138	49	0.00%	0.000%
13	3.529	772	774	776	rBV2	236	112	0.01%	0.001%
14	3.667	813	817	821	rBV2	245	202	0.01%	0.002%
15	3.716	827	832	833	rBV	181	154	0.01%	0.001%
16	3.738	836	839	841	rBV3	284	152	0.01%	0.001%
17	3.751	841	843	847	rBV2	292	148	0.01%	0.001%
18	3.851	871	874	877	rBV2	224	152	0.01%	0.001%
19	3.867	877	879	880	rBV	236	93	0.01%	0.001%
20	3.902	880	890	917	rBV2	60891	222880	13.73%	1.864%
21	4.346	1015	1028	1061	rVB	267535	664006	40.92%	5.552%
22	4.761	1155	1157	1160	rVB2	466	256	0.02%	0.002%
23	4.777	1160	1162	1164	rBV	386	229	0.01%	0.002%
24	4.818	1172	1175	1179	rBV2	829	832	0.05%	0.007%
25	4.863	1187	1189	1192	rBV2	237	107	0.01%	0.001%
26	4.966	1218	1221	1226	rBV2	447	381	0.02%	0.003%
27	5.044	1229	1245	1270	rBV2	641540	1622886	100.00%	13.570%
28	5.343	1336	1338	1340	rBV2	419	218	0.01%	0.002%
29	5.445	1368	1370	1373	rBV2	251	196	0.01%	0.002%
30	5.474	1377	1379	1382	rBV	348	209	0.01%	0.002%
31	5.507	1385	1389	1392	rVB2	372	335	0.02%	0.003%
32	5.616	1408	1423	1457	rBV	390916	802853	49.47%	6.713%
33	5.905	1502	1513	1530	rBV2	20919	46594	2.87%	0.390%
34	6.069	1550	1564	1602	rBV	368424	767582	47.30%	6.418%
35	6.288	1630	1632	1637	rVB2	541	339	0.02%	0.003%
36	6.375	1656	1659	1661	rBV	354	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025999.D
 Acq On : 06 Jun 2022 14:02
 Operator : SY/MD
 Sample : N3171-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	6.465	1684	1687	1691	rBV2	324	336	0.02%	0.003%
38	6.587	1719	1725	1727	rBV4	429	382	0.02%	0.003%
39	6.613	1730	1733	1735	rBV	139	86	0.01%	0.001%
40	6.625	1735	1737	1738	rBV	130	54	0.00%	0.000%
41	6.645	1741	1743	1744	rBV	206	88	0.01%	0.001%
42	6.677	1748	1753	1755	rBV	212	153	0.01%	0.001%
43	6.703	1758	1761	1764	rBV2	453	318	0.02%	0.003%
44	6.735	1767	1771	1774	rBV	387	262	0.02%	0.002%
45	6.815	1793	1796	1797	rBV	173	98	0.01%	0.001%
46	6.847	1803	1806	1809	rBV	350	240	0.01%	0.002%
47	6.883	1816	1817	1820	rVB	424	127	0.01%	0.001%
48	6.902	1820	1823	1828	rVB3	389	339	0.02%	0.003%
49	6.924	1828	1830	1833	rBV	416	239	0.01%	0.002%
50	6.986	1837	1849	1880	rBV	181201	343095	21.14%	2.869%
51	7.243	1925	1929	1932	rBV2	466	427	0.03%	0.004%
52	7.314	1939	1951	1997	rBV	755512	1321251	81.41%	11.048%
53	7.584	2033	2035	2036	rBV	386	174	0.01%	0.001%
54	7.619	2037	2046	2072	rVV	122946	222951	13.74%	1.864%
55	7.908	2131	2136	2138	rBV	404	323	0.02%	0.003%
56	7.941	2144	2146	2150	rVB4	603	330	0.02%	0.003%
57	7.986	2152	2160	2166	rBV6	1960	2724	0.17%	0.023%
58	8.088	2182	2192	2231	rBV	318257	733683	45.21%	6.135%
59	8.522	2324	2327	2330	rBV3	543	387	0.02%	0.003%
60	8.580	2342	2345	2351	rBV4	511	451	0.03%	0.004%
61	8.722	2386	2389	2392	rBV2	443	219	0.01%	0.002%
62	8.850	2417	2429	2459	rBV	615507	1016253	62.62%	8.497%
63	9.082	2497	2501	2504	rBV3	415	348	0.02%	0.003%
64	9.108	2506	2509	2512	rBV4	727	496	0.03%	0.004%
65	9.230	2545	2547	2550	rBV2	329	124	0.01%	0.001%
66	9.285	2561	2564	2567	rVB4	368	195	0.01%	0.002%
67	9.307	2567	2571	2573	rBV2	674	374	0.02%	0.003%
68	9.355	2583	2586	2589	rBV	435	325	0.02%	0.003%
69	9.391	2595	2597	2600	rVB	475	215	0.01%	0.002%
70	9.413	2600	2604	2607	rBV2	238	174	0.01%	0.001%
71	9.432	2607	2610	2611	rVV2	201	113	0.01%	0.001%
72	9.442	2611	2613	2615	rVB	344	116	0.01%	0.001%
73	9.471	2620	2622	2623	rBV	230	98	0.01%	0.001%
74	9.516	2634	2636	2638	rBV	200	87	0.01%	0.001%
75	9.551	2641	2647	2652	rBV4	2521	3649	0.22%	0.031%
76	9.706	2693	2695	2698	rBV	259	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025999.D
 Acq On : 06 Jun 2022 14:02
 Operator : SY/MD
 Sample : N3171-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.760	2710	2712	2719	rBV2	368	326	0.02%	0.003%
78	9.793	2720	2722	2725	rVB	528	256	0.02%	0.002%
79	9.812	2725	2728	2729	rBV	266	136	0.01%	0.001%
80	9.937	2761	2767	2774	rVB3	3357	4049	0.25%	0.034%
81	10.111	2819	2821	2824	rBV2	160	106	0.01%	0.001%
82	10.214	2841	2853	2877	rBV	482311	769925	47.44%	6.438%
83	10.667	2992	2994	2997	rVB2	363	202	0.01%	0.002%
84	10.699	3002	3004	3007	rVB	304	138	0.01%	0.001%
85	10.715	3007	3009	3011	rBV	226	96	0.01%	0.001%
86	10.754	3018	3021	3026	rVB2	338	194	0.01%	0.002%
87	10.805	3034	3037	3041	rVB3	553	315	0.02%	0.003%
88	10.860	3051	3054	3059	rBV2	616	593	0.04%	0.005%
89	10.921	3067	3073	3085	rVB5	3318	4918	0.30%	0.041%
90	10.992	3093	3095	3096	rBV	282	106	0.01%	0.001%
91	11.040	3107	3110	3112	rBV	392	251	0.02%	0.002%
92	11.092	3123	3126	3128	rBV	293	200	0.01%	0.002%
93	11.185	3148	3155	3163	rBV3	5040	8013	0.49%	0.067%
94	11.246	3163	3174	3201	rVV	613374	961630	59.25%	8.041%
95	11.622	3277	3291	3314	rBV	741017	1181936	72.83%	9.883%
96	12.391	3527	3530	3534	rBV2	581	411	0.03%	0.003%
97	12.648	3603	3610	3621	rVB4	7361	10883	0.67%	0.091%
98	13.265	3794	3802	3812	rBV2	9807	14569	0.90%	0.122%
99	13.503	3867	3876	3889	rBV	27330	44815	2.76%	0.375%
100	13.744	3943	3951	3962	rVB2	11411	17383	1.07%	0.145%



Sum of corrected areas: 11959666

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025999.D
Acq On : 06 Jun 2022 14:02
Operator : SY/MD
Sample : N3171-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

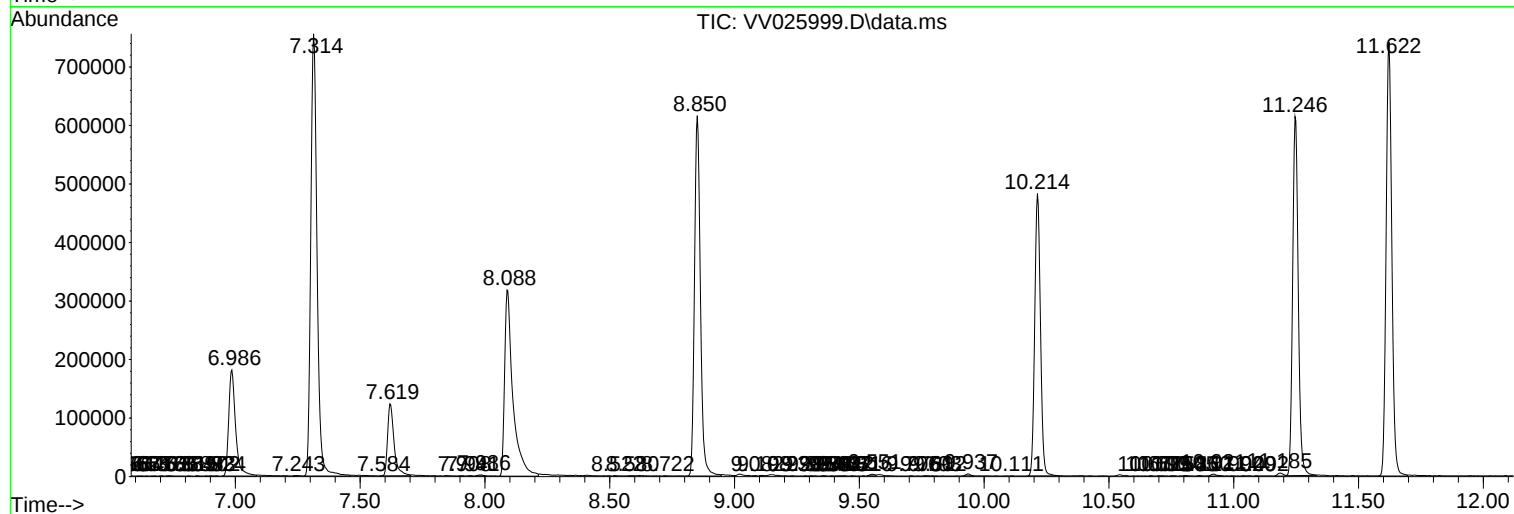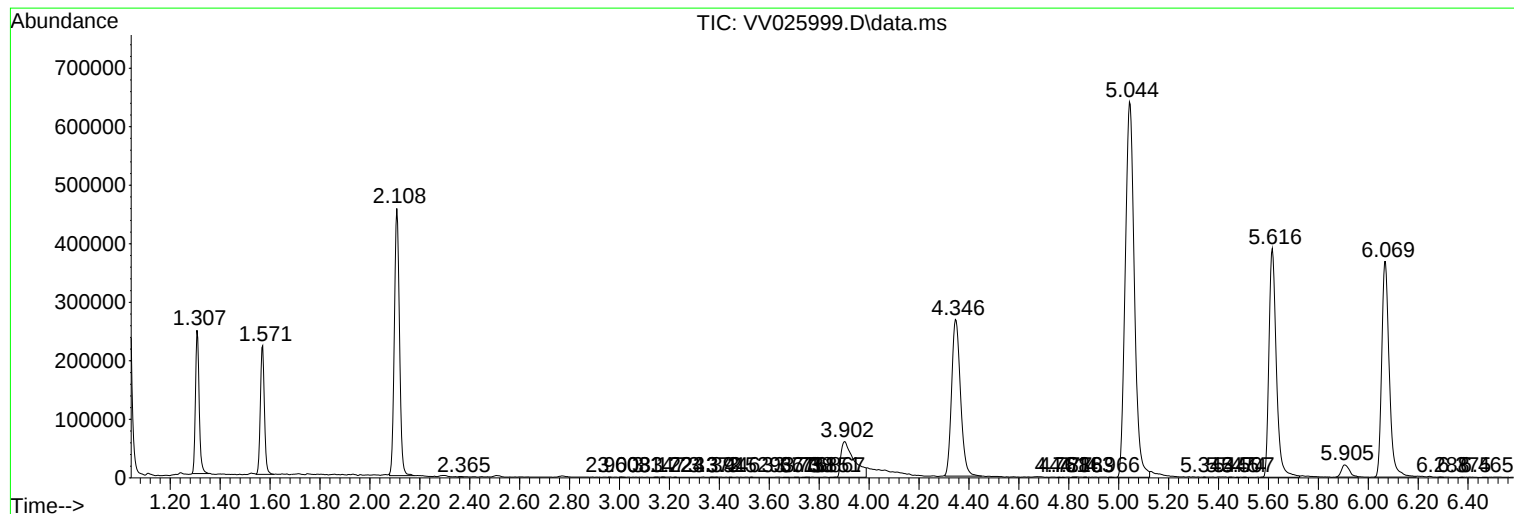

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025999.D
Acq On : 06 Jun 2022 14:02
Operator : SY/MD
Sample : N3171-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV025999.D
Acq On : 06 Jun 2022 14:02
Operator : SY/MD
Sample : N3171-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------