

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV026000.D
 Acq On : 06 Jun 2022 14:28
 Operator : SY/MD
 Sample : N3173-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV026000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	103	rVB	229894	245105	15.73%	2.157%
2	1.571	157	165	177	rVB	201594	229271	14.72%	2.018%
3	2.108	322	332	356	rVB	439432	630292	40.46%	5.548%
4	2.664	503	505	510	rBV	357	196	0.01%	0.002%
5	2.732	524	526	530	rVB	366	242	0.02%	0.002%
6	2.770	530	538	544	rBV8	1355	2501	0.16%	0.022%
7	2.860	564	566	568	rBV	302	117	0.01%	0.001%
8	3.088	635	637	639	rVB2	435	180	0.01%	0.002%
9	3.204	671	673	675	rBV	372	166	0.01%	0.001%
10	3.278	693	696	697	rBV	271	173	0.01%	0.002%
11	3.304	701	704	710	rVB	362	312	0.02%	0.003%
12	3.330	710	712	714	rBV	171	62	0.00%	0.001%
13	3.539	774	777	780	rBV3	349	266	0.02%	0.002%
14	3.593	791	794	796	rBV2	531	393	0.03%	0.003%
15	3.648	808	811	813	rBV	264	157	0.01%	0.001%
16	3.748	838	842	843	rBV	230	173	0.01%	0.002%
17	3.757	843	845	848	rVB2	386	179	0.01%	0.002%
18	3.777	848	851	853	rBV2	223	131	0.01%	0.001%
19	3.905	881	891	928	rBV	57386	261390	16.78%	2.301%
20	4.349	1014	1029	1054	rBV	258515	635343	40.78%	5.592%
21	4.606	1106	1109	1117	rVB6	869	995	0.06%	0.009%
22	4.641	1117	1120	1121	rBV2	397	239	0.02%	0.002%
23	4.770	1156	1160	1162	rBV	345	239	0.02%	0.002%
24	4.783	1162	1164	1165	rVV	247	78	0.01%	0.001%
25	4.940	1211	1213	1216	rBV3	332	145	0.01%	0.001%
26	5.047	1229	1246	1286	rBV2	605317	1557855	100.00%	13.712%
27	5.410	1356	1359	1361	rBV2	783	434	0.03%	0.004%
28	5.510	1386	1390	1394	rBV2	415	329	0.02%	0.003%
29	5.529	1394	1396	1399	rVB	227	104	0.01%	0.001%
30	5.555	1402	1404	1406	rVB2	302	116	0.01%	0.001%
31	5.574	1406	1410	1411	rBV2	501	317	0.02%	0.003%
32	5.616	1412	1423	1447	rBV	365771	742148	47.64%	6.532%
33	5.908	1503	1514	1533	rBV3	21498	47901	3.07%	0.422%
34	6.069	1550	1564	1595	rBV	357345	737035	47.31%	6.487%
35	6.336	1643	1647	1648	rBV2	374	258	0.02%	0.002%
36	6.403	1667	1668	1672	rBV2	250	187	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV026000.D
 Acq On : 06 Jun 2022 14:28
 Operator : SY/MD
 Sample : N3173-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	6.423	1672	1674	1676	rVB	453	202	0.01%	0.002%
38	6.445	1679	1681	1684	rBV	545	340	0.02%	0.003%
39	6.465	1685	1687	1689	rVB2	275	94	0.01%	0.001%
40	6.558	1713	1716	1721	rBV2	386	307	0.02%	0.003%
41	6.583	1721	1724	1726	rVV2	271	143	0.01%	0.001%
42	6.628	1736	1738	1741	rVB2	299	144	0.01%	0.001%
43	6.641	1741	1742	1745	rBV	340	212	0.01%	0.002%
44	6.667	1748	1750	1752	rVB	303	97	0.01%	0.001%
45	6.680	1752	1754	1755	rBV	123	57	0.00%	0.001%
46	6.728	1766	1769	1772	rBV	214	138	0.01%	0.001%
47	6.911	1824	1826	1828	rVB	159	44	0.00%	0.000%
48	6.921	1828	1829	1830	rVB	108	21	0.00%	0.000%
49	6.931	1830	1832	1833	rBV	201	99	0.01%	0.001%
50	6.985	1838	1849	1878	rBV	172803	323031	20.74%	2.843%
51	7.313	1939	1951	1980	rBV	705399	1240358	79.62%	10.917%
52	7.619	2037	2046	2074	rBV	116774	213604	13.71%	1.880%
53	7.882	2126	2128	2132	rVB3	524	294	0.02%	0.003%
54	7.934	2140	2144	2146	rBV3	389	301	0.02%	0.003%
55	7.972	2154	2156	2157	rBV	697	286	0.02%	0.003%
56	8.091	2182	2193	2241	rBV	325795	746329	47.91%	6.569%
57	8.667	2370	2372	2373	rBV	246	90	0.01%	0.001%
58	8.763	2400	2402	2405	rVB	385	139	0.01%	0.001%
59	8.780	2405	2407	2411	rBV2	419	212	0.01%	0.002%
60	8.805	2413	2415	2418	rVB2	371	224	0.01%	0.002%
61	8.850	2418	2429	2453	rBV	591678	956781	61.42%	8.421%
62	9.062	2492	2495	2500	rBV5	956	640	0.04%	0.006%
63	9.217	2541	2543	2547	rBV2	311	185	0.01%	0.002%
64	9.355	2581	2586	2588	rBV2	297	242	0.02%	0.002%
65	9.480	2622	2625	2630	rVB2	348	226	0.01%	0.002%
66	9.644	2675	2676	2677	rBV2	216	70	0.00%	0.001%
67	9.751	2705	2709	2714	rBV2	407	475	0.03%	0.004%
68	9.995	2782	2785	2788	rVB2	312	182	0.01%	0.002%
69	10.011	2788	2790	2794	rVB2	479	310	0.02%	0.003%
70	10.030	2794	2796	2799	rBV	321	236	0.02%	0.002%
71	10.214	2842	2853	2878	rBV	482408	753066	48.34%	6.628%
72	10.583	2965	2968	2970	rBV2	421	245	0.02%	0.002%
73	10.622	2976	2980	2983	rBV	358	321	0.02%	0.003%
74	10.683	2995	2999	3000	rBV	246	158	0.01%	0.001%
75	10.879	3058	3060	3061	rBV	245	119	0.01%	0.001%
76	10.953	3080	3083	3085	rBV2	430	294	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV026000.D
 Acq On : 06 Jun 2022 14:28
 Operator : SY/MD
 Sample : N3173-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M

Title : VOC Analysis

77	10.982	3090	3092	3094	rBV	346	196	0.01%	0.002%
78	11.249	3163	3175	3195	rBV	585411	899971	57.77%	7.921%
79	11.561	3269	3272	3274	rBV	516	309	0.02%	0.003%
80	11.622	3279	3291	3315	rBV	720387	1117257	71.72%	9.834%
81	12.210	3466	3474	3476	rBV2	421	650	0.04%	0.006%
82	12.384	3526	3528	3531	rBV2	408	246	0.02%	0.002%
83	12.648	3605	3610	3619	rVB6	1875	2653	0.17%	0.023%
84	13.127	3757	3759	3762	rBV	393	277	0.02%	0.002%
85	13.744	3945	3951	3962	rVB6	2838	4471	0.29%	0.039%




Sum of corrected areas: 11361375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV026000.D
Acq On : 06 Jun 2022 14:28
Operator : SY/MD
Sample : N3173-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

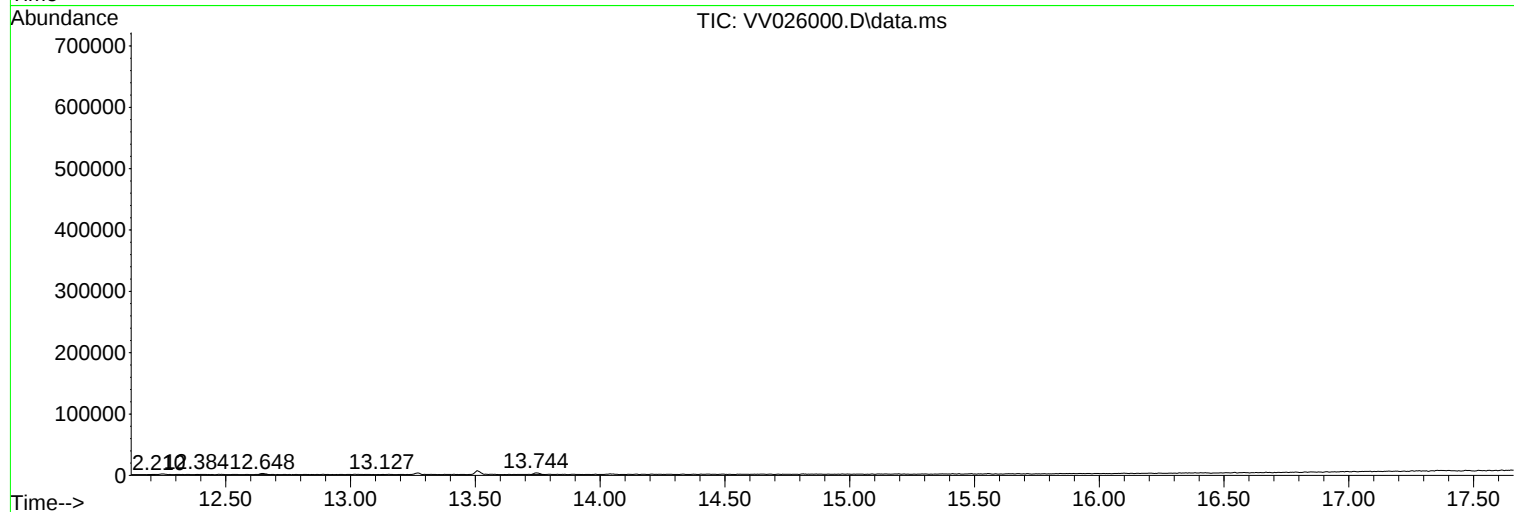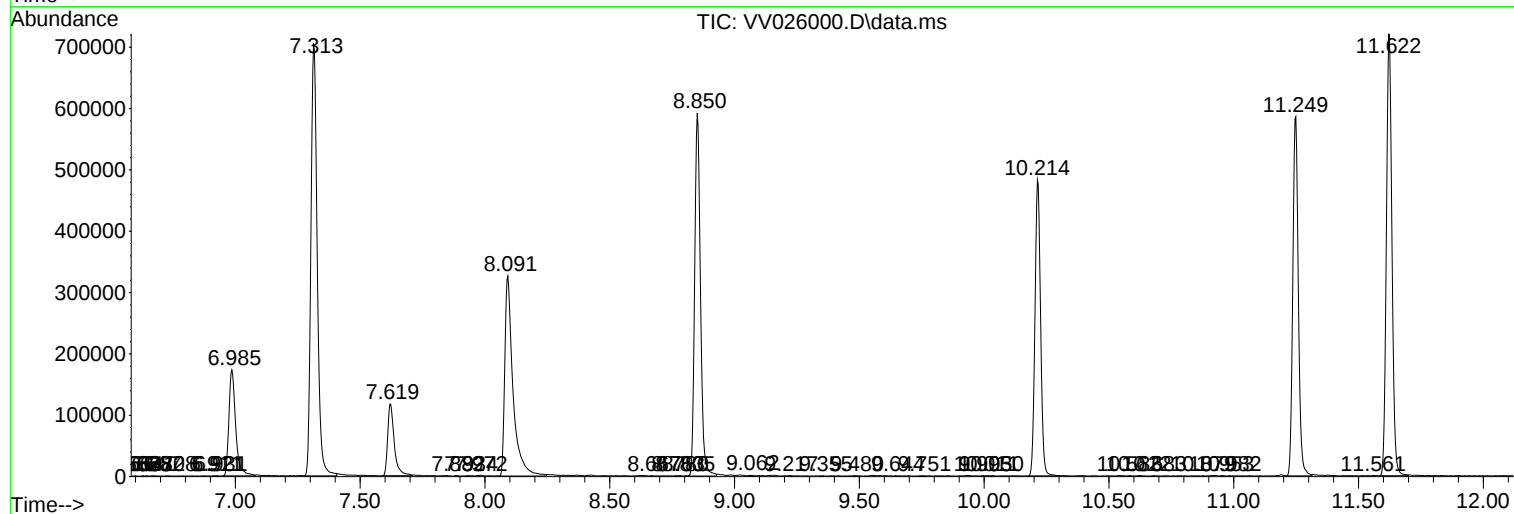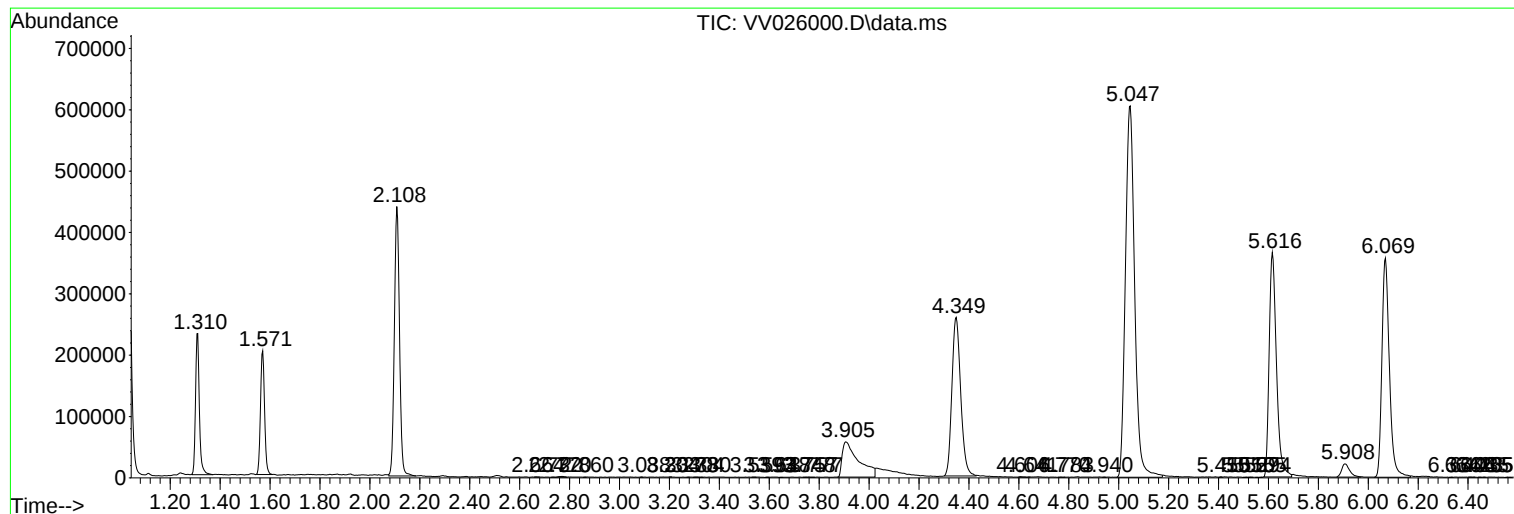

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV026000.D
Acq On : 06 Jun 2022 14:28
Operator : SY/MD
Sample : N3173-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
Data File : VV026000.D
Acq On : 06 Jun 2022 14:28
Operator : SY/MD
Sample : N3173-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------