
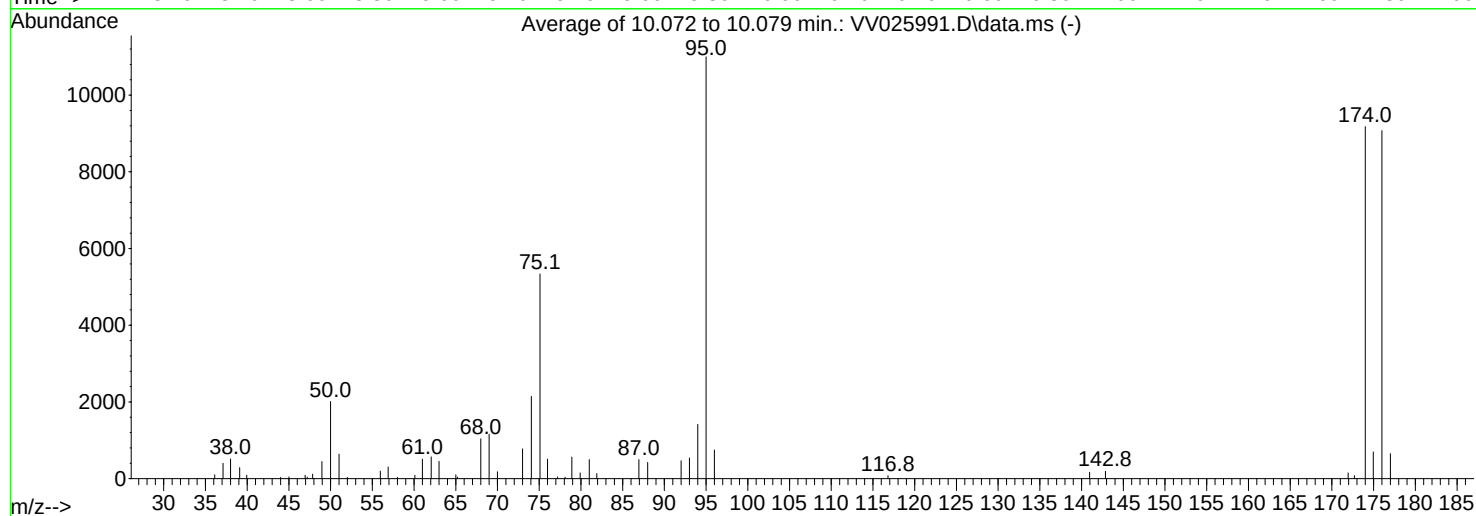


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060622\
 Data File : VV025991.D
 Acq On : 06 Jun 2022 08:51
 Operator : SY/MD
 Sample : BFB286
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB286

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 07 02:25:55 2022

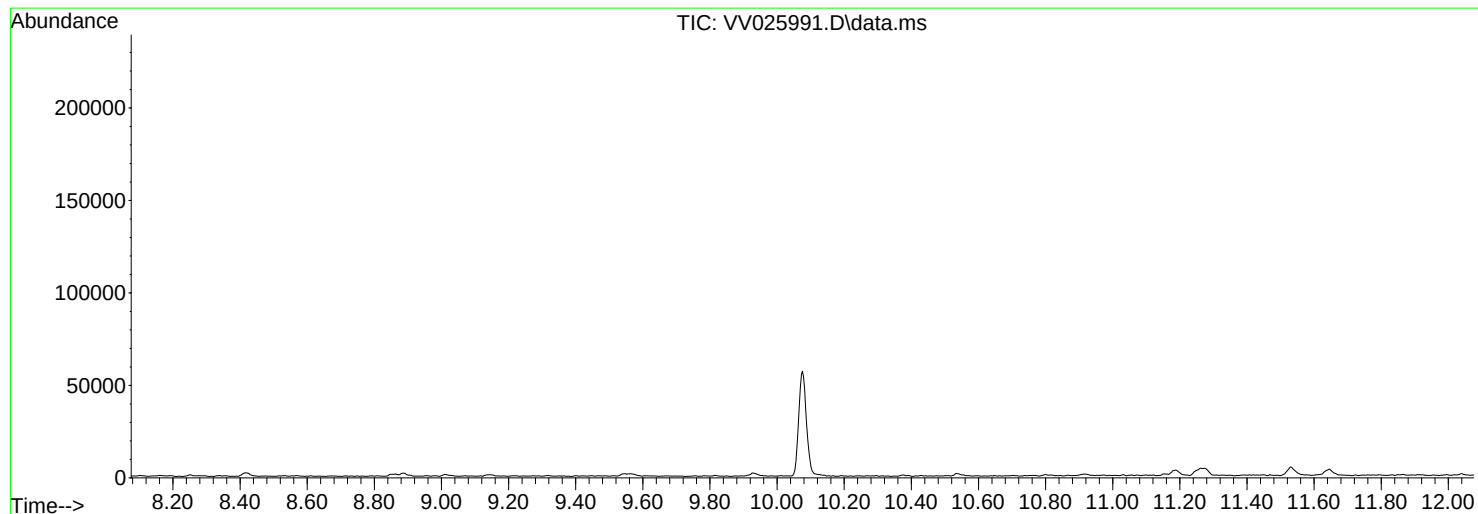

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	2011	PASS
75	95	30	80	48.5	5334	PASS
95	95	100	100	100.0	10997	PASS
96	95	5	9	6.8	748	PASS
173	174	0.00	2	0.9	81	PASS
174	95	50	120	83.5	9178	PASS
175	174	5	9	7.6	698	PASS
176	174	95	105	98.8	9072	PASS
177	176	5	10	7.2	651	PASS

m/z	Abundance
39.90	578.0
44.00	456.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
37.10	413.0
38.00	468.0
39.10	264.0
40.00	636.0
44.00	475.0
45.00	133.0
46.90	140.0
47.90	131.0
49.00	449.0
50.00	2064.0
51.00	689.0
52.00	105.0
55.90	197.0
56.90	356.0
58.00	102.0
60.10	142.0
61.00	502.0
62.00	639.0
63.00	425.0
65.00	168.0
68.00	939.0
69.00	1238.0
70.00	160.0
73.00	803.0
74.00	2225.0
75.10	5264.0
76.00	484.0
78.90	601.0
79.90	171.0
81.00	498.0
81.90	105.0
87.00	511.0
88.00	366.0
92.00	450.0
93.00	587.0
94.00	1415.0
95.00	10893.0
96.00	693.0
116.80	131.0
141.00	163.0
142.90	146.0
171.90	155.0
172.70	137.0
174.00	9090.0
174.90	639.0
176.00	8853.0
177.00	618.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
36.10	144.0
37.10	401.0
38.00	555.0
39.10	294.0
40.00	692.0
44.00	489.0
47.00	128.0
47.80	119.0
49.00	452.0
50.00	2030.0
51.00	645.0
56.00	206.0
56.90	316.0
60.10	125.0
61.00	507.0
62.00	588.0
63.00	458.0
65.00	133.0
68.00	1111.0
69.00	1174.0
70.00	190.0
73.00	821.0
74.10	2201.0
75.10	5481.0
76.00	522.0
78.90	580.0
79.90	154.0
81.00	505.0
81.90	137.0
87.00	507.0
88.00	442.0
92.00	495.0
93.00	540.0
94.00	1476.0
95.00	11357.0
96.00	766.0
116.80	103.0
141.00	185.0
142.90	193.0
171.90	145.0
172.70	106.0
174.00	9481.0
174.90	719.0
176.00	9350.0
177.00	672.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
36.10	152.0
37.10	387.0
38.00	519.0
39.10	304.0
40.00	682.0
44.00	507.0
47.20	125.0
47.80	104.0
48.90	436.0
50.00	1938.0
51.00	583.0
56.00	192.0
56.90	246.0
61.00	516.0
62.10	479.0
63.00	469.0
65.20	121.0
68.00	1071.0
69.00	1063.0
70.00	185.0
73.00	701.0
74.10	2004.0
75.10	5257.0
76.00	516.0
77.20	136.0
78.10	116.0
78.90	511.0
79.90	130.0
81.00	486.0
81.90	158.0
86.90	474.0
88.00	452.0
92.00	456.0
93.00	492.0
94.00	1347.0
95.00	10742.0
96.00	784.0
140.90	159.0
142.80	231.0
172.00	149.0
174.00	8963.0
175.00	737.0
176.00	9014.0
177.00	663.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286