




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031366.D
 Acq On : 06 Jun 2023 11:35
 Operator : SY/MD
 Sample : 03000-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C40

Manual IntegrationsAPPROVED

Quant Time: Jun 07 02:01:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123wMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 07 01:59:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/08/2023
 Supervised By :Mahesh Dadoda 06/08/2023

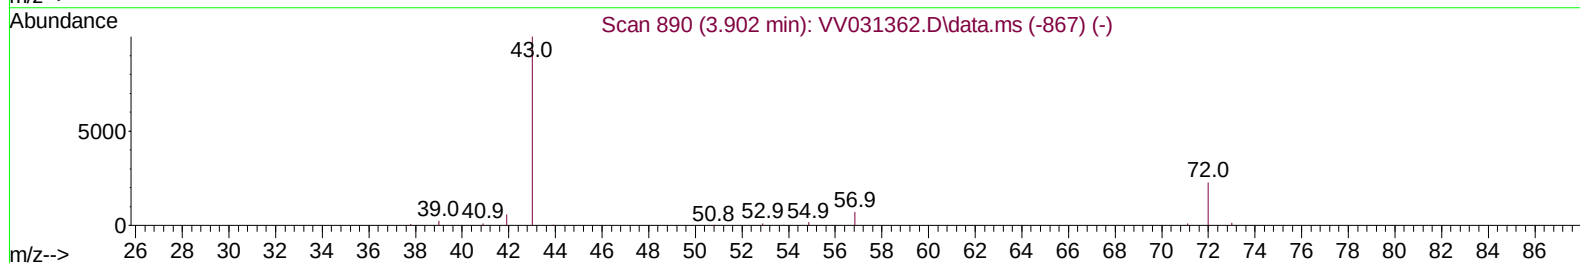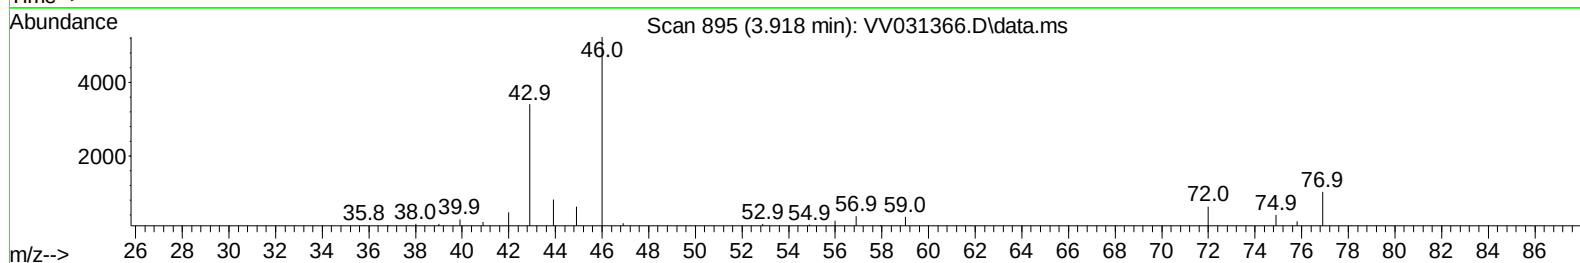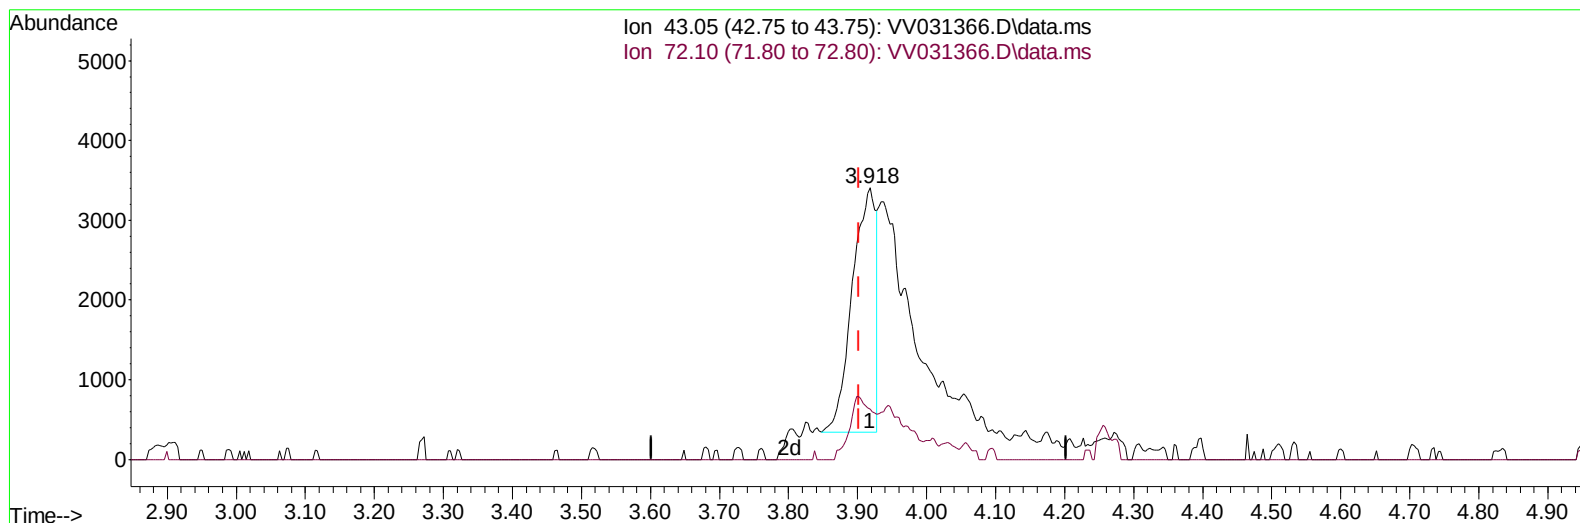

TIC: VV031366.D\data.ms

(21) 2-Butanone (T)

3.918min (+ 0.016) 1.61 ug/L

response 7328

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	15.70	24.96#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031366.D
 Acq On : 06 Jun 2023 11:35
 Operator : SY/MD
 Sample : 03000-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C40

Manual IntegrationsAPPROVED

Quant Time: Jun 07 02:01:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 07 01:59:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/08/2023
 Supervised By :Mahesh Dadoda 06/08/2023

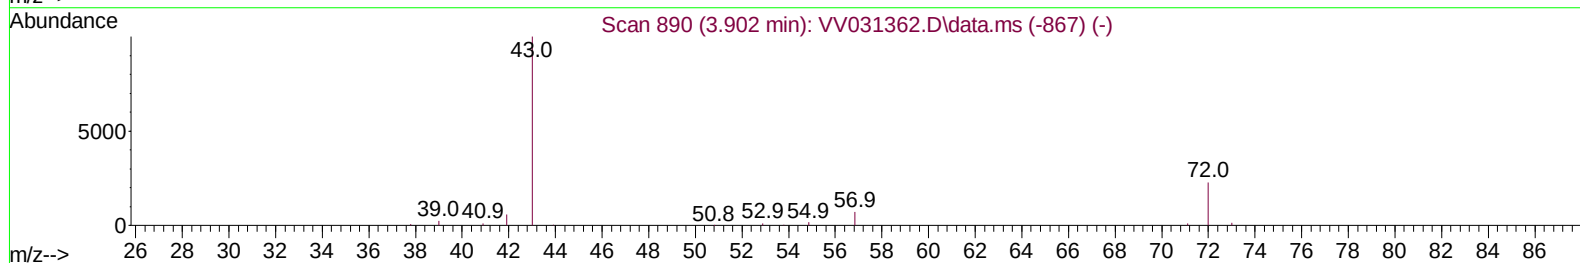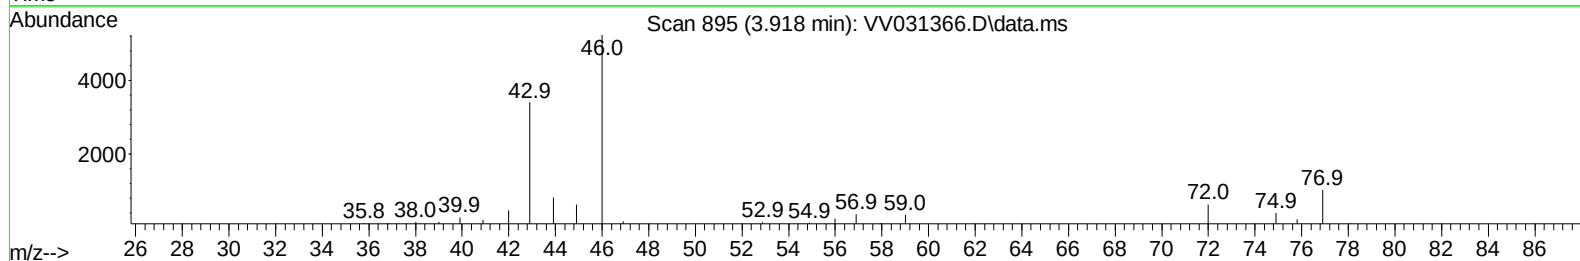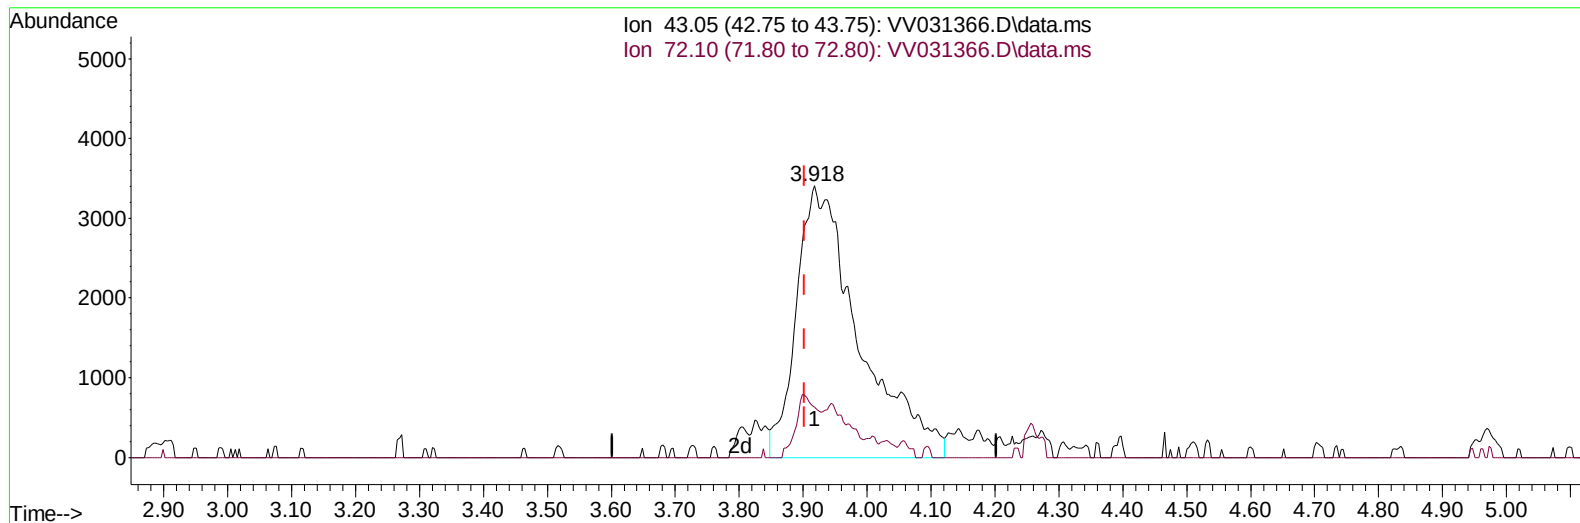

TIC: VV031366.D\data.ms

(21) 2-Butanone (T)

3.918min (+ 0.016) 5.08 ug/L m

response 23118

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	15.70	7.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031366.D
 Acq On : 06 Jun 2023 11:35
 Operator : SY/MD
 Sample : 03000-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C40

Manual IntegrationsAPPROVED

Quant Time: Jun 07 02:01:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 07 01:59:39 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/08/2023
 Supervised By :Mahesh Dadoda 06/08/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	128680	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	133438	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	60895	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	51015	3.897	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	78.000%		
7) Chloroethane-d5	1.536	69	48618	4.397	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	88.000%		
11) 1,1-Dichloroethene-d2	2.060	65	27390	4.310	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	86.200%		
20) 2-Butanone-d5	3.825	46	129530	42.754	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	85.500%		
24) Chloroform-d	4.256	84	112583	5.116	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	102.400%		
26) 1,2-Dichloroethane-d4	4.950	65	57396	4.863	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.200%		
32) Benzene-d6	4.966	84	191706	4.726	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.600%		
36) 1,2-Dichloropropane-d6	5.995	67	68515	5.001	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	100.000%		
41) Toluene-d8	7.249	98	164381	4.315	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	86.400%		
43) trans-1,3-Dichloroprop...	7.561	79	20442	4.098	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	82.000%		
46) 2-Hexanone-d5	8.034	63	77333	38.591	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	77.180%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	42508	4.081	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	81.600%		
66) 1,2-Dichlorobenzene-d4	11.567	152	58319	5.078	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	101.600%		
Target Compounds						
						Qvalue
13) Acetone	2.153	43	39472	11.274	ug/L	75
14) Carbon disulfide	2.246	76	3455	0.097	ug/L	99
21) 2-Butanone	3.918	43	23118m	5.077	ug/L	
47) Tetrachloroethene	7.915	164	2021	0.202	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031366.D
Acq On : 06 Jun 2023 11:35
Operator : SY/MD
Sample : 03000-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C40

Manual IntegrationsAPPROVED

Quant Time: Jun 07 02:01:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 07 01:59:39 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/08/2023
Supervised By :Mahesh Dadoda 06/08/2023

