

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031364.D
 Acq On : 06 Jun 2023 10:46
 Operator : SY/MD
 Sample : 03000-03 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	95	rVB	73042	85717	4.43%	1.331%
2	1.532	145	153	167	rBV	72863	85286	4.41%	1.324%
3	2.060	306	317	336	rBV	146984	215328	11.14%	3.343%
4	2.709	507	519	532	rBV3	8191	19492	1.01%	0.303%
5	3.828	853	867	890	rBV4	54771	189766	9.82%	2.947%
6	4.256	985	1000	1023	rBV2	93842	240140	12.42%	3.729%
7	4.963	1204	1220	1246	rBV4	209433	542526	28.06%	8.424%
8	5.538	1387	1399	1419	rBV	149285	316476	16.37%	4.914%
9	5.838	1478	1492	1516	rBV2	163948	344858	17.84%	5.355%
10	5.995	1529	1541	1560	rBV2	127012	266097	13.76%	4.132%
11	6.921	1816	1829	1854	rBV2	48097	102077	5.28%	1.585%
12	7.249	1919	1931	1960	rBV	218270	404330	20.91%	6.278%
13	7.561	2017	2028	2050	rBV2	28386	60296	3.12%	0.936%
14	7.908	2121	2136	2166	rBV	1104272	1933373	100.00%	30.020%
15	8.037	2167	2176	2220	rVV	159389	425125	21.99%	6.601%
16	8.789	2399	2410	2436	rBV	231407	407663	21.09%	6.330%
17	10.159	2824	2836	2855	rBV2	77245	131838	6.82%	2.047%
18	11.191	3146	3157	3179	rBV	211109	342314	17.71%	5.315%
19	11.567	3260	3274	3294	rBV	202926	327563	16.94%	5.086%




Sum of corrected areas: 6440265

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031364.D
Acq On : 06 Jun 2023 10:46
Operator : SY/MD
Sample : 03000-03 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

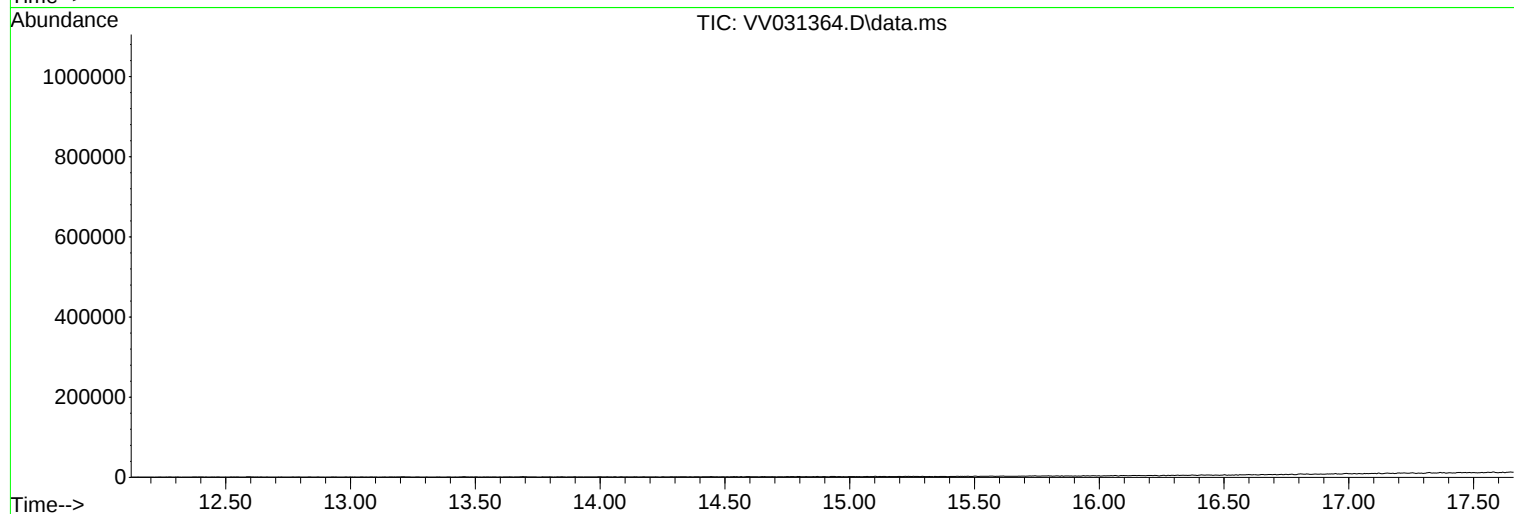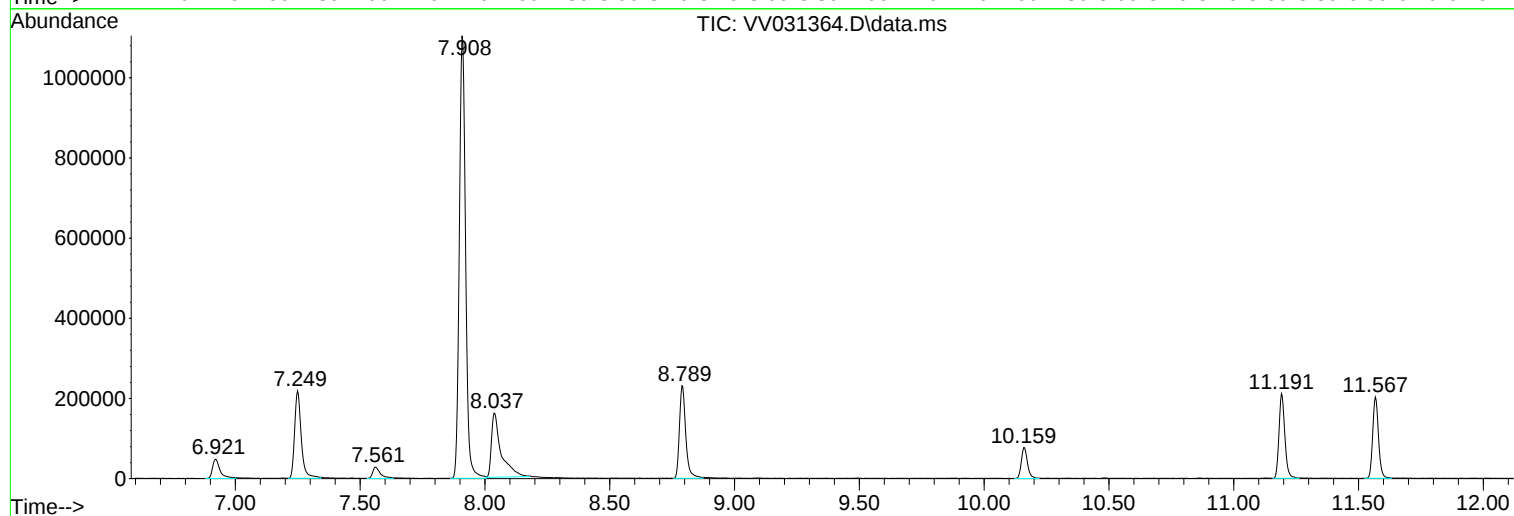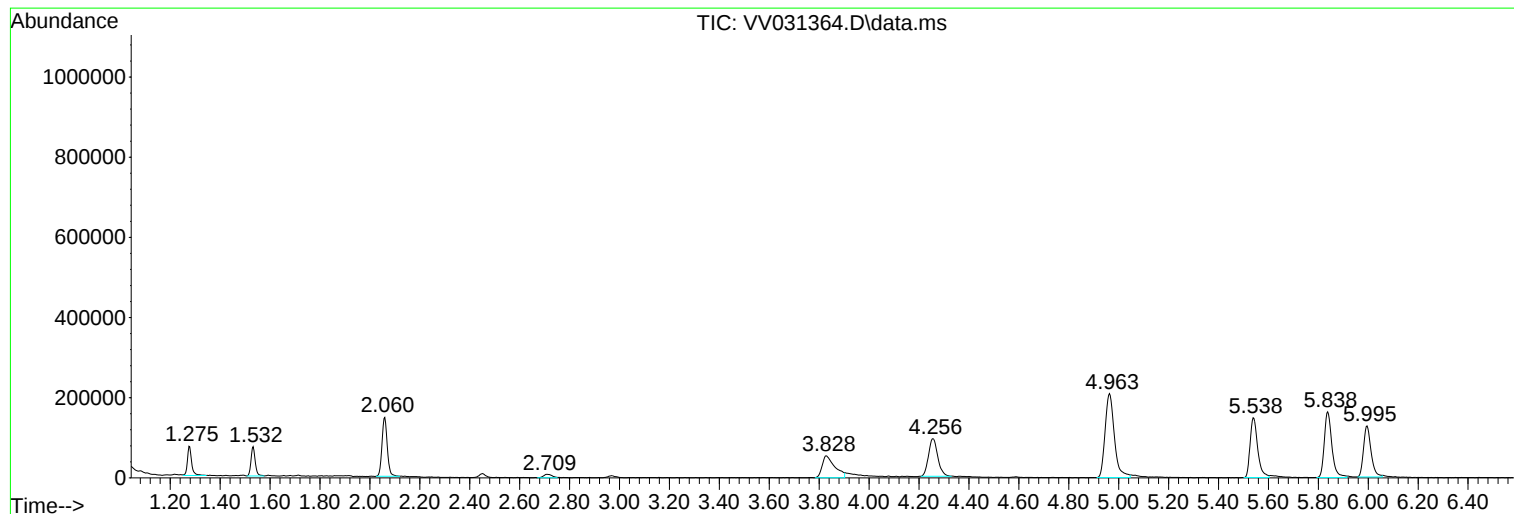

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031364.D
Acq On : 06 Jun 2023 10:46
Operator : SY/MD
Sample : 03000-03 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031364.D
Acq On : 06 Jun 2023 10:46
Operator : SY/MD
Sample : 03000-03 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------