

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031365.D
 Acq On : 06 Jun 2023 11:10
 Operator : SY/MD
 Sample : 03000-04 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	85	rVB	76272	82970	5.36%	1.384%
2	1.532	145	153	166	rVB	75909	86797	5.60%	1.448%
3	2.060	304	317	330	rBV	150890	218834	14.13%	3.651%
4	2.716	506	521	539	rBV3	9896	22485	1.45%	0.375%
5	3.825	852	866	901	rBV4	91124	298642	19.28%	4.982%
6	4.256	984	1000	1029	rVB2	97030	250263	16.16%	4.175%
7	4.963	1202	1220	1247	rBV2	213618	545229	35.21%	9.096%
8	5.539	1388	1399	1419	rBV	144777	302220	19.51%	5.042%
9	5.841	1479	1493	1511	rBV2	75997	163987	10.59%	2.736%
10	5.995	1528	1541	1559	rBV	126688	269681	17.41%	4.499%
11	6.921	1819	1829	1846	rBV	48906	96525	6.23%	1.610%
12	7.249	1919	1931	1962	rBV	216568	408850	26.40%	6.821%
13	7.561	2018	2028	2045	rBV3	28700	57847	3.74%	0.965%
14	7.908	2118	2136	2166	rBV	884558	1548708	100.00%	25.838%
15	8.037	2167	2176	2217	rVV	164929	440542	28.45%	7.350%
16	8.792	2399	2411	2441	rBV	226011	391982	25.31%	6.540%
17	10.159	2826	2836	2853	rBV	83736	141828	9.16%	2.366%
18	11.191	3146	3157	3180	rBV	203343	329612	21.28%	5.499%
19	11.567	3262	3274	3293	rBV	208755	336896	21.75%	5.621%




Sum of corrected areas: 5993898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031365.D
Acq On : 06 Jun 2023 11:10
Operator : SY/MD
Sample : 03000-04 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

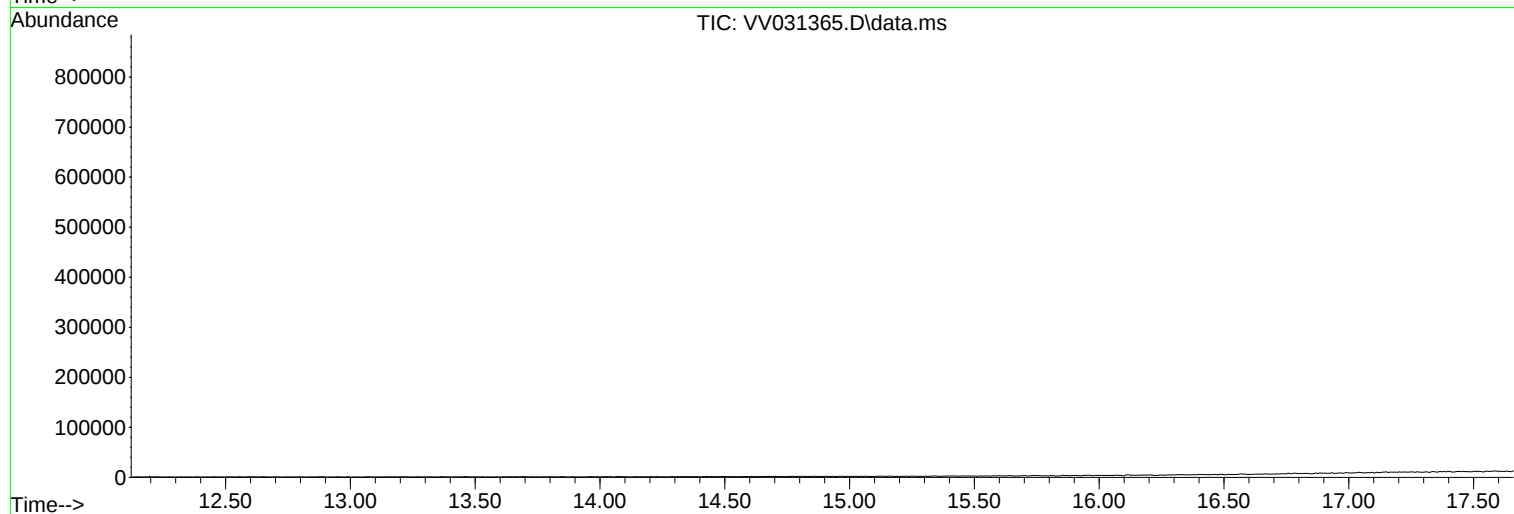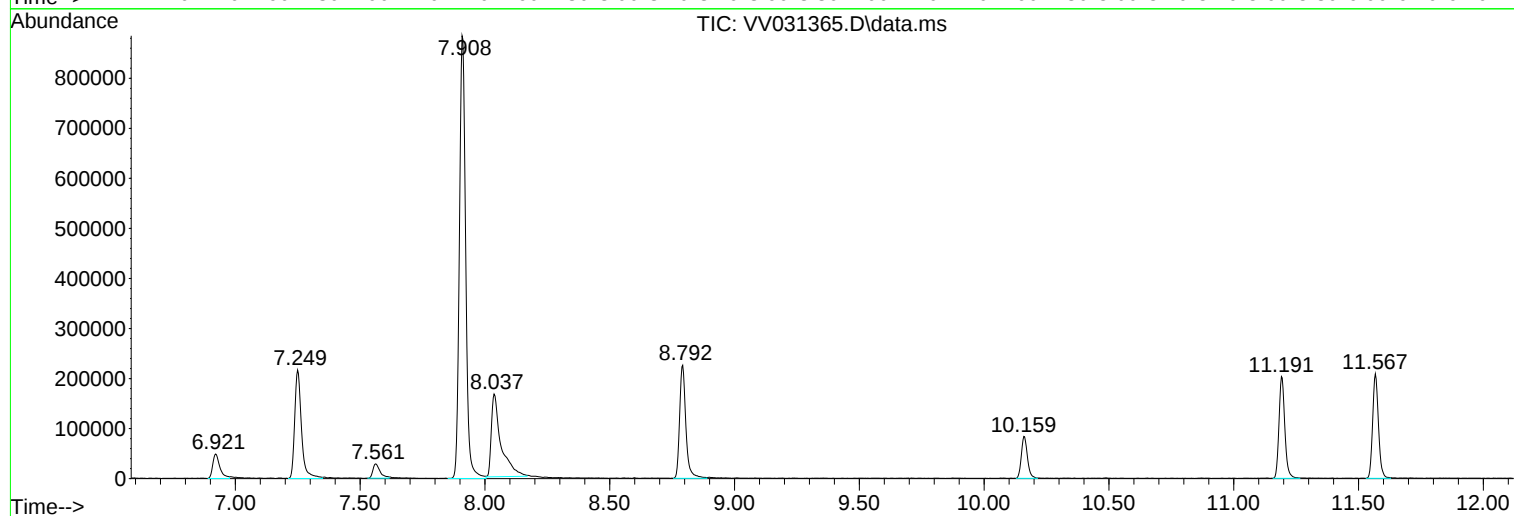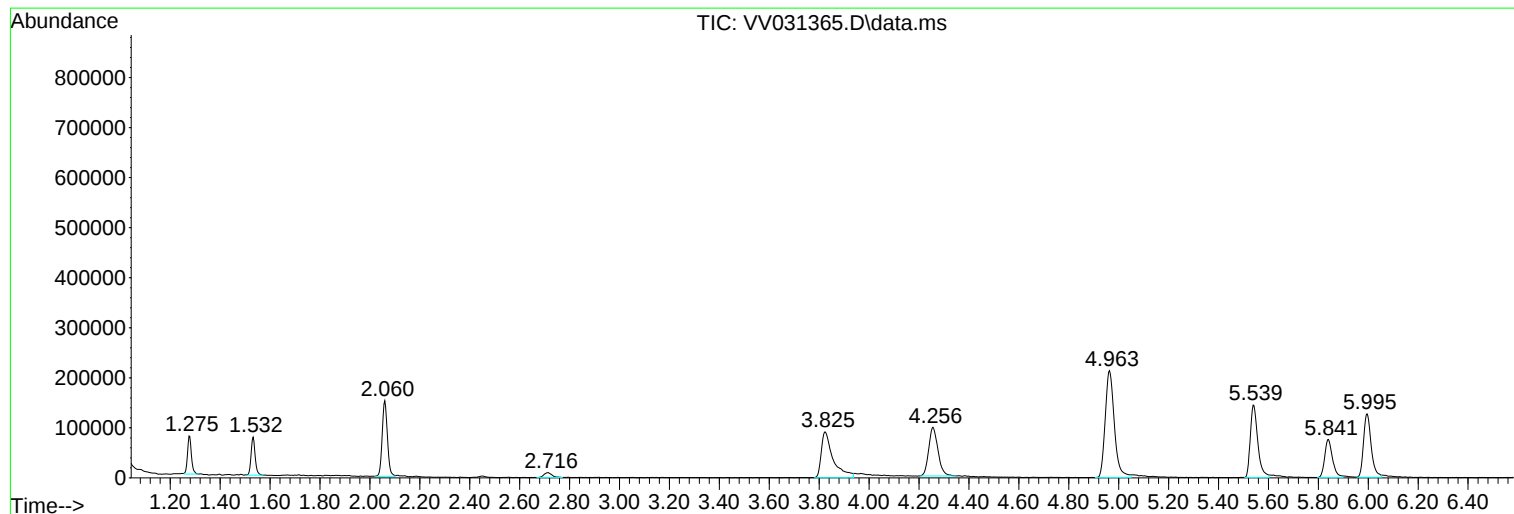

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031365.D
Acq On : 06 Jun 2023 11:10
Operator : SY/MD
Sample : 03000-04 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031365.D
Acq On : 06 Jun 2023 11:10
Operator : SY/MD
Sample : 03000-04 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------