

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031367.D
 Acq On : 06 Jun 2023 11:59
 Operator : SY/MD
 Sample : 03000-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C41

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	70565	76351	14.52%	1.808%
2	1.535	145	154	165	rBV	68820	82529	15.69%	1.955%
3	2.063	307	318	333	rBV	138084	202150	38.43%	4.788%
4	3.822	851	865	901	rBV2	46325	186351	35.43%	4.414%
5	4.256	984	1000	1022	rBV2	94215	245292	46.63%	5.810%
6	4.963	1202	1220	1244	rBV2	200652	525996	100.00%	12.459%
7	5.542	1386	1400	1419	rBV	153928	331128	62.95%	7.843%
8	5.834	1480	1491	1507	rVB7	9570	20490	3.90%	0.485%
9	5.995	1527	1541	1567	rBV	126253	273946	52.08%	6.489%
10	6.172	1586	1596	1613	rBV5	7984	17835	3.39%	0.422%
11	6.921	1818	1829	1852	rBV	49240	98445	18.72%	2.332%
12	7.249	1919	1931	1957	rBV	213577	400540	76.15%	9.487%
13	7.561	2019	2028	2043	rBV	29474	56757	10.79%	1.344%
14	8.037	2166	2176	2211	rBV2	177395	436812	83.04%	10.346%
15	8.792	2400	2411	2435	rBV	247626	427027	81.18%	10.114%
16	10.159	2826	2836	2857	rVB2	74111	118259	22.48%	2.801%
17	10.333	2878	2890	2899	rBV2	12185	19897	3.78%	0.471%
18	11.191	3144	3157	3175	rBV	233613	368377	70.03%	8.725%
19	11.567	3262	3274	3293	rBV	206840	333796	63.46%	7.906%




Sum of corrected areas: 4221978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031367.D
Acq On : 06 Jun 2023 11:59
Operator : SY/MD
Sample : 03000-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

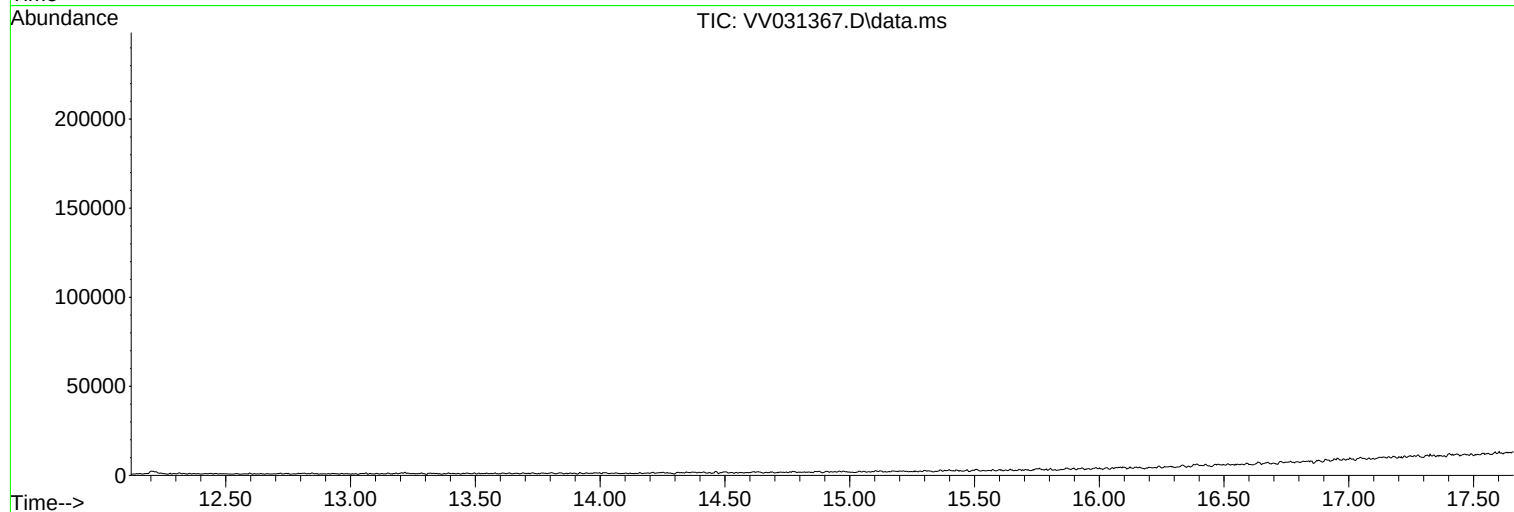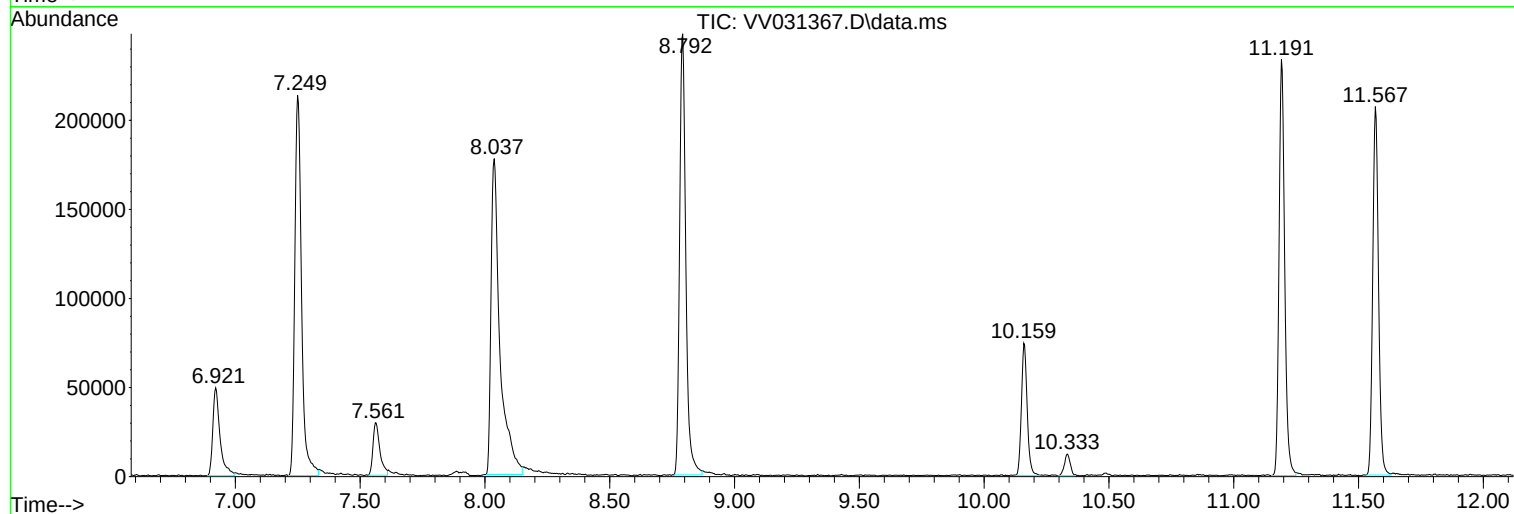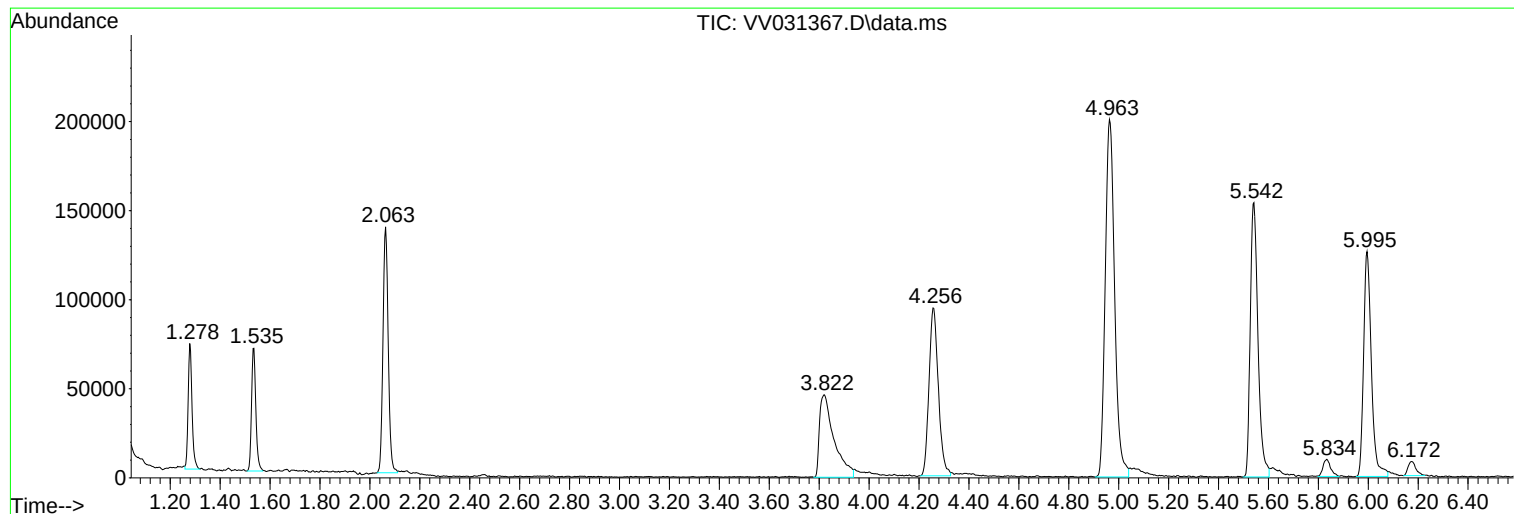

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031367.D
Acq On : 06 Jun 2023 11:59
Operator : SY/MD
Sample : 03000-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031367.D
Acq On : 06 Jun 2023 11:59
Operator : SY/MD
Sample : 03000-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc