

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031368.D
 Acq On : 06 Jun 2023 12:24
 Operator : SY/MD
 Sample : 03000-01DL 25X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C03DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	76695	86964	12.35%	1.669%
2	1.536	146	154	167	rVB	73504	85978	12.21%	1.650%
3	2.060	306	317	336	rBV	144059	217546	30.89%	4.175%
4	2.452	430	439	452	rVB3	8595	14530	2.06%	0.279%
5	2.709	505	519	536	rBV3	18989	41430	5.88%	0.795%
6	3.818	851	864	899	rBV	61026	240028	34.09%	4.606%
7	4.256	984	1000	1024	rBV2	100377	264870	37.61%	5.083%
8	4.963	1201	1220	1245	rBV4	217905	569714	80.91%	10.933%
9	5.542	1386	1400	1422	rBV	153469	325868	46.28%	6.254%
10	5.841	1480	1493	1510	rBV7	23936	56613	8.04%	1.086%
11	5.995	1528	1541	1562	rBV2	134293	286147	40.64%	5.491%
12	6.921	1814	1829	1852	rBV	52607	106693	15.15%	2.048%
13	7.249	1919	1931	1953	rBV	230501	419974	59.64%	8.060%
14	7.561	2019	2028	2046	rBV	31753	62964	8.94%	1.208%
15	7.911	2117	2137	2162	rBV	396223	704171	100.00%	13.513%
16	8.037	2166	2176	2211	rBV2	206513	470149	66.77%	9.022%
17	8.792	2399	2411	2431	rBV	241093	410818	58.34%	7.884%
18	10.159	2825	2836	2850	rBV	86587	141369	20.08%	2.713%
19	11.191	3146	3157	3180	rBV	213948	348103	49.43%	6.680%
20	11.567	3262	3274	3295	rBV	221708	356950	50.69%	6.850%




Sum of corrected areas: 5210879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031368.D
Acq On : 06 Jun 2023 12:24
Operator : SY/MD
Sample : 03000-01DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C03DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

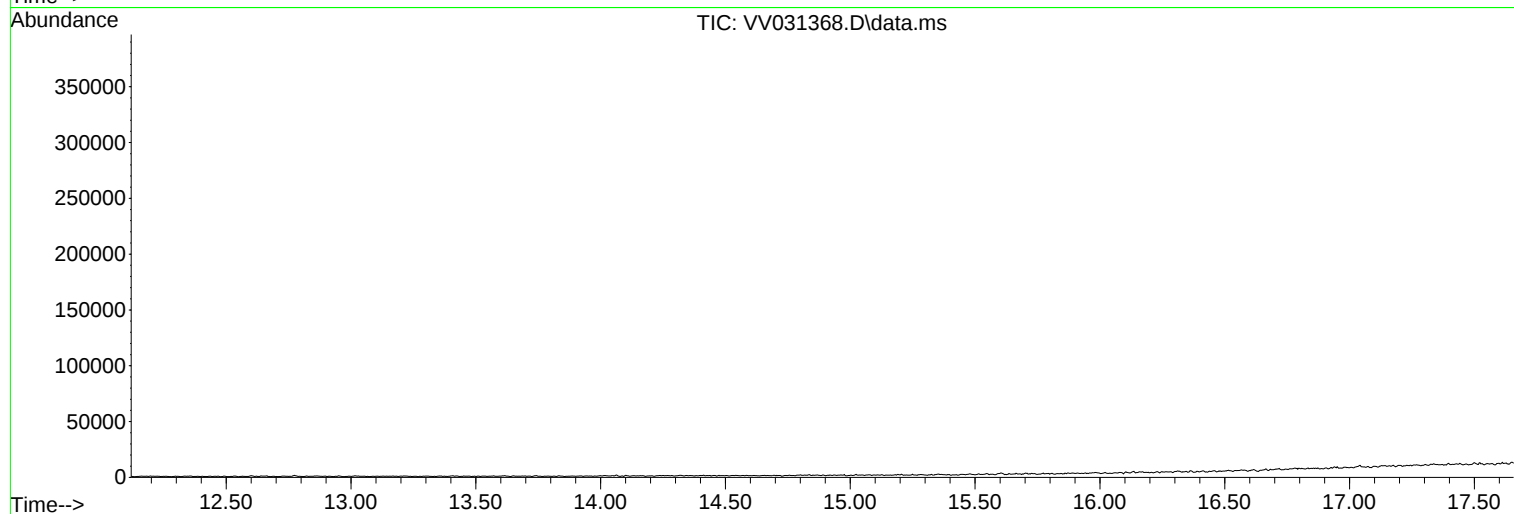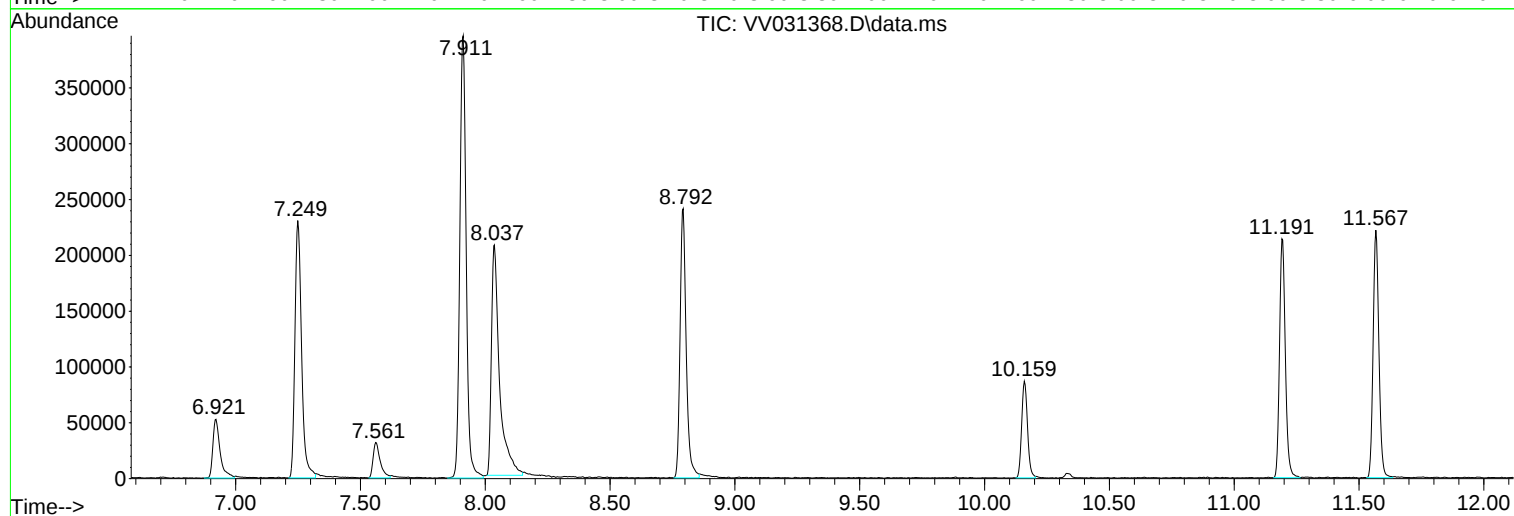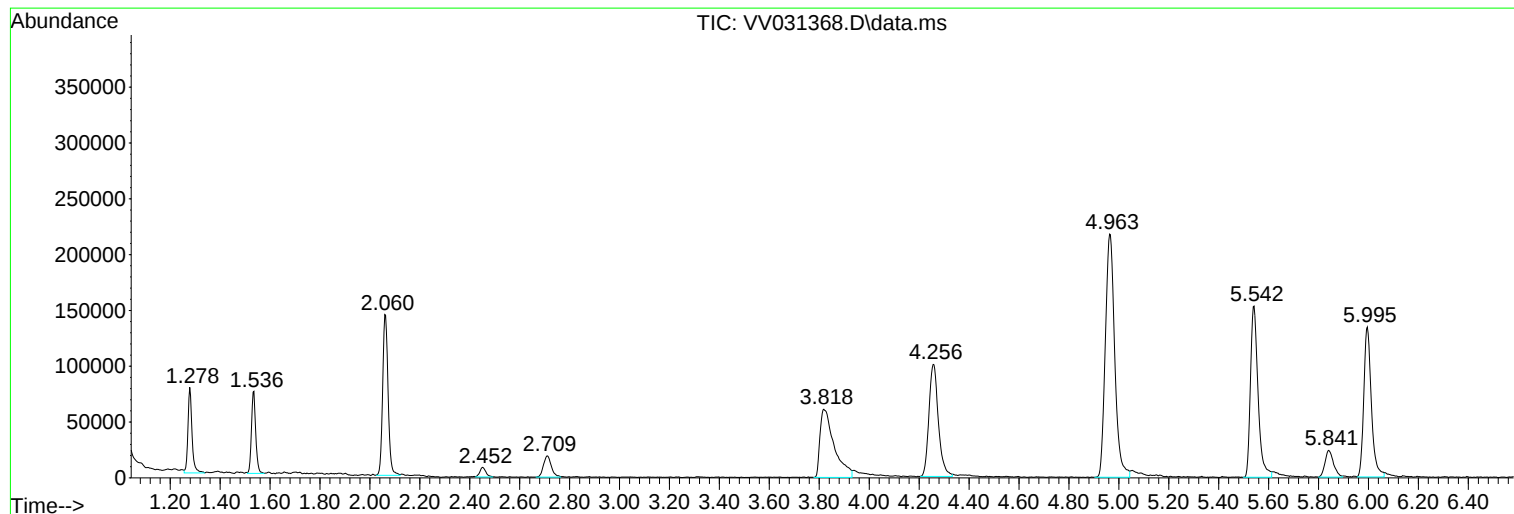

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031368.D
Acq On : 06 Jun 2023 12:24
Operator : SY/MD
Sample : 03000-01DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C03DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031368.D
Acq On : 06 Jun 2023 12:24
Operator : SY/MD
Sample : 03000-01DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C03DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc