

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031369.D
 Acq On : 06 Jun 2023 12:48
 Operator : SY/MD
 Sample : 03000-02DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C25DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	71979	81637	15.31%	1.731%
2	1.536	145	154	166	rBV	70812	84026	15.76%	1.781%
3	2.063	307	318	333	rBV	138698	205030	38.45%	4.347%
4	2.452	429	439	452	rBV	10557	17999	3.38%	0.382%
5	3.825	850	866	898	rBV2	51846	217398	40.77%	4.609%
6	4.259	982	1001	1025	rBV2	94908	249209	46.74%	5.284%
7	4.963	1202	1220	1248	rBV3	205561	533175	100.00%	11.304%
8	5.542	1388	1400	1423	rBV2	154612	332377	62.34%	7.047%
9	5.841	1479	1493	1513	rBV4	34012	77711	14.58%	1.648%
10	5.995	1526	1541	1566	rBV	124508	272411	51.09%	5.776%
11	6.921	1816	1829	1851	rBV2	47714	97421	18.27%	2.065%
12	7.249	1918	1931	1955	rBV	210384	390819	73.30%	8.286%
13	7.561	2015	2028	2043	rBV3	29405	59328	11.13%	1.258%
14	7.911	2122	2137	2158	rBV	217896	380447	71.35%	8.066%
15	8.037	2166	2176	2211	rBV2	188925	446166	83.68%	9.459%
16	8.371	2271	2280	2293	rVB4	3861	7155	1.34%	0.152%
17	8.792	2397	2411	2435	rBV	243990	428363	80.34%	9.082%
18	10.159	2826	2836	2855	rBV2	82231	133593	25.06%	2.832%
19	11.191	3147	3157	3180	rBV	231316	367889	69.00%	7.800%
20	11.567	3262	3274	3290	rBV	209368	334500	62.74%	7.092%




Sum of corrected areas: 4716654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031369.D
Acq On : 06 Jun 2023 12:48
Operator : SY/MD
Sample : 03000-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

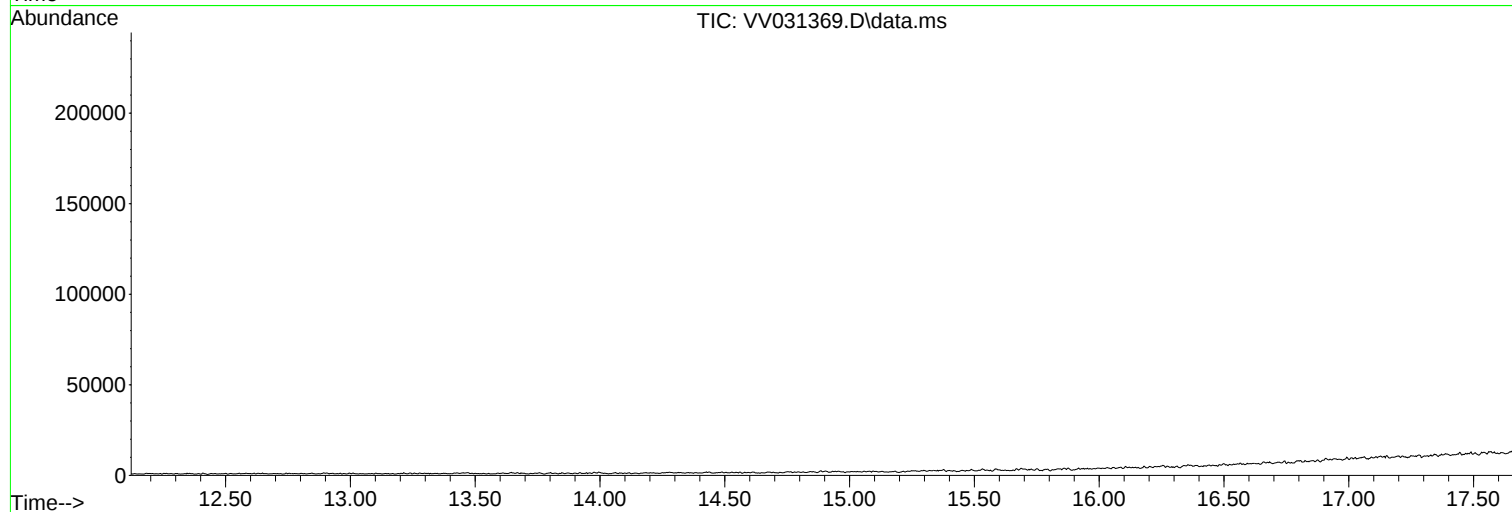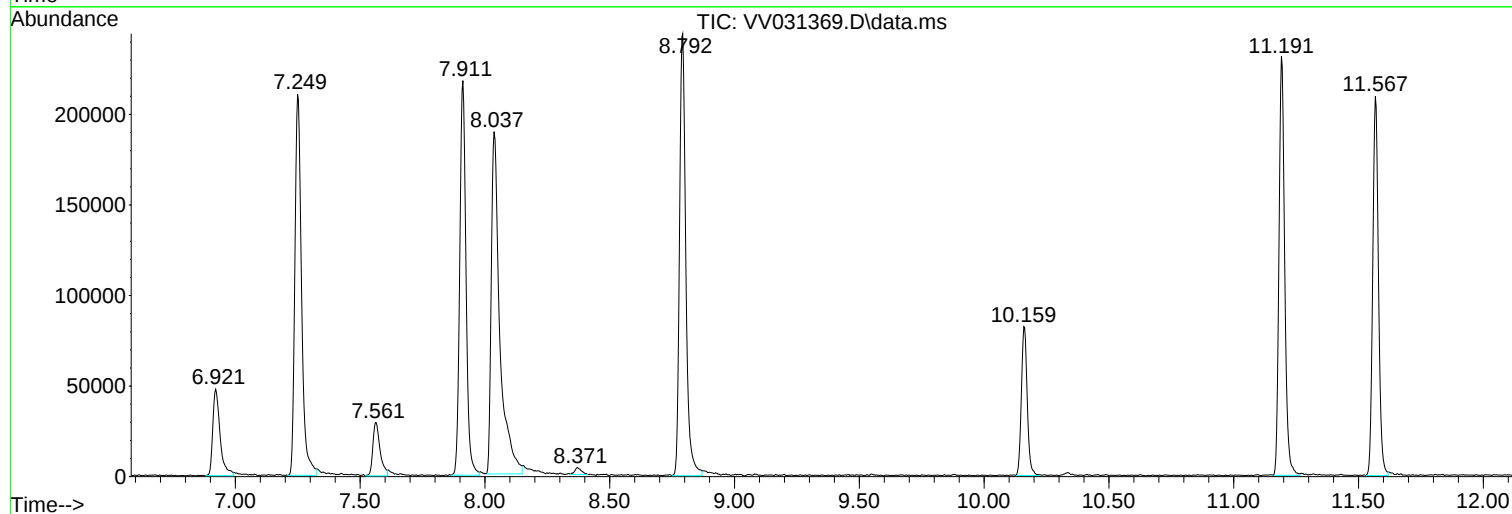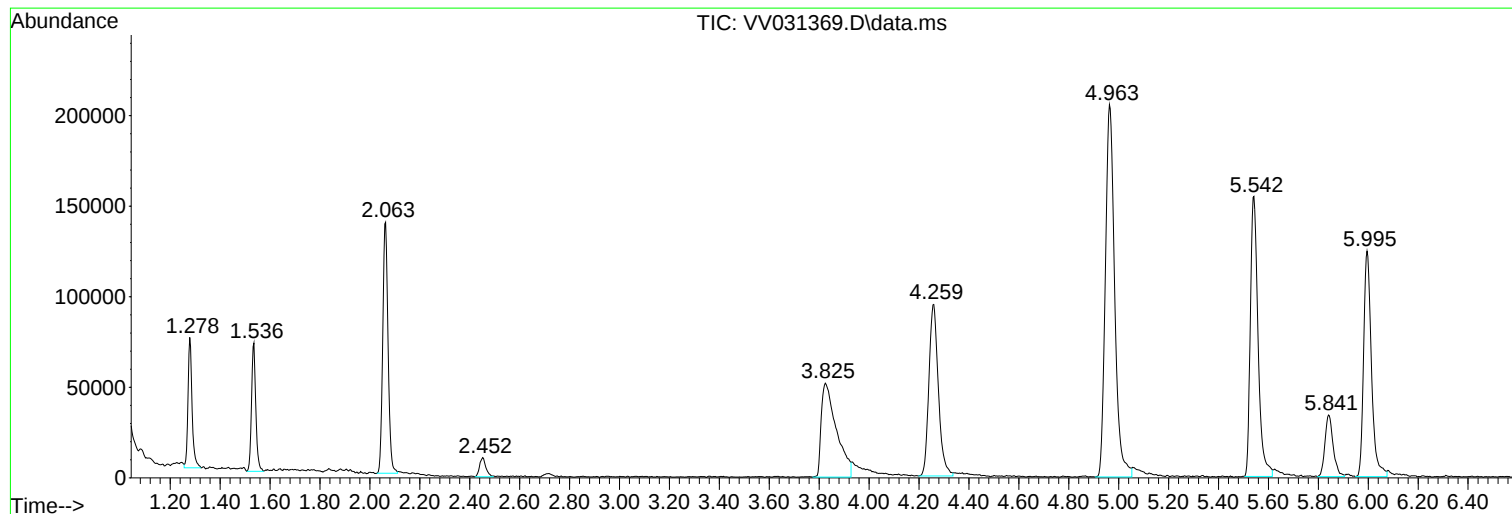

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031369.D
Acq On : 06 Jun 2023 12:48
Operator : SY/MD
Sample : 03000-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031369.D
Acq On : 06 Jun 2023 12:48
Operator : SY/MD
Sample : 03000-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------