

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031370.D
 Acq On : 06 Jun 2023 13:13
 Operator : SY/MD
 Sample : 03000-03DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C26DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	84	rVB	75992	79799	8.31%	1.435%
2	1.532	146	153	167	rVB	73031	86025	8.96%	1.546%
3	2.060	307	317	333	rBV	152227	223612	23.29%	4.020%
4	2.452	429	439	451	rVB3	8373	14105	1.47%	0.254%
5	3.828	852	867	910	rBV2	53803	248306	25.86%	4.464%
6	4.256	984	1000	1022	rBV	100433	260071	27.09%	4.675%
7	4.963	1204	1220	1246	rBV2	221190	571940	59.58%	10.282%
8	5.542	1388	1400	1420	rBV2	147431	311709	32.47%	5.604%
9	5.841	1480	1493	1526	rBV3	82424	179532	18.70%	3.227%
10	5.995	1526	1541	1577	rVV	133910	290274	30.24%	5.218%
11	6.921	1819	1829	1852	rBV	52467	104731	10.91%	1.883%
12	7.249	1920	1931	1965	rBV	230122	429264	44.71%	7.717%
13	7.561	2019	2028	2051	rBV	32929	65203	6.79%	1.172%
14	7.908	2122	2136	2165	rBV	550189	960016	100.00%	17.258%
15	8.037	2165	2176	2221	rVV2	202884	494900	51.55%	8.897%
16	8.789	2399	2410	2438	rBV	227303	401683	41.84%	7.221%
17	10.159	2822	2836	2852	rBV2	88299	145133	15.12%	2.609%
18	11.191	3142	3157	3179	rBV	213299	345188	35.96%	6.206%
19	11.567	3262	3274	3291	rBV	220633	351094	36.57%	6.312%




Sum of corrected areas: 5562585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031370.D
Acq On : 06 Jun 2023 13:13
Operator : SY/MD
Sample : 03000-03DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

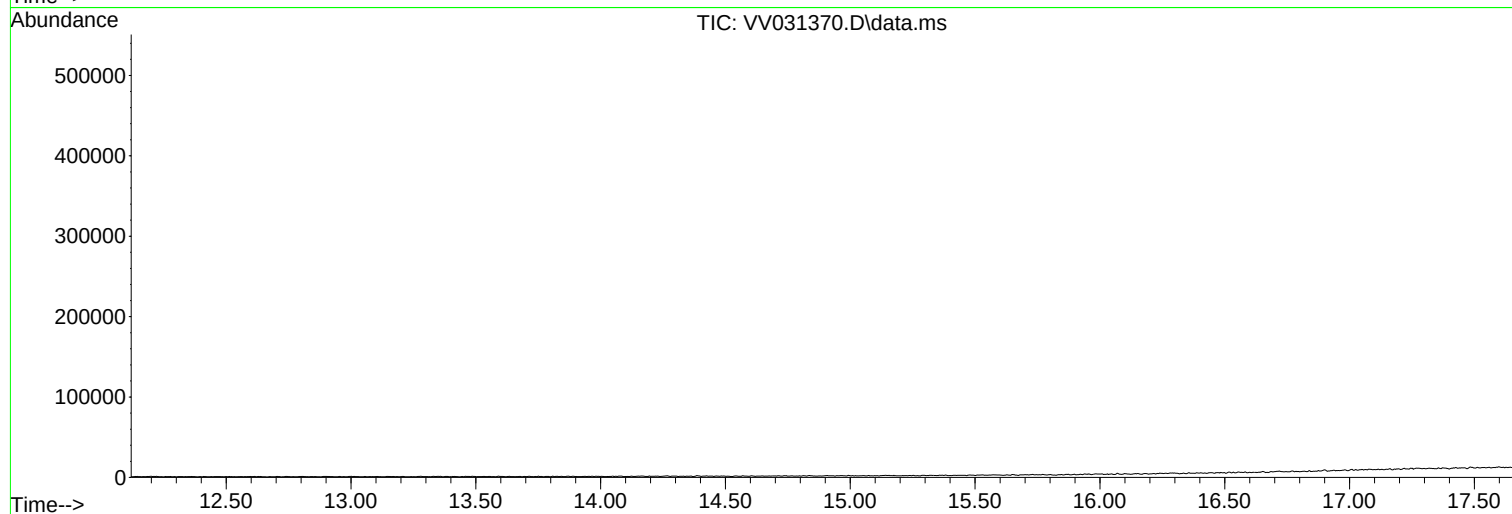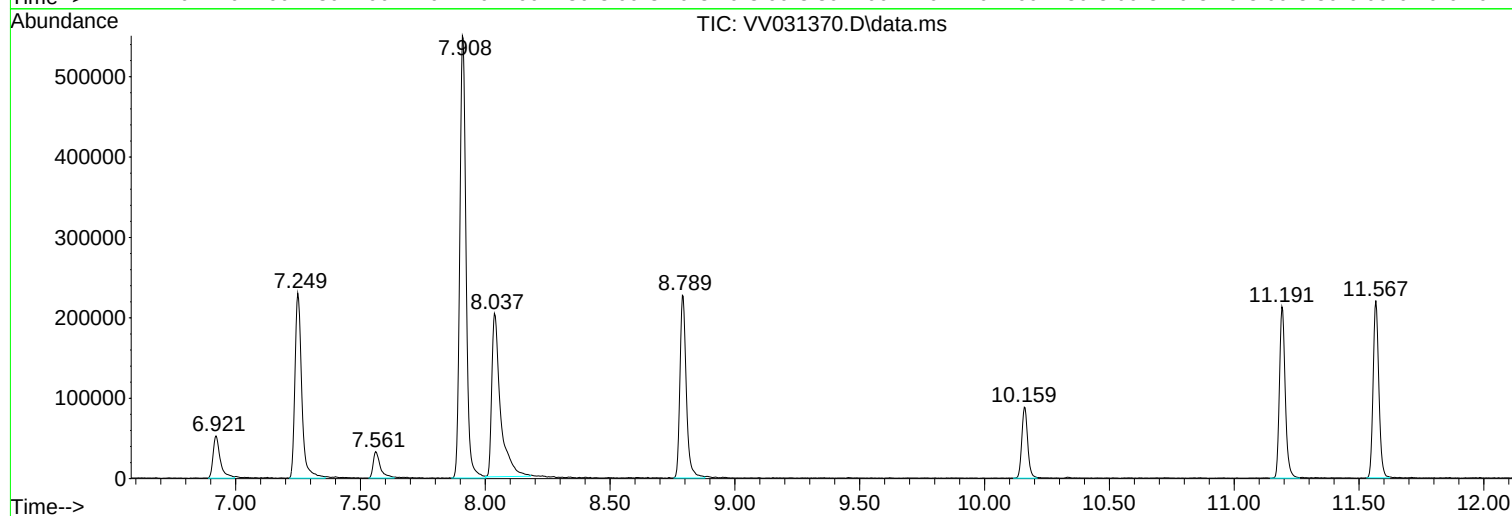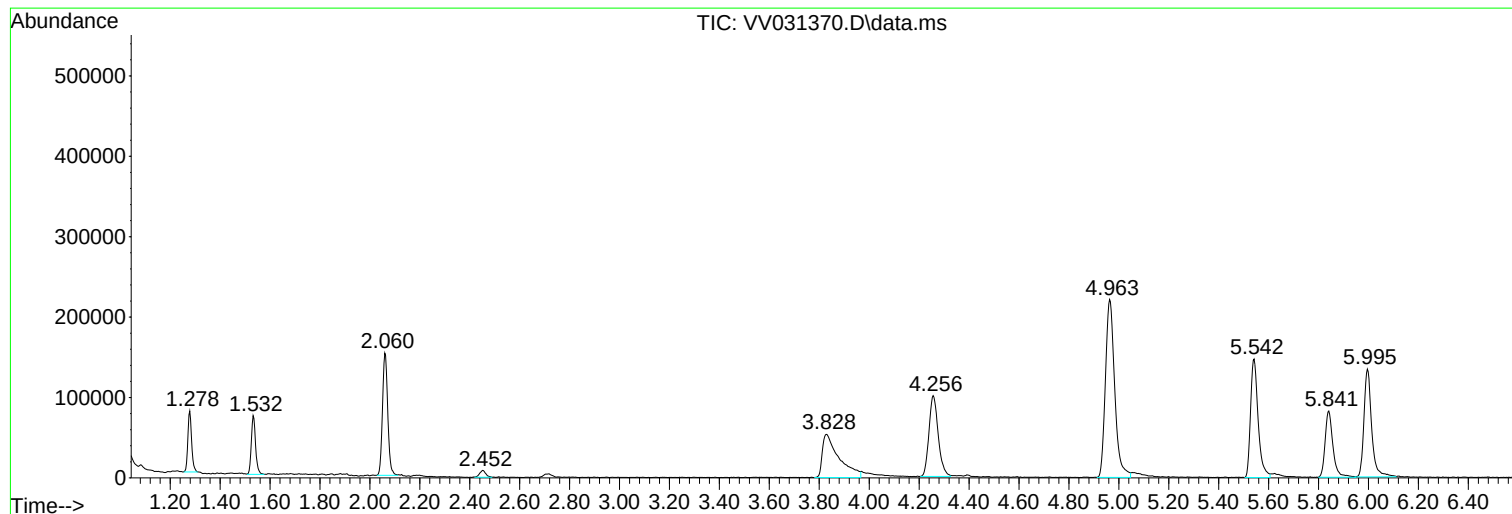

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031370.D
Acq On : 06 Jun 2023 13:13
Operator : SY/MD
Sample : 03000-03DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031370.D
Acq On : 06 Jun 2023 13:13
Operator : SY/MD
Sample : 03000-03DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------