

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031371.D
 Acq On : 06 Jun 2023 13:34
 Operator : SY/MD
 Sample : 03000-04DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C28DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	83	rBV	68813	72461	9.82%	1.443%
2	1.532	144	153	166	rVB	66460	80213	10.87%	1.597%
3	2.060	303	317	333	rBV	140683	210421	28.53%	4.189%
4	2.452	424	439	450	rBV2	13481	24740	3.35%	0.493%
5	2.712	509	520	534	rBV6	5533	12424	1.68%	0.247%
6	3.828	855	867	905	rBV4	60902	263151	35.68%	5.239%
7	4.259	983	1001	1030	rBV2	92367	244186	33.11%	4.861%
8	4.966	1203	1221	1247	rBV3	204933	531183	72.01%	10.575%
9	5.542	1388	1400	1422	rBV	149441	313125	42.45%	6.234%
10	5.844	1480	1494	1508	rBV3	38683	83773	11.36%	1.668%
11	5.995	1527	1541	1563	rBV2	123007	264809	35.90%	5.272%
12	6.924	1817	1830	1849	rBV	46393	95774	12.98%	1.907%
13	7.249	1920	1931	1955	rBV	208245	384219	52.09%	7.649%
14	7.564	2015	2029	2050	rBV	29685	61170	8.29%	1.218%
15	7.911	2124	2137	2162	rBV	422954	737610	100.00%	14.684%
16	8.037	2167	2176	2213	rBV2	182159	442691	60.02%	8.813%
17	8.792	2399	2411	2435	rBV	232798	401010	54.37%	7.983%
18	10.162	2826	2837	2853	rBV	81863	134262	18.20%	2.673%
19	11.191	3146	3157	3178	rBV	214004	340490	46.16%	6.779%
20	11.567	3262	3274	3296	rBV	202545	325344	44.11%	6.477%




Sum of corrected areas: 5023056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031371.D
Acq On : 06 Jun 2023 13:34
Operator : SY/MD
Sample : 03000-04DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

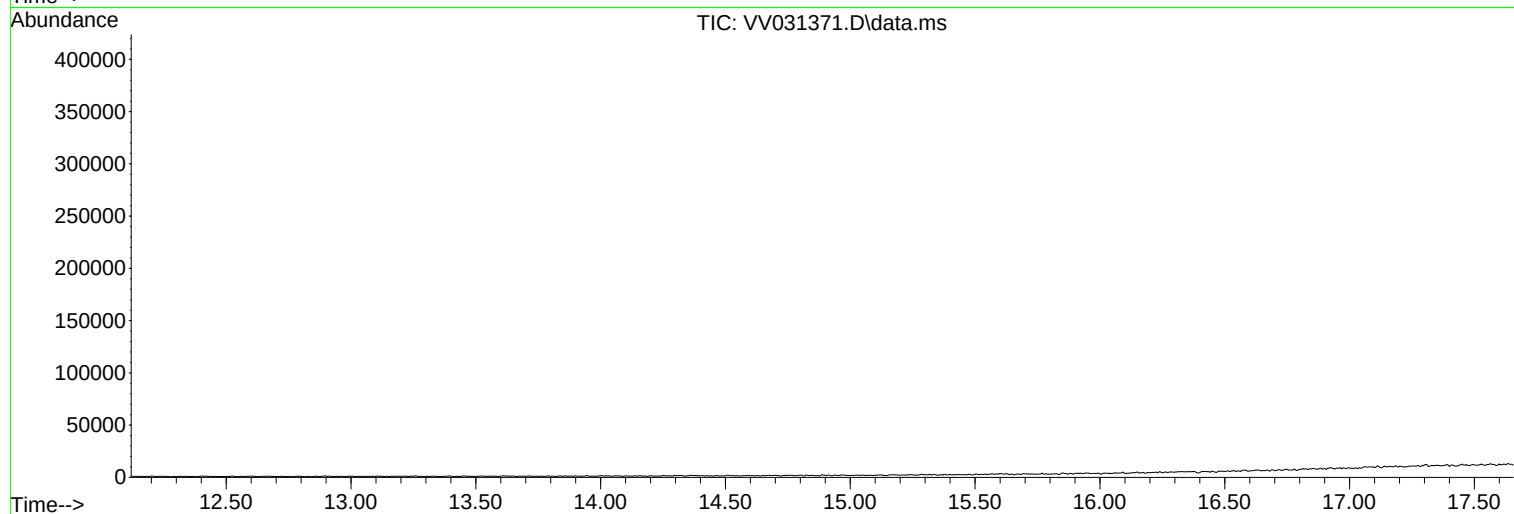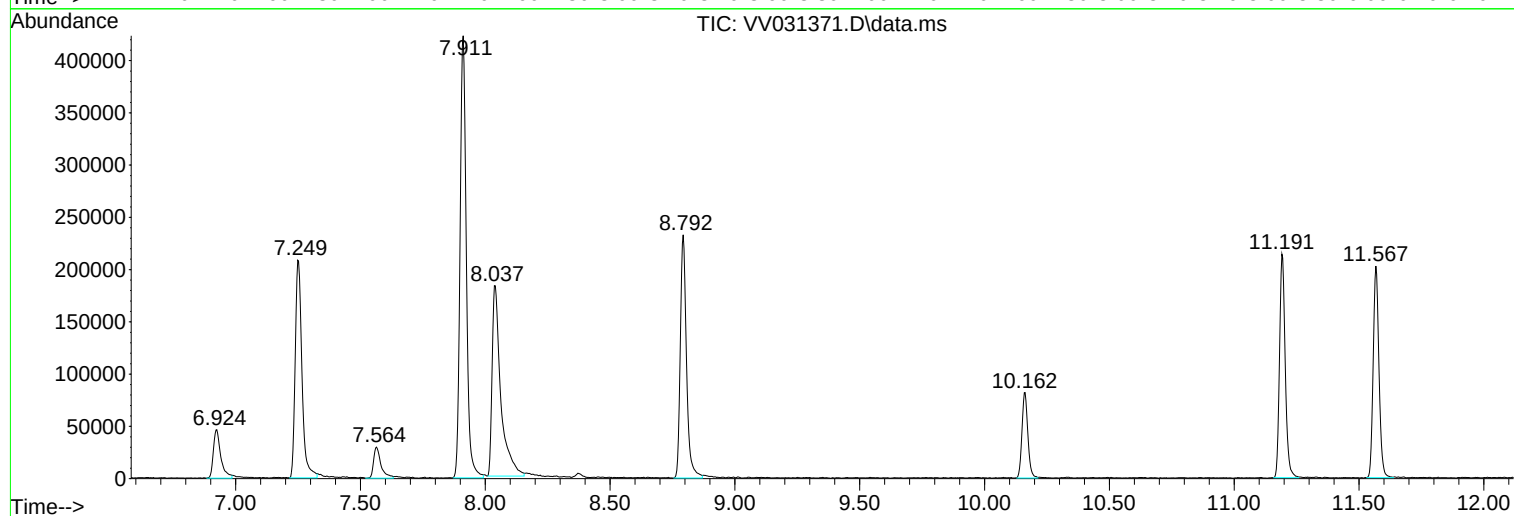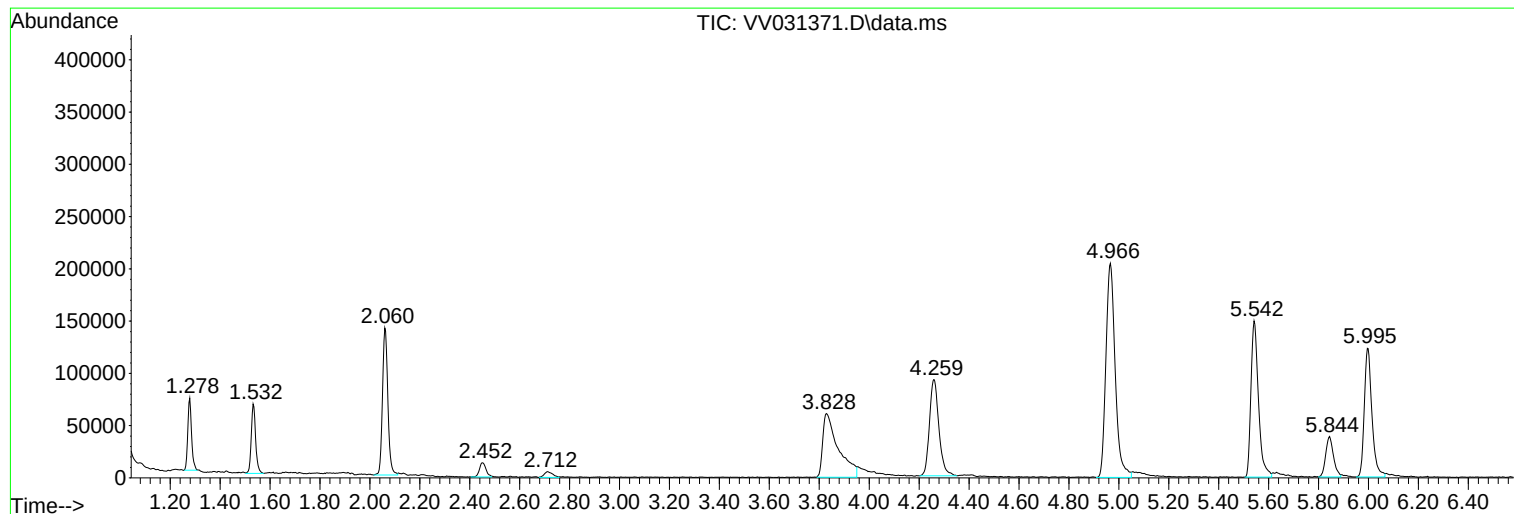

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031371.D
Acq On : 06 Jun 2023 13:34
Operator : SY/MD
Sample : 03000-04DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031371.D
Acq On : 06 Jun 2023 13:34
Operator : SY/MD
Sample : 03000-04DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------