

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031373.D
 Acq On : 06 Jun 2023 14:22
 Operator : SY/MD
 Sample : 02990-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	41765	45599	3.01%	0.904%
2	1.532	146	153	163	rVB	43208	50389	3.33%	0.999%
3	2.063	306	318	330	rBV	81536	122293	8.08%	2.424%
4	2.709	508	519	536	rBV3	19949	43261	2.86%	0.858%
5	3.818	845	864	895	rBV4	118940	416965	27.55%	8.266%
6	4.259	984	1001	1026	rBV	59115	154406	10.20%	3.061%
7	4.963	1205	1220	1244	rBV3	126219	340313	22.49%	6.747%
8	5.542	1382	1400	1420	rBV	82016	175343	11.59%	3.476%
9	5.838	1480	1492	1513	rBV2	220874	464123	30.67%	9.201%
10	5.995	1529	1541	1564	rBV2	78771	163518	10.81%	3.242%
11	6.924	1817	1830	1851	rBV2	31920	66181	4.37%	1.312%
12	7.252	1921	1932	1955	rBV	119501	223216	14.75%	4.425%
13	7.564	2020	2029	2048	rBV2	21088	40956	2.71%	0.812%
14	7.911	2120	2137	2165	rBV	880229	1513330	100.00%	30.001%
15	8.034	2165	2175	2211	rVV	218733	465753	30.78%	9.233%
16	8.792	2400	2411	2430	rBV	133444	227949	15.06%	4.519%
17	10.159	2826	2836	2849	rBV2	72351	117724	7.78%	2.334%
18	11.194	3148	3158	3178	rBV	122375	200265	13.23%	3.970%
19	11.567	3260	3274	3295	rBV	127680	212601	14.05%	4.215%




Sum of corrected areas: 5044185

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031373.D
Acq On : 06 Jun 2023 14:22
Operator : SY/MD
Sample : 02990-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

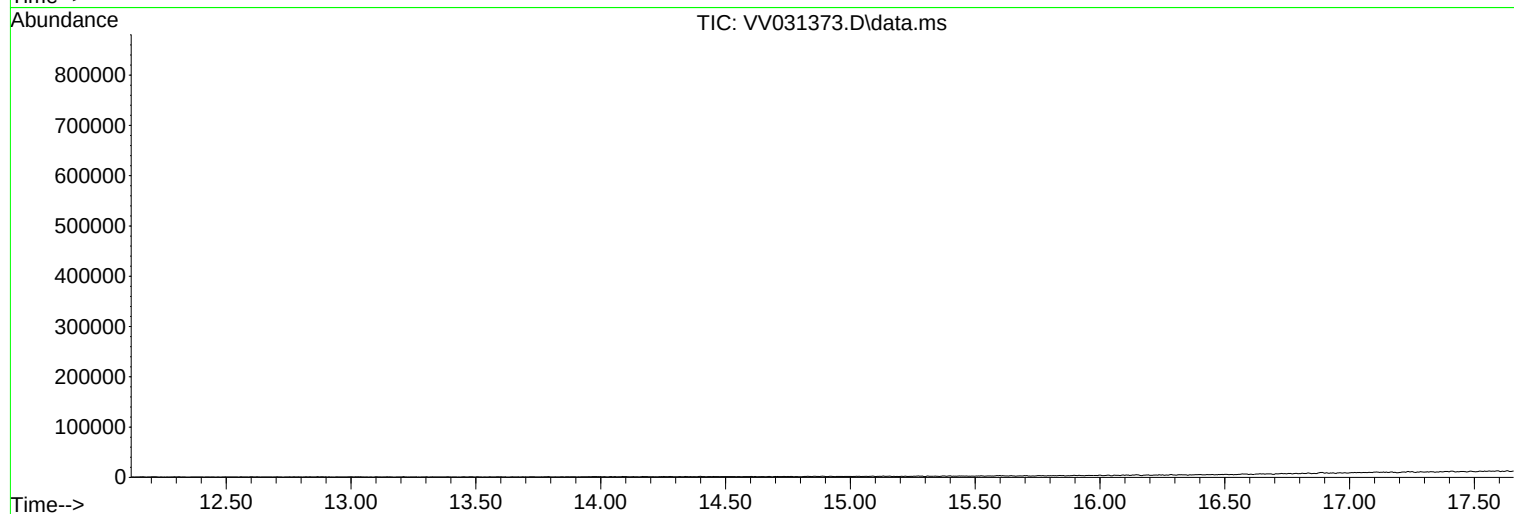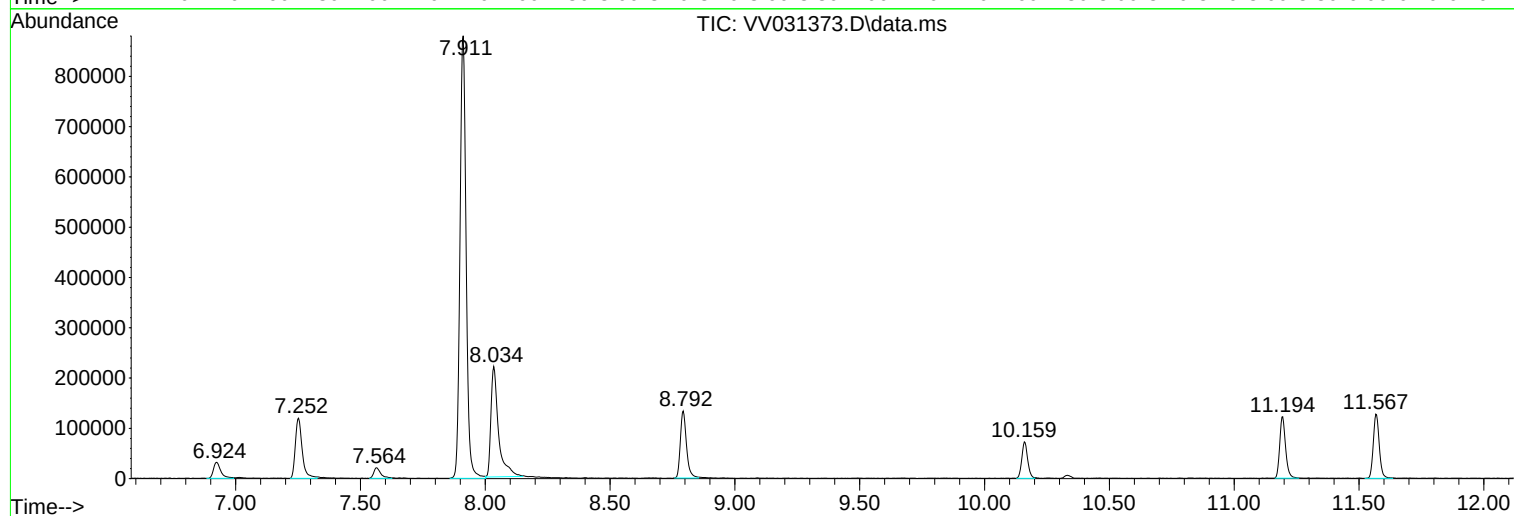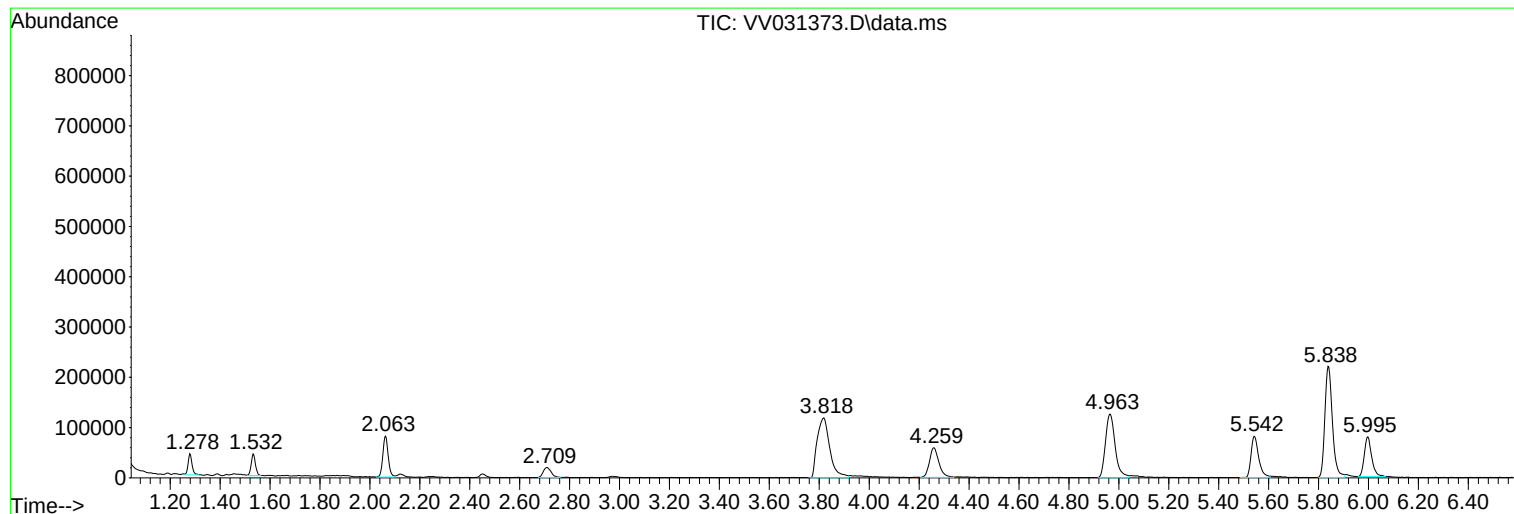

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031373.D
Acq On : 06 Jun 2023 14:22
Operator : SY/MD
Sample : 02990-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031373.D
Acq On : 06 Jun 2023 14:22
Operator : SY/MD
Sample : 02990-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------