

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031376.D
 Acq On : 06 Jun 2023 15:32
 Operator : SY/MD
 Sample : VIBLK302
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK302

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	71957	78748	14.57%	1.822%
2	1.535	145	154	167	rVB	69680	84328	15.61%	1.951%
3	2.063	307	318	330	rBV	139535	204257	37.80%	4.726%
4	2.452	427	439	452	rBV2	21494	36734	6.80%	0.850%
5	3.818	849	864	898	rBV3	54659	213511	39.51%	4.940%
6	4.256	983	1000	1029	rBV	98586	256962	47.55%	5.945%
7	4.963	1203	1220	1248	rBV3	206726	540371	100.00%	12.503%
8	5.542	1388	1400	1426	rBV	148446	315640	58.41%	7.303%
9	5.837	1481	1492	1505	rBV10	6694	14556	2.69%	0.337%
10	5.995	1527	1541	1569	rBV	131408	282383	52.26%	6.534%
11	6.921	1818	1829	1847	rBV	49868	98496	18.23%	2.279%
12	7.252	1919	1932	1962	rBV	220882	409652	75.81%	9.478%
13	7.564	2019	2029	2049	rBV	31480	62227	11.52%	1.440%
14	7.915	2122	2138	2148	rVB8	5796	11498	2.13%	0.266%
15	8.037	2163	2176	2216	rBV2	200586	468565	86.71%	10.841%
16	8.374	2273	2281	2293	rVB3	4678	8121	1.50%	0.188%
17	8.792	2399	2411	2442	rBV	235312	410383	75.94%	9.495%
18	10.159	2826	2836	2851	rBV	81923	134377	24.87%	3.109%
19	11.194	3147	3158	3182	rBV	215504	347509	64.31%	8.040%
20	11.567	3260	3274	3301	rBV	211880	343750	63.61%	7.953%




Sum of corrected areas: 4322068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031376.D
Acq On : 06 Jun 2023 15:32
Operator : SY/MD
Sample : VIBLK302
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

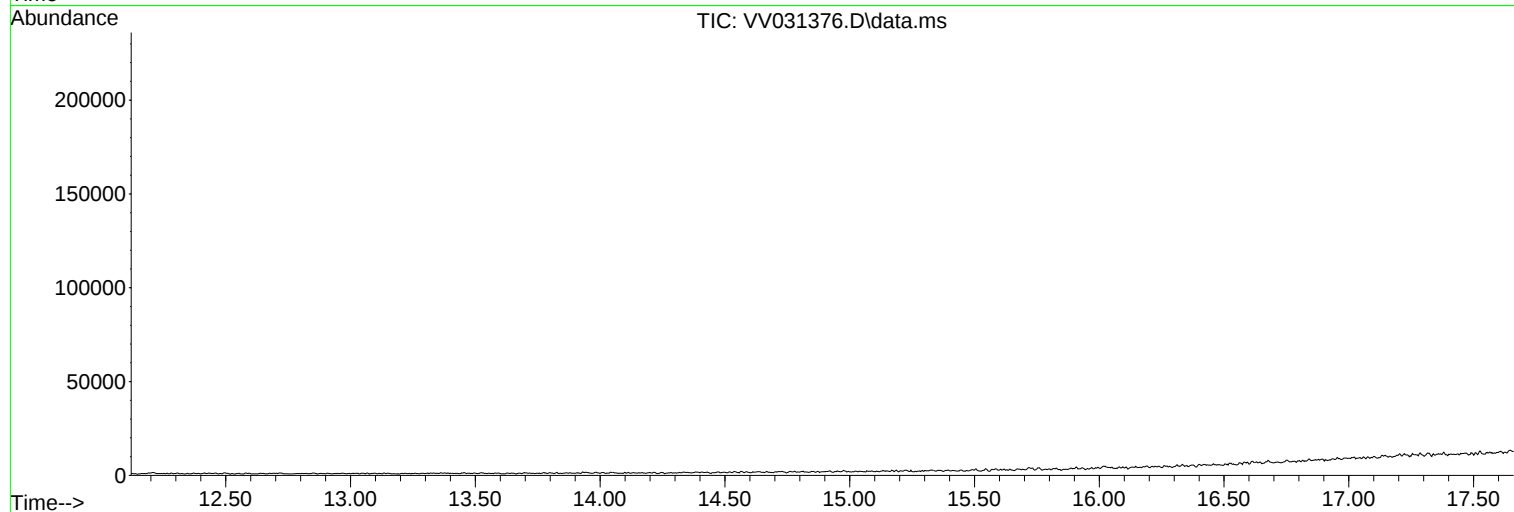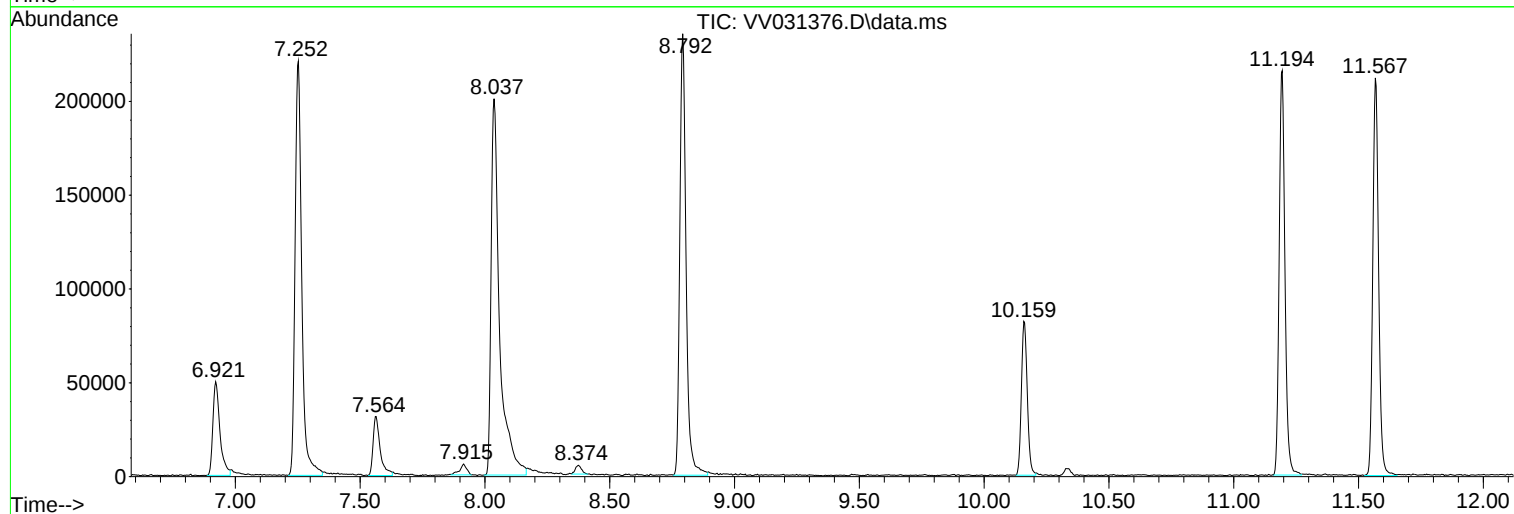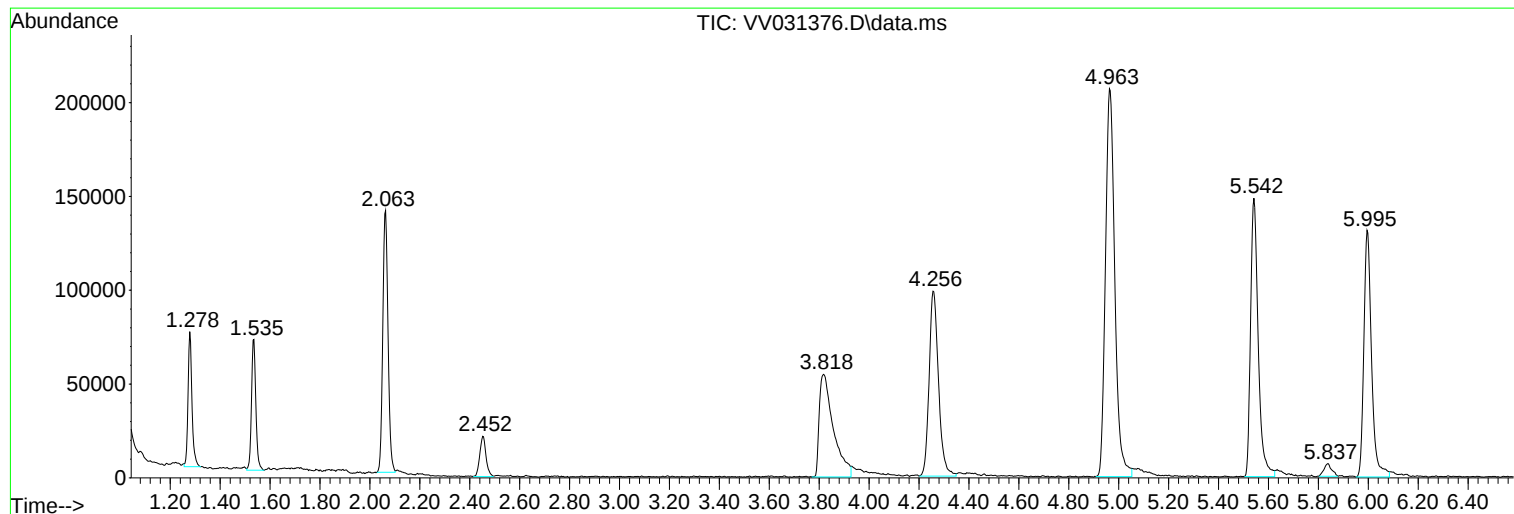

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031376.D
Acq On : 06 Jun 2023 15:32
Operator : SY/MD
Sample : VIBLK302
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031376.D
Acq On : 06 Jun 2023 15:32
Operator : SY/MD
Sample : VIBLK302
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc