

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031378.D
 Acq On : 06 Jun 2023 16:17
 Operator : SY/MD
 Sample : 02990-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C36

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	41	47	51	rBV3	6300	5969	1.15%	0.156%
2	1.278	68	74	91	rVB	49181	54726	10.55%	1.435%
3	1.388	102	108	116	rVB	17672	19793	3.81%	0.519%
4	1.535	146	154	165	rVB	52863	62091	11.97%	1.628%
5	2.063	308	318	330	rBV	94646	137944	26.58%	3.616%
6	2.130	332	339	352	rVB	7251	13963	2.69%	0.366%
7	3.805	850	860	892	rBV2	71121	237050	45.68%	6.214%
8	4.259	981	1001	1027	rBV	81574	210712	40.61%	5.524%
9	4.966	1202	1221	1247	rBV2	166902	445604	85.88%	11.681%
10	5.542	1388	1400	1422	rBV	122570	264766	51.03%	6.941%
11	5.838	1482	1492	1510	rVB9	8181	18515	3.57%	0.485%
12	5.995	1529	1541	1560	rBV	108739	231512	44.62%	6.069%
13	6.924	1819	1830	1848	rBV	43409	86285	16.63%	2.262%
14	7.252	1921	1932	1953	rBV	164358	304069	58.60%	7.971%
15	7.561	2016	2028	2049	rBV	27773	54605	10.52%	1.431%
16	7.915	2122	2138	2151	rBV6	10356	20483	3.95%	0.537%
17	8.034	2166	2175	2218	rBV2	229028	518894	100.00%	13.603%
18	8.792	2393	2411	2428	rBV	208996	358275	69.05%	9.392%
19	10.162	2825	2837	2850	rBV	84924	139412	26.87%	3.655%
20	10.333	2881	2890	2903	rVB2	8539	13212	2.55%	0.346%
21	11.191	3147	3157	3180	rBV	195971	317830	61.25%	8.332%
22	11.567	3262	3274	3289	rBV	179774	293524	56.57%	7.695%
23	12.304	3495	3503	3512	rBV7	3427	5421	1.04%	0.142%




Sum of corrected areas: 3814655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031378.D
Acq On : 06 Jun 2023 16:17
Operator : SY/MD
Sample : 02990-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

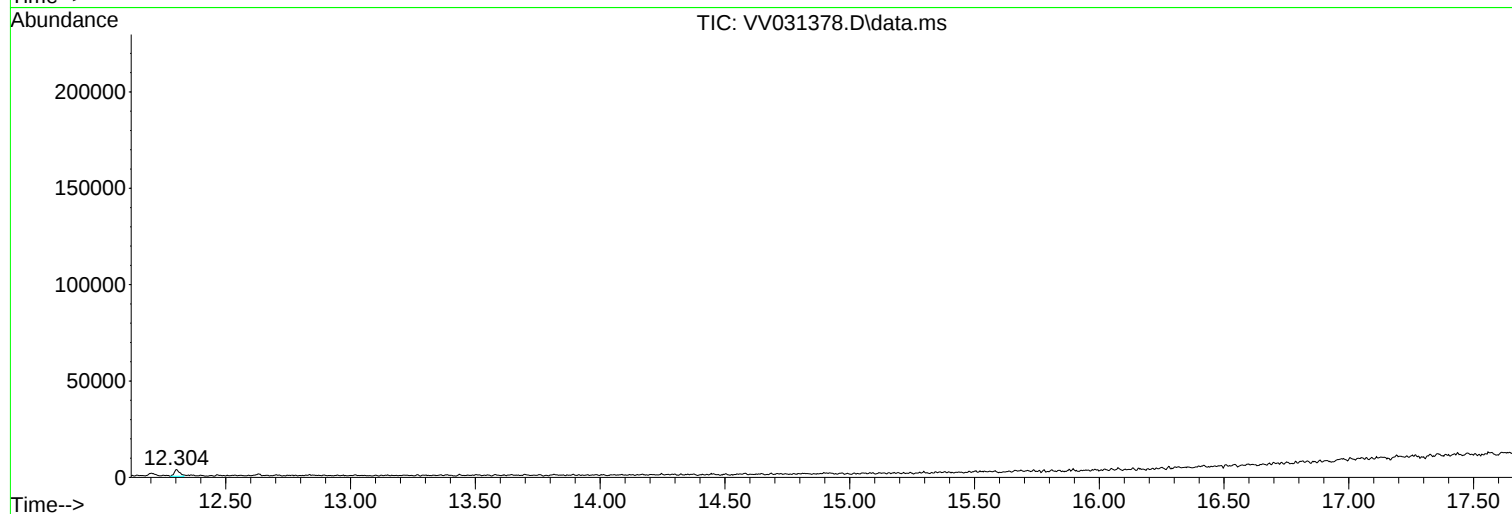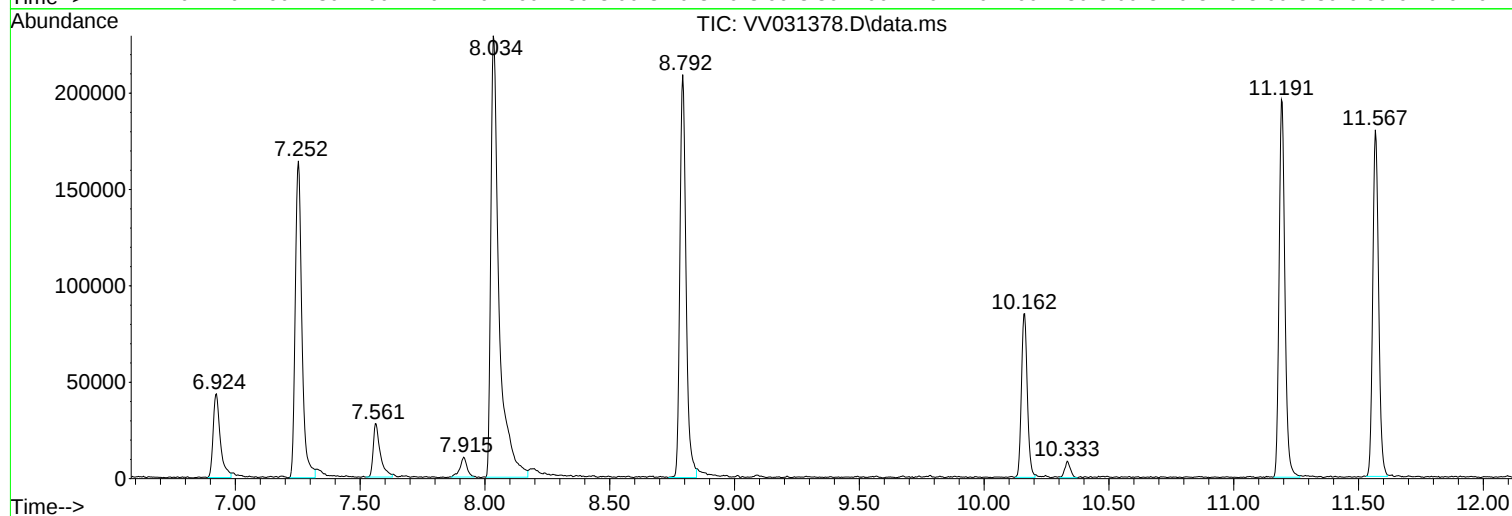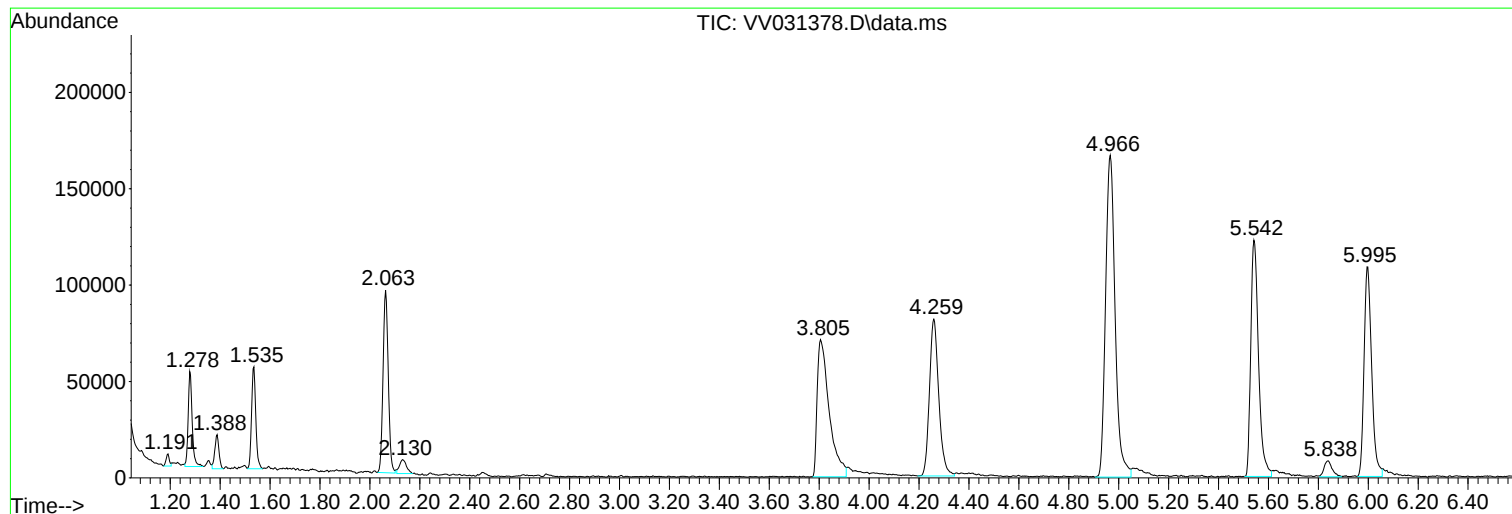

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031378.D
Acq On : 06 Jun 2023 16:17
Operator : SY/MD
Sample : 02990-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031378.D
Acq On : 06 Jun 2023 16:17
Operator : SY/MD
Sample : 02990-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------